

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049919.D
 Acq On : 20 Aug 2021 21:30
 Operator : CG/JU
 Sample : M3398-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-04-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.067	3	5	22	rVB	109521	198979	8.35%	0.628%
2	5.052	338	343	350	rBV	34986	58066	2.44%	0.183%
3	5.534	419	425	436	rBV	524222	861808	36.16%	2.718%
4	7.149	692	700	709	rBV2	567809	990384	41.55%	3.123%
5	7.978	835	841	849	rBV	134440	227411	9.54%	0.717%
6	9.153	1031	1041	1054	rBV	350732	649274	27.24%	2.048%
7	10.562	1274	1281	1289	rBV	27787	52631	2.21%	0.166%
8	10.797	1315	1321	1327	rBV	180058	319982	13.42%	1.009%
9	13.253	1732	1739	1746	rBV	955612	1440151	60.42%	4.542%
10	13.952	1851	1858	1864	rBV3	20865	40536	1.70%	0.128%
11	14.363	1922	1928	1941	rBV	67375	162032	6.80%	0.511%
12	14.633	1964	1974	1982	rBV	271346	448555	18.82%	1.415%
13	15.033	2037	2042	2048	rBV	38193	61226	2.57%	0.193%
14	15.103	2050	2054	2059	rBV2	17327	25809	1.08%	0.081%
15	15.244	2071	2078	2084	rBV5	17595	37100	1.56%	0.117%
16	15.426	2101	2109	2112	rBV7	12880	27756	1.16%	0.088%
17	15.685	2148	2153	2159	rBV2	33656	68459	2.87%	0.216%
18	15.973	2197	2202	2209	rVB4	22849	45685	1.92%	0.144%
19	16.131	2218	2229	2238	rBV	751135	1169981	49.09%	3.690%
20	16.331	2255	2263	2265	rBV2	27935	45497	1.91%	0.143%
21	16.360	2265	2268	2276	rVB7	30029	44269	1.86%	0.140%
22	16.689	2318	2324	2329	rBV6	21578	40682	1.71%	0.128%
23	16.919	2357	2363	2366	rBV8	16713	30104	1.26%	0.095%
24	17.042	2379	2384	2391	rVB	51918	81609	3.42%	0.257%
25	17.124	2393	2398	2404	rVV3	20529	40310	1.69%	0.127%
26	17.206	2404	2412	2419	rVB	45753	80679	3.38%	0.254%
27	17.388	2437	2443	2446	rBV	295348	467859	19.63%	1.476%
28	17.430	2446	2450	2458	rVB	684781	1037931	43.55%	3.273%
29	17.524	2458	2466	2470	rBV	83704	137517	5.77%	0.434%
30	17.582	2470	2476	2482	rVB9	21937	46346	1.94%	0.146%
31	17.794	2508	2512	2518	rBV3	28012	54559	2.29%	0.172%
32	17.905	2527	2531	2536	rVB	31729	41544	1.74%	0.131%
33	17.970	2538	2542	2549	rVB4	39663	68962	2.89%	0.217%
34	18.111	2563	2566	2572	rVB2	16822	31138	1.31%	0.098%
35	18.187	2574	2579	2582	rBV3	17874	30750	1.29%	0.097%
36	18.264	2587	2592	2597	rVV	175610	272705	11.44%	0.860%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049919.D
 Acq On : 20 Aug 2021 21:30
 Operator : CG/JU
 Sample : M3398-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-04-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.317	2597	2601	2606	rVB	206919	299098	12.55%	0.943%
38	18.393	2606	2614	2619	rBV2	43217	80456	3.38%	0.254%
39	18.458	2619	2625	2629	rVV4	190720	370930	15.56%	1.170%
40	18.499	2629	2632	2636	rVB	113173	155512	6.52%	0.490%

41	18.569	2640	2644	2648	rBV7	21246	38568	1.62%	0.122%
42	18.763	2672	2677	2681	rBV	107642	152620	6.40%	0.481%
43	18.810	2681	2685	2695	rVB2	94790	154768	6.49%	0.488%
44	19.010	2711	2719	2723	rBV3	53198	101613	4.26%	0.320%
45	19.057	2723	2727	2731	rBV	72950	88868	3.73%	0.280%

46	19.098	2731	2734	2740	rVB2	54781	70045	2.94%	0.221%
47	19.180	2743	2748	2753	rBV	173316	301786	12.66%	0.952%
48	19.233	2753	2757	2761	rBV3	53109	83835	3.52%	0.264%
49	19.327	2767	2773	2784	rBV2	135554	286892	12.04%	0.905%
50	19.450	2787	2794	2799	rBV	1662740	2354535	98.78%	7.426%

51	19.503	2799	2803	2806	rBV2	38599	52488	2.20%	0.166%
52	19.538	2806	2809	2814	rVB3	49321	67110	2.82%	0.212%
53	19.597	2814	2819	2823	rBV	78856	119058	5.00%	0.375%
54	19.685	2831	2834	2839	rVV	49339	67837	2.85%	0.214%
55	19.773	2844	2849	2850	rBV	175969	203597	8.54%	0.642%

56	19.815	2850	2856	2862	rVB	1560587	2383519	100.00%	7.517%
57	19.879	2862	2867	2870	rBV2	124742	198191	8.32%	0.625%
58	20.003	2882	2888	2892	rVB	1351105	1761245	73.89%	5.555%
59	20.044	2892	2895	2902	rVB3	66345	109626	4.60%	0.346%
60	20.132	2903	2910	2911	rBV4	141493	256979	10.78%	0.810%

61	20.267	2927	2933	2934	rBV3	116827	186822	7.84%	0.589%
62	20.296	2935	2938	2943	rVB	204423	304086	12.76%	0.959%
63	20.402	2951	2956	2960	rBV2	96996	175701	7.37%	0.554%
64	20.461	2960	2966	2970	rVB2	234611	355747	14.93%	1.122%
65	20.596	2985	2989	2993	rBV	176993	232654	9.76%	0.734%

66	20.643	2993	2997	3001	rVV	130932	174884	7.34%	0.552%
67	20.854	3029	3033	3036	rBV3	101882	144323	6.06%	0.455%
68	21.060	3063	3068	3074	rVB	214267	330736	13.88%	1.043%
69	21.154	3082	3084	3090	rVB	53054	67693	2.84%	0.213%
70	21.242	3091	3099	3103	rVV2	183872	433070	18.17%	1.366%

71	21.289	3103	3107	3111	rVV	162581	292336	12.26%	0.922%
72	21.336	3111	3115	3120	rVV2	159802	322635	13.54%	1.018%
73	21.395	3120	3125	3132	rVB2	183902	363387	15.25%	1.146%
74	21.653	3162	3169	3175	rBV2	884042	2076485	87.12%	6.549%
75	21.712	3175	3179	3190	rVB	741312	1349634	56.62%	4.256%

76	21.929	3212	3216	3223	rBV3	127518	233669	9.80%	0.737%
----	--------	------	------	------	------	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049919.D
 Acq On : 20 Aug 2021 21:30
 Operator : CG/JU
 Sample : M3398-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-04-0002

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	22.070	3236	3240	3247	rBV4	78971	186088	7.81%	0.587%
78	22.399	3292	3296	3301	rVB	160901	261734	10.98%	0.825%
79	22.464	3305	3307	3317	rVB2	103738	194705	8.17%	0.614%
80	22.664	3339	3341	3347	rVB3	54257	78147	3.28%	0.246%
81	23.886	3539	3549	3555	rBV2	530790	1787121	74.98%	5.636%
82	24.138	3587	3592	3602	rVB	111366	247975	10.40%	0.782%
83	24.608	3665	3672	3684	rVB	341467	999118	41.92%	3.151%
84	24.755	3688	3697	3710	rVB	499496	1407044	59.03%	4.438%
85	24.902	3716	3722	3729	rBV	119059	304731	12.78%	0.961%




Sum of corrected areas: 31707987

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049919.D
Acq On : 20 Aug 2021 21:30
Operator : CG/JU
Sample : M3398-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-04-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

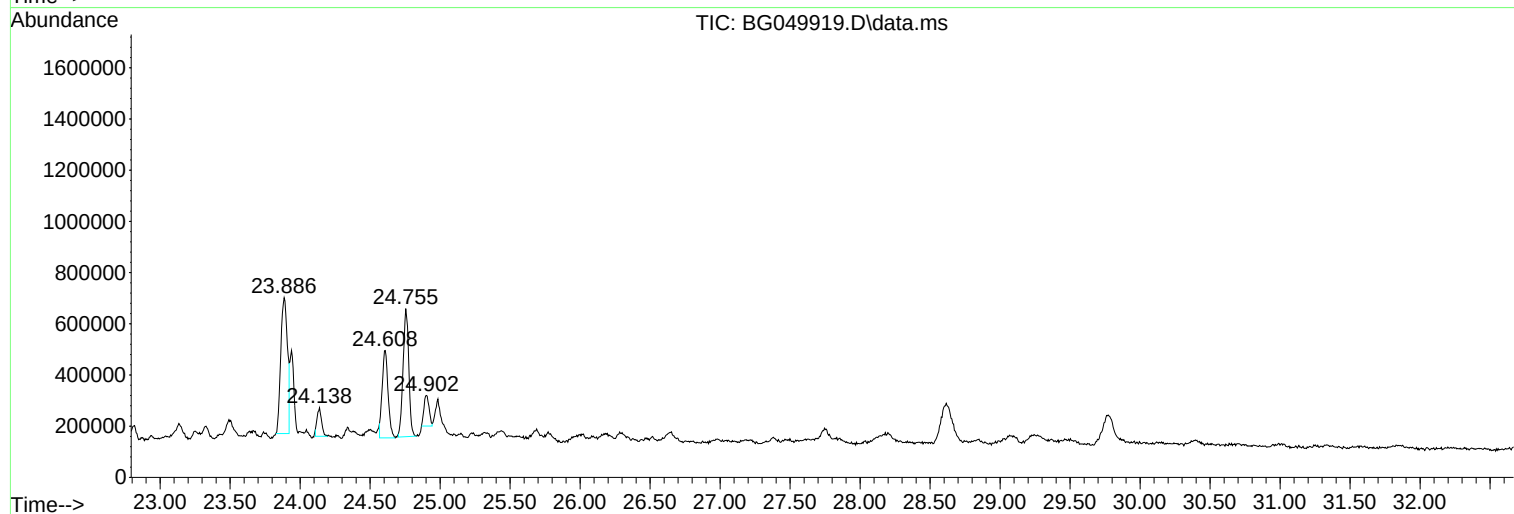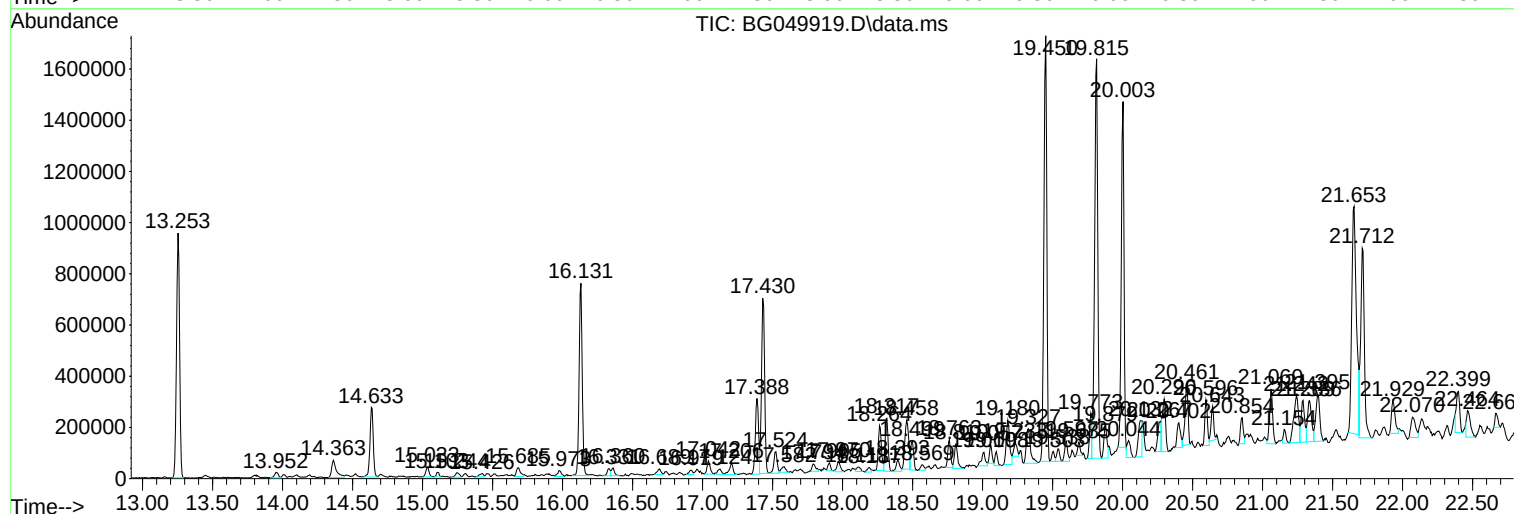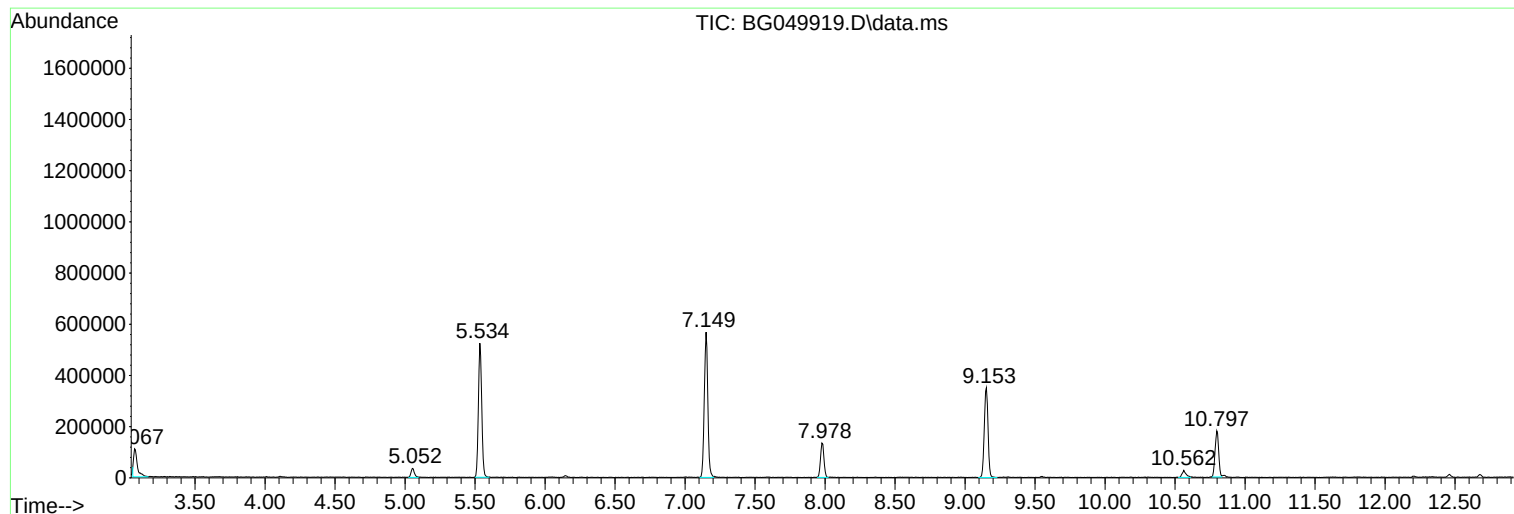

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049919.D
Acq On : 20 Aug 2021 21:30
Operator : CG/JU
Sample : M3398-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-04-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049919.D
Acq On : 20 Aug 2021 21:30
Operator : CG/JU
Sample : M3398-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-04-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------