

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049920.D
 Acq On : 20 Aug 2021 22:11
 Operator : CG/JU
 Sample : M3398-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-05-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	3	5	22	rVB	101648	159454	10.22%	1.693%
2	5.055	338	343	351	rBV	35246	57418	3.68%	0.609%
3	5.537	418	425	436	rBV	490376	821928	52.70%	8.724%
4	7.152	693	700	713	rBV	517914	926714	59.42%	9.837%
5	7.980	832	841	848	rVB	137182	234284	15.02%	2.487%
6	9.155	1028	1041	1048	rBV	334496	605280	38.81%	6.425%
7	10.565	1273	1281	1297	rBV	142475	277995	17.83%	2.951%
8	10.800	1313	1321	1328	rVB	182531	326012	20.90%	3.460%
9	13.256	1732	1739	1746	rVB	864202	1350990	86.63%	14.340%
10	13.520	1778	1784	1790	rVB2	61647	100151	6.42%	1.063%
11	14.636	1966	1974	1981	rBV	268799	434061	27.83%	4.607%
12	15.030	2036	2041	2051	rBV7	10701	25771	1.65%	0.274%
13	15.594	2130	2137	2145	rBV8	17115	34765	2.23%	0.369%
14	16.075	2214	2219	2222	rBV5	12515	19854	1.27%	0.211%
15	16.134	2222	2229	2238	rVB	663709	1053503	67.55%	11.182%
16	16.328	2257	2262	2265	rBV4	12697	22204	1.42%	0.236%
17	17.391	2436	2443	2448	rBV	304532	458803	29.42%	4.870%
18	17.432	2448	2450	2458	rVB2	22879	31961	2.05%	0.339%
19	18.043	2549	2554	2558	rBV	30306	45105	2.89%	0.479%
20	18.267	2588	2592	2597	rBV5	32648	59904	3.84%	0.636%
21	18.314	2598	2600	2605	rVB5	16788	22314	1.43%	0.237%
22	19.212	2750	2753	2758	rVB2	75729	86062	5.52%	0.914%
23	19.342	2773	2775	2779	rVB	30345	33820	2.17%	0.359%
24	19.447	2788	2793	2798	rVB	95440	136789	8.77%	1.452%
25	19.806	2850	2854	2861	rVB	89769	144801	9.28%	1.537%
26	20.005	2882	2888	2893	rBV	1193141	1559524	100.00%	16.554%
27	21.662	3165	3170	3176	rVB	230146	391644	25.11%	4.157%




Sum of corrected areas: 9421111

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049920.D
Acq On : 20 Aug 2021 22:11
Operator : CG/JU
Sample : M3398-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-05-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

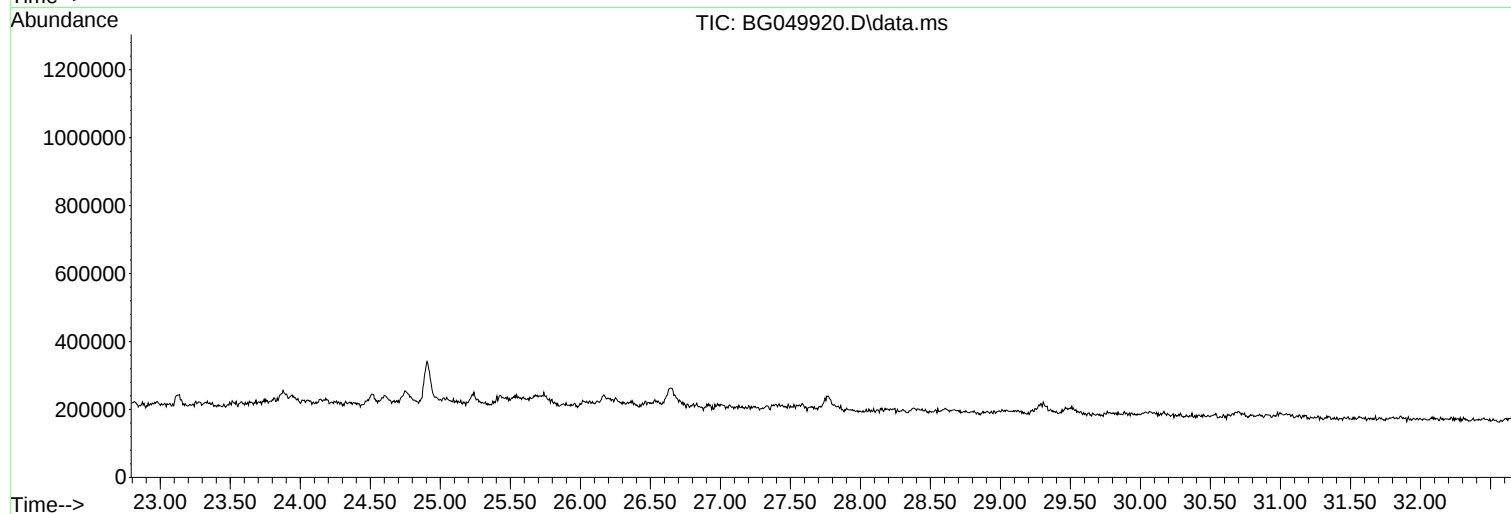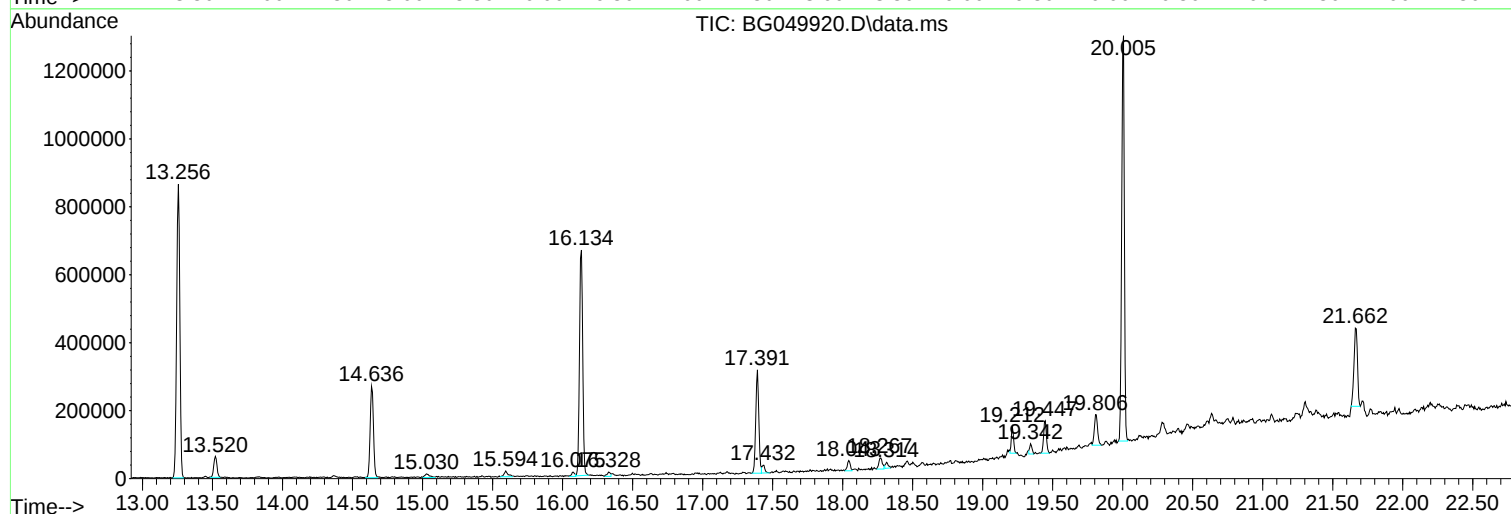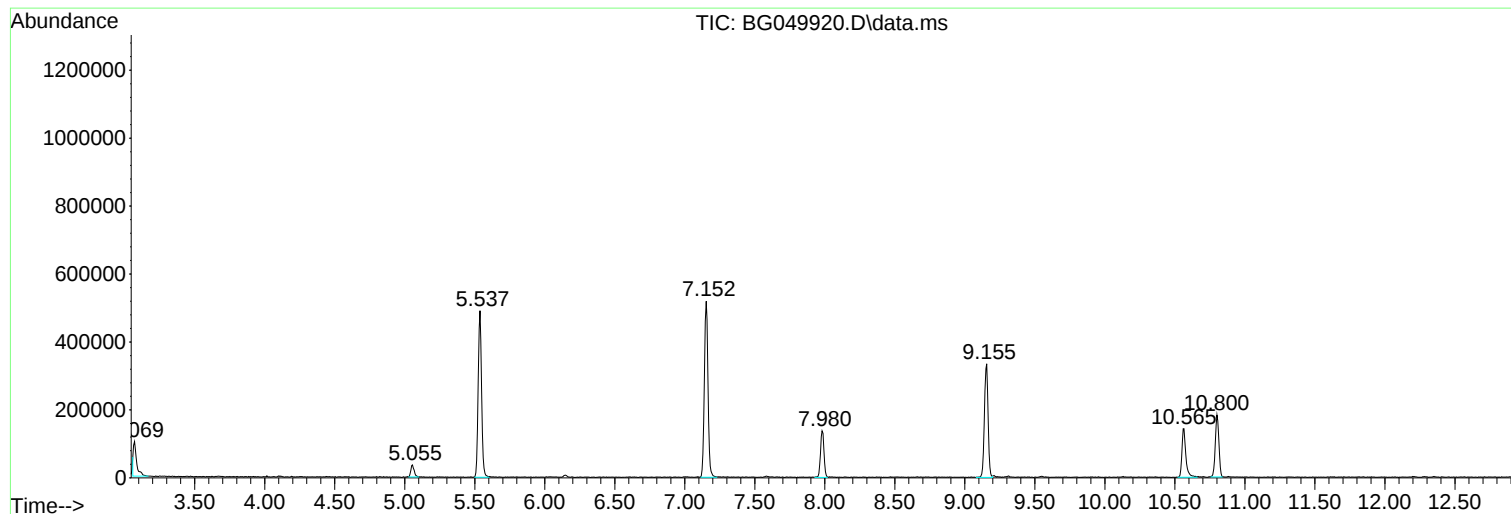

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049920.D
Acq On : 20 Aug 2021 22:11
Operator : CG/JU
Sample : M3398-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-05-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049920.D
Acq On : 20 Aug 2021 22:11
Operator : CG/JU
Sample : M3398-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-05-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------