

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049921.D
 Acq On : 20 Aug 2021 22:52
 Operator : CG/JU
 Sample : M3419-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.067	3	5	22	rVB	101911	165824	8.44%	0.710%
2	5.058	338	344	348	rBV2	11623	21733	1.11%	0.093%
3	5.540	418	426	434	rBV	461139	793258	40.40%	3.397%
4	7.155	694	701	715	rBV	519312	922494	46.98%	3.951%
5	7.984	835	842	851	rVB	149576	250778	12.77%	1.074%
6	9.153	1034	1041	1049	rBV	332203	609494	31.04%	2.610%
7	10.568	1276	1282	1290	rBV2	27470	57295	2.92%	0.245%
8	10.803	1315	1322	1328	rBV	199066	364497	18.56%	1.561%
9	10.856	1328	1331	1339	rVB	13591	21183	1.08%	0.091%
10	13.259	1732	1740	1750	rBV	903898	1404983	71.55%	6.017%
11	13.811	1829	1834	1842	rVB8	10017	24274	1.24%	0.104%
12	13.958	1855	1859	1865	rBV2	17091	28087	1.43%	0.120%
13	14.369	1923	1929	1940	rBV2	47205	106865	5.44%	0.458%
14	14.639	1965	1975	1982	rBV	309696	512276	26.09%	2.194%
15	14.704	1982	1986	1992	rVB3	18144	36396	1.85%	0.156%
16	15.039	2036	2043	2048	rVV	32926	54174	2.76%	0.232%
17	15.109	2052	2055	2065	rVB3	20502	38987	1.99%	0.167%
18	15.256	2073	2080	2085	rBV4	20107	45033	2.29%	0.193%
19	15.309	2085	2089	2094	rVB6	16639	24353	1.24%	0.104%
20	15.474	2112	2117	2120	rVB5	13969	26024	1.33%	0.111%
21	15.515	2120	2124	2130	rBV6	11307	23620	1.20%	0.101%
22	15.691	2148	2154	2161	rBV	68291	123704	6.30%	0.530%
23	15.979	2200	2203	2211	rVB3	25149	45029	2.29%	0.193%
24	16.137	2223	2230	2237	rBV	718432	1091626	55.59%	4.675%
25	16.337	2259	2264	2266	rBV2	34999	49553	2.52%	0.212%
26	16.366	2266	2269	2274	rVB5	33766	50161	2.55%	0.215%
27	16.695	2317	2325	2330	rBV4	38143	87513	4.46%	0.375%
28	16.742	2330	2333	2338	rVB3	27006	40161	2.05%	0.172%
29	16.842	2347	2350	2356	rVB3	25069	31611	1.61%	0.135%
30	16.925	2356	2364	2367	rBV6	23853	49460	2.52%	0.212%
31	17.048	2380	2385	2391	rVB3	38154	65212	3.32%	0.279%
32	17.130	2396	2399	2403	rVV6	30210	47003	2.39%	0.201%
33	17.183	2404	2408	2409	rVV4	20792	29357	1.50%	0.126%
34	17.212	2409	2413	2420	rVB	64021	103592	5.28%	0.444%
35	17.394	2438	2444	2447	rBV	314036	496203	25.27%	2.125%
36	17.436	2447	2451	2458	rVV	753723	1139134	58.01%	4.878%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049921.D
 Acq On : 20 Aug 2021 22:52
 Operator : CG/JU
 Sample : M3419-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.530	2462	2467	2472	rVV	148575	219500	11.18%	0.940%
38	17.588	2472	2477	2482	rVB3	28508	60018	3.06%	0.257%
39	17.800	2509	2513	2521	rVB	50446	88810	4.52%	0.380%
40	17.906	2529	2531	2536	rVB	29131	39093	1.99%	0.167%
41	17.976	2539	2543	2551	rVB2	47970	92569	4.71%	0.396%
42	18.047	2551	2555	2558	rBV5	22306	34598	1.76%	0.148%
43	18.117	2564	2567	2573	rVB2	23363	42417	2.16%	0.182%
44	18.270	2588	2593	2598	rBV	187733	296352	15.09%	1.269%
45	18.323	2598	2602	2608	rVB	230762	338223	17.22%	1.448%
46	18.405	2612	2616	2620	rVV	59164	91956	4.68%	0.394%
47	18.469	2621	2627	2630	rVV3	250411	479399	24.41%	2.053%
48	18.505	2630	2633	2639	rVB	142869	208222	10.60%	0.892%
49	18.669	2657	2661	2664	rBV5	26204	37495	1.91%	0.161%
50	18.763	2673	2677	2682	rBV	108927	158473	8.07%	0.679%
51	18.816	2682	2686	2691	rVB3	95886	145764	7.42%	0.624%
52	19.016	2717	2720	2725	rVB3	46236	61052	3.11%	0.261%
53	19.063	2725	2728	2732	rVV	67078	87624	4.46%	0.375%
54	19.104	2732	2735	2739	rVB2	46702	60365	3.07%	0.259%
55	19.186	2744	2749	2754	rBV	175454	317281	16.16%	1.359%
56	19.327	2769	2773	2780	rBV4	87525	205043	10.44%	0.878%
57	19.456	2788	2795	2800	rBV	1414009	1963644	100.00%	8.409%
58	19.509	2801	2804	2807	rBV3	39219	52670	2.68%	0.226%
59	19.603	2816	2820	2823	rBV	72961	100096	5.10%	0.429%
60	19.779	2846	2850	2852	rBV	172124	249589	12.71%	1.069%
61	19.821	2852	2857	2863	rVB	1234227	1879846	95.73%	8.050%
62	19.885	2864	2868	2875	rVB	93456	142532	7.26%	0.610%
63	20.009	2883	2889	2893	rVB	1215897	1588475	80.89%	6.803%
64	20.138	2906	2911	2917	rBV3	110742	249938	12.73%	1.070%
65	20.302	2936	2939	2944	rVB	240947	365701	18.62%	1.566%
66	20.408	2953	2957	2961	rBV2	168492	248304	12.65%	1.063%
67	20.467	2963	2967	2971	rVB	174364	245578	12.51%	1.052%
68	20.602	2987	2990	2994	rBV	142611	174055	8.86%	0.745%
69	20.649	2995	2998	3003	rVB	115139	155101	7.90%	0.664%
70	21.066	3066	3069	3075	rVB	121171	198640	10.12%	0.851%
71	21.295	3105	3108	3112	rVB3	114369	141602	7.21%	0.606%
72	21.659	3164	3170	3177	rBV3	679702	1693899	86.26%	7.254%
73	21.724	3177	3181	3192	rVB	583753	1054515	53.70%	4.516%
74	23.892	3544	3550	3557	rBV	268237	801426	40.81%	3.432%

Sum of corrected areas: 23350812

Instrument :

BNA_G

ClientSampleId :


SWCS-03-0002

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049921.D
Acq On : 20 Aug 2021 22:52
Operator : CG/JU
Sample : M3419-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

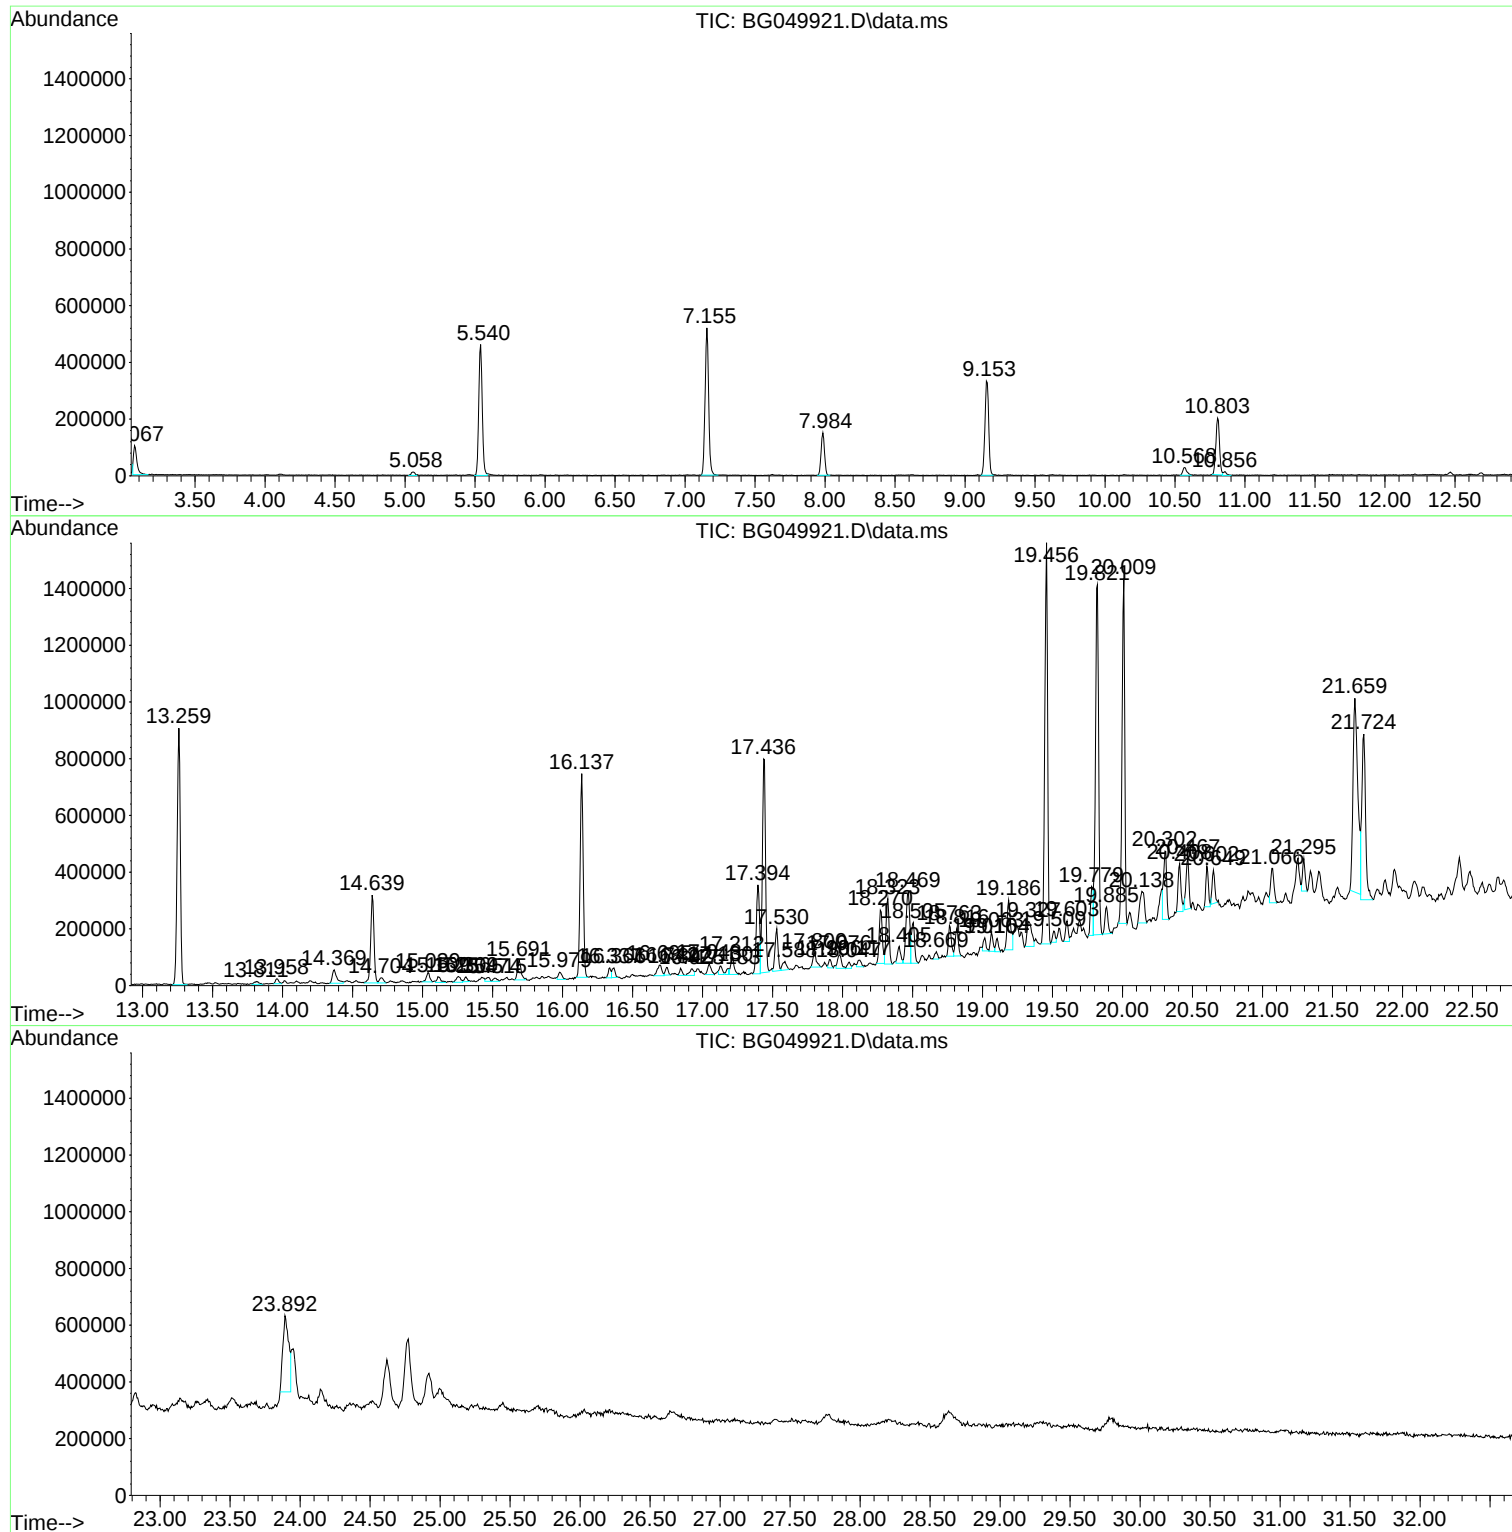

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049921.D
Acq On : 20 Aug 2021 22:52
Operator : CG/JU
Sample : M3419-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049921.D
Acq On : 20 Aug 2021 22:52
Operator : CG/JU
Sample : M3419-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------