

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049922.D
 Acq On : 20 Aug 2021 23:33
 Operator : CG/JU
 Sample : M3419-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.067	3	5	17	rVB	47175	72923	2.31%	0.261%
2	5.540	417	426	440	rBV	475838	796572	25.20%	2.854%
3	7.156	690	701	711	rBV	521420	937440	29.66%	3.359%
4	7.984	835	842	852	rVB	271507	464755	14.70%	1.665%
5	9.159	1034	1042	1048	rBV	333823	608620	19.25%	2.181%
6	10.575	1277	1283	1289	rBV2	18635	34402	1.09%	0.123%
7	10.804	1310	1322	1328	rBV	357823	670473	21.21%	2.402%
8	10.857	1328	1331	1336	rVB2	26942	41799	1.32%	0.150%
9	12.466	1599	1605	1612	rVB	31906	59504	1.88%	0.213%
10	12.684	1636	1642	1650	rBV	31940	51151	1.62%	0.183%
11	13.259	1731	1740	1752	rBV	911247	1376704	43.55%	4.932%
12	13.823	1826	1836	1840	rBV7	19035	49369	1.56%	0.177%
13	13.964	1853	1860	1864	rBV3	43562	79536	2.52%	0.285%
14	14.011	1864	1868	1872	rVV4	21477	38334	1.21%	0.137%
15	14.058	1872	1876	1880	rVV3	34975	53452	1.69%	0.192%
16	14.370	1922	1929	1936	rBV	97445	219279	6.94%	0.786%
17	14.464	1941	1945	1951	rVV4	42191	75656	2.39%	0.271%
18	14.528	1952	1956	1963	rVV10	13912	34662	1.10%	0.124%
19	14.646	1965	1976	1982	rVB	526010	866337	27.41%	3.104%
20	14.710	1982	1987	1993	rBV4	29616	64792	2.05%	0.232%
21	14.857	2006	2012	2017	rBV9	15592	40119	1.27%	0.144%
22	15.039	2039	2043	2048	rVV	38374	54301	1.72%	0.195%
23	15.116	2052	2056	2060	rVB3	32616	45623	1.44%	0.163%
24	15.263	2074	2081	2085	rBV5	41910	94296	2.98%	0.338%
25	15.427	2102	2109	2113	rBV6	60715	111636	3.53%	0.400%
26	15.527	2121	2126	2129	rBV4	26770	40503	1.28%	0.145%
27	15.691	2149	2154	2167	rVB4	62296	136481	4.32%	0.489%
28	16.138	2224	2230	2238	rBV	691407	1033413	32.69%	3.702%
29	16.367	2265	2269	2275	rVB5	60314	99826	3.16%	0.358%
30	16.749	2331	2334	2338	rVB4	37976	51701	1.64%	0.185%
31	17.048	2382	2385	2391	rVB2	48696	73193	2.32%	0.262%
32	17.213	2411	2413	2421	rVB	61557	90340	2.86%	0.324%
33	17.401	2439	2445	2448	rBV	521237	839077	26.54%	3.006%
34	17.442	2448	2452	2458	rVB	875163	1273383	40.28%	4.562%
35	17.530	2463	2467	2472	rBV	102280	158054	5.00%	0.566%
36	17.589	2473	2477	2482	rVV4	43876	86747	2.74%	0.311%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049922.D
 Acq On : 20 Aug 2021 23:33
 Operator : CG/JU
 Sample : M3419-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.982	2541	2544	2549	rVB	81438	114600	3.63%	0.411%
38	18.276	2590	2594	2598	rBV	302275	459323	14.53%	1.646%
39	18.323	2598	2602	2608	rVB	373083	569568	18.02%	2.041%
40	18.464	2622	2626	2631	rBV2	352114	675513	21.37%	2.420%
41	18.505	2631	2633	2641	rVB	251256	345198	10.92%	1.237%
42	18.770	2675	2678	2682	rBV	156333	216587	6.85%	0.776%
43	18.822	2683	2687	2693	rVB3	208481	301109	9.53%	1.079%
44	19.069	2727	2729	2733	rVB	111245	110706	3.50%	0.397%
45	19.192	2746	2750	2754	rBV	337479	523884	16.57%	1.877%
46	19.339	2771	2775	2782	rBV3	138222	284199	8.99%	1.018%
47	19.463	2790	2796	2801	rVB	1891640	2704679	85.56%	9.690%
48	19.827	2848	2858	2864	rBV	1920179	3161056	100.00%	11.325%
49	19.892	2866	2869	2871	rBV	151157	197290	6.24%	0.707%
50	20.015	2885	2890	2894	rVB	1208024	1646673	52.09%	5.900%
51	20.426	2955	2960	2964	rBV2	594702	860513	27.22%	3.083%
52	20.473	2965	2968	2972	rVB	325809	398514	12.61%	1.428%
53	20.614	2989	2992	2996	rVV	245618	291207	9.21%	1.043%
54	20.655	2996	2999	3008	rVB2	255017	460274	14.56%	1.649%
55	21.677	3167	3173	3179	rBV3	829596	2249829	71.17%	8.060%
56	21.736	3180	3183	3193	rVB	909122	1516648	47.98%	5.434%



Sum of corrected areas: 27911823

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049922.D
Acq On : 20 Aug 2021 23:33
Operator : CG/JU
Sample : M3419-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

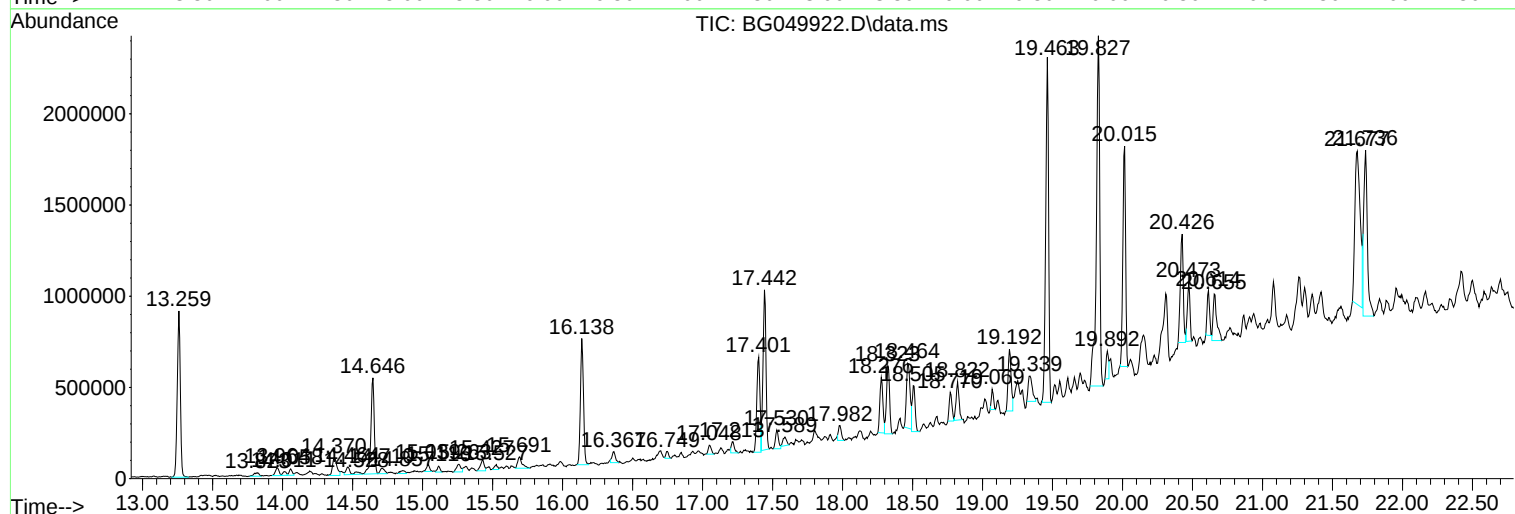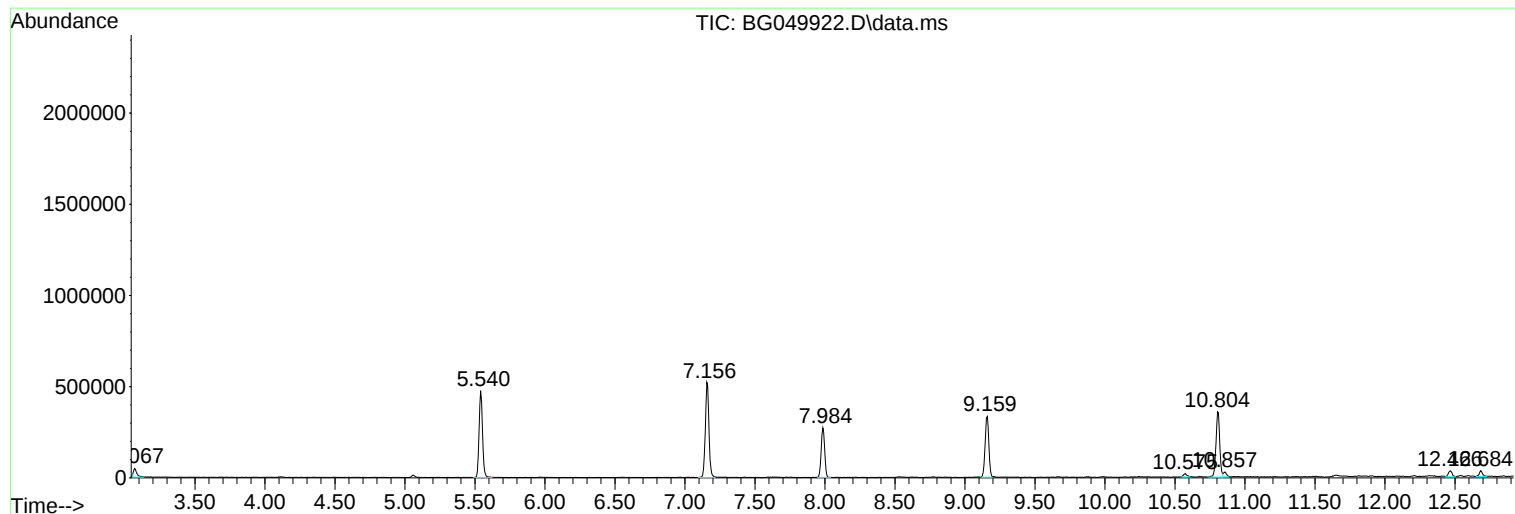

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049922.D
Acq On : 20 Aug 2021 23:33
Operator : CG/JU
Sample : M3419-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049922.D
Acq On : 20 Aug 2021 23:33
Operator : CG/JU
Sample : M3419-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
