

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049923.D
 Acq On : 21 Aug 2021 00:15
 Operator : CG/JU
 Sample : M3394-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-07-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.542	420	426	440	rBV	392649	670278	4.27%	0.600%
2	7.164	694	702	716	rBV	427839	772893	4.92%	0.692%
3	7.986	834	842	851	rVB	132442	231492	1.47%	0.207%
4	9.161	1034	1042	1049	rBV	285864	518567	3.30%	0.464%
5	10.812	1314	1323	1328	rBV	176381	329503	2.10%	0.295%
6	13.261	1733	1740	1747	rVB	735597	1135312	7.23%	1.016%
7	13.966	1854	1860	1865	rBV2	100390	182160	1.16%	0.163%
8	14.372	1921	1929	1942	rBV	184142	440077	2.80%	0.394%
9	14.648	1971	1976	1981	rVB	248980	394254	2.51%	0.353%
10	14.712	1981	1987	1994	rVB	230516	382307	2.43%	0.342%
11	15.047	2037	2044	2051	rVB	384154	605773	3.86%	0.542%
12	15.699	2148	2155	2166	rVB	696040	1115985	7.10%	0.999%
13	15.987	2200	2204	2210	rVB	226553	370042	2.36%	0.331%
14	16.146	2222	2231	2238	rBV	742380	1337199	8.51%	1.197%
15	16.704	2315	2326	2331	rBV3	202280	419920	2.67%	0.376%
16	16.933	2357	2365	2368	rBV2	137539	246621	1.57%	0.221%
17	17.062	2381	2387	2393	rVB	454435	716647	4.56%	0.642%
18	17.133	2393	2399	2406	rVV	134709	270715	1.72%	0.242%
19	17.221	2409	2414	2424	rVB	459594	744960	4.74%	0.667%
20	17.473	2440	2457	2462	rBV	6277002	12884280	82.01%	11.536%
21	17.550	2462	2470	2475	rVV	2042809	2998718	19.09%	2.685%
22	17.808	2506	2514	2528	rVV	574049	1194492	7.60%	1.069%
23	17.920	2528	2533	2537	rVV	166570	265685	1.69%	0.238%
24	17.990	2540	2545	2552	rVB5	215253	392769	2.50%	0.352%
25	18.125	2565	2568	2577	rVB	93411	190745	1.21%	0.171%
26	18.284	2589	2595	2599	rBV	886578	1313608	8.36%	1.176%
27	18.337	2599	2604	2610	rVB	1179875	1769514	11.26%	1.584%
28	18.413	2612	2617	2622	rBV	390701	570572	3.63%	0.511%
29	18.484	2622	2629	2633	rBV3	1213489	2357340	15.01%	2.111%
30	18.777	2674	2679	2684	rBV	717917	981337	6.25%	0.879%
31	18.836	2684	2689	2695	rVB	555690	807655	5.14%	0.723%
32	19.024	2717	2721	2725	rVB	123875	170649	1.09%	0.153%
33	19.071	2726	2729	2733	rVB	174194	203262	1.29%	0.182%
34	19.112	2733	2736	2741	rVB2	149974	209219	1.33%	0.187%
35	19.195	2745	2750	2755	rBV	344488	632459	4.03%	0.566%
36	19.359	2773	2778	2784	rVB	468236	835520	5.32%	0.748%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049923.D
 Acq On : 21 Aug 2021 00:15
 Operator : CG/JU
 Sample : M3394-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-07-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.500	2790	2802	2806	rBV	7276322	15710147	100.00%	14.066%
38	19.565	2809	2813	2818	rVB2	222094	327774	2.09%	0.293%
39	19.618	2818	2822	2826	rBV	259516	371018	2.36%	0.332%
40	19.712	2835	2838	2842	rVB	233602	301916	1.92%	0.270%
41	19.853	2850	2862	2866	rBV2	5672303	13110255	83.45%	11.738%
42	19.894	2866	2869	2876	rVB	458514	624782	3.98%	0.559%
43	20.011	2883	2889	2894	rBV2	1128996	1828485	11.64%	1.637%
44	20.070	2895	2899	2905	rVB	346056	559051	3.56%	0.501%
45	20.158	2906	2914	2919	rBV2	546383	1487756	9.47%	1.332%
46	20.205	2919	2922	2926	rVB	169230	198852	1.27%	0.178%
47	20.281	2930	2935	2937	rBV2	397805	697600	4.44%	0.625%
48	20.322	2938	2942	2946	rVB	1049513	1510493	9.61%	1.352%
49	20.416	2954	2958	2962	rBV	535673	752537	4.79%	0.674%
50	20.481	2962	2969	2973	rVB2	611382	1186391	7.55%	1.062%
51	20.616	2989	2992	2996	rBV	309039	412144	2.62%	0.369%
52	20.663	2997	3000	3003	rVB	328570	375448	2.39%	0.336%
53	21.086	3067	3072	3081	rVB	984016	1554466	9.89%	1.392%
54	21.268	3097	3103	3107	rBV2	947314	1837806	11.70%	1.645%
55	21.309	3107	3110	3114	rVV	656083	1012978	6.45%	0.907%
56	21.362	3115	3119	3124	rVV2	693836	1305366	8.31%	1.169%
57	21.433	3127	3131	3142	rVB	942941	1660517	10.57%	1.487%
58	21.691	3165	3175	3180	rBV2	3367652	8405731	53.51%	7.526%
59	21.762	3181	3187	3196	rVB	3312174	6509271	41.43%	5.828%
60	21.897	3207	3210	3216	rVB	237116	356498	2.27%	0.319%
61	21.967	3218	3222	3227	rBV3	228369	438234	2.79%	0.392%
62	22.102	3240	3245	3251	rBV2	489101	975913	6.21%	0.874%
63	22.425	3297	3300	3307	rVB	428358	730554	4.65%	0.654%
64	23.953	3547	3560	3566	rBV	1486028	6012092	38.27%	5.383%
65	24.828	3701	3709	3718	rVB	966340	2774489	17.66%	2.484%


Sum of corrected areas: 111691093

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049923.D
Acq On : 21 Aug 2021 00:15
Operator : CG/JU
Sample : M3394-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-07-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

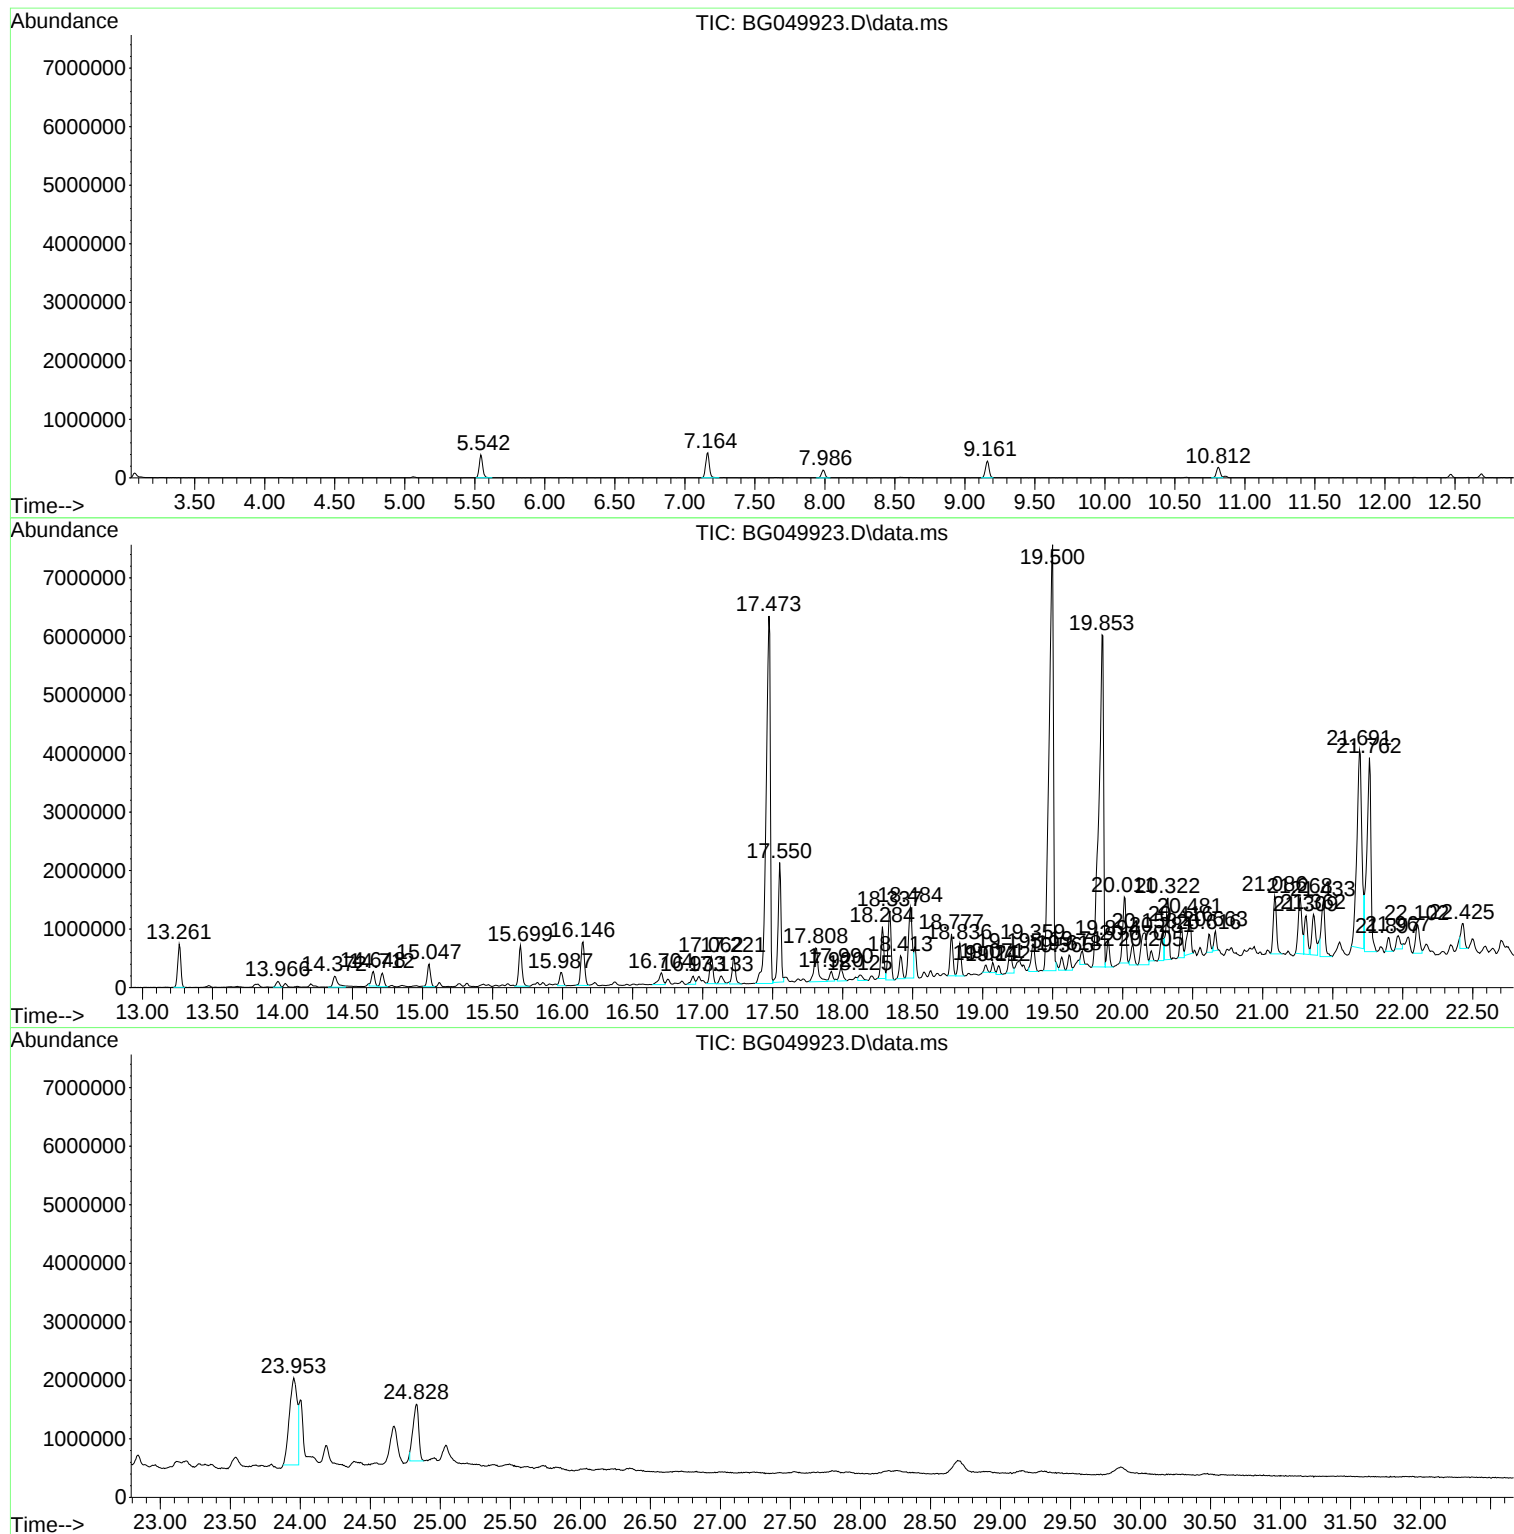

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049923.D
Acq On : 21 Aug 2021 00:15
Operator : CG/JU
Sample : M3394-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-07-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049923.D
Acq On : 21 Aug 2021 00:15
Operator : CG/JU
Sample : M3394-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-07-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------