

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049924.D
 Acq On : 21 Aug 2021 00:56
 Operator : CG/JU
 Sample : M3434-35
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-15-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.073	3	6	15	rVB	59498	99181	8.30%	0.798%
2	4.113	178	183	192	rVB2	8993	15673	1.31%	0.126%
3	5.059	339	344	352	rVB2	10195	16760	1.40%	0.135%
4	5.546	419	427	438	rBV	362900	654377	54.79%	5.263%
5	7.162	689	702	712	rBV	410775	748428	62.66%	6.019%
6	7.990	833	843	851	rBV	147731	260525	21.81%	2.095%
7	9.159	1035	1042	1049	rBV	268186	484119	40.53%	3.893%
8	10.575	1276	1283	1291	rBV4	11620	24922	2.09%	0.200%
9	10.810	1312	1323	1329	rBV	200528	369020	30.90%	2.968%
10	10.862	1329	1332	1337	rVB2	20205	31149	2.61%	0.251%
11	12.466	1599	1605	1612	rVB	18808	33014	2.76%	0.266%
12	12.689	1637	1643	1651	rVB2	11570	21271	1.78%	0.171%
13	13.259	1733	1740	1749	rVB	642886	1024222	85.75%	8.237%
14	13.964	1854	1860	1865	rBV5	13412	25286	2.12%	0.203%
15	14.017	1865	1869	1873	rVB5	7660	13312	1.11%	0.107%
16	14.105	1879	1884	1890	rBV7	10968	18334	1.54%	0.147%
17	14.369	1923	1929	1937	rBV	52828	110765	9.27%	0.891%
18	14.646	1967	1976	1983	rBV	290904	465098	38.94%	3.740%
19	14.710	1983	1987	1995	rVB4	14722	30212	2.53%	0.243%
20	15.045	2038	2044	2051	rBV	26375	48690	4.08%	0.392%
21	15.116	2053	2056	2062	rVB5	11125	18317	1.53%	0.147%
22	15.262	2075	2081	2085	rBV8	9760	20084	1.68%	0.162%
23	15.521	2122	2125	2131	rVB6	9118	12459	1.04%	0.100%
24	15.697	2150	2155	2161	rBV2	35236	56988	4.77%	0.458%
25	15.985	2199	2204	2210	rBV7	17289	33915	2.84%	0.273%
26	16.144	2224	2231	2237	rBV	527940	810982	67.90%	6.522%
27	16.349	2260	2266	2267	rBV5	13449	21890	1.83%	0.176%
28	16.373	2267	2270	2277	rVB9	21069	36165	3.03%	0.291%
29	16.696	2323	2325	2330	rVB6	15929	22521	1.89%	0.181%
30	16.749	2330	2334	2338	rBV5	13982	18506	1.55%	0.149%
31	17.054	2382	2386	2392	rBV2	26161	37874	3.17%	0.305%
32	17.130	2396	2399	2403	rBV6	16376	22810	1.91%	0.183%
33	17.219	2410	2414	2421	rVB2	28094	53050	4.44%	0.427%
34	17.401	2439	2445	2449	rBV	296371	469606	39.32%	3.777%
35	17.442	2449	2452	2460	rVB	372262	543501	45.51%	4.371%
36	17.536	2464	2468	2472	rVB	52049	69893	5.85%	0.562%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049924.D
 Acq On : 21 Aug 2021 00:56
 Operator : CG/JU
 Sample : M3434-35
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-15-0205

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.282	2591	2595	2598	rBV	85245	106157	8.89%	0.854%
38	18.329	2599	2603	2609	rVB	103531	153176	12.82%	1.232%
39	18.476	2622	2628	2632	rBV3	117790	234765	19.66%	1.888%
40	18.769	2675	2678	2683	rBV	50095	72594	6.08%	0.584%
41	18.822	2683	2687	2692	rBV2	85700	137066	11.48%	1.102%
42	19.192	2747	2750	2757	rBV3	76858	126579	10.60%	1.018%
43	19.463	2790	2796	2801	rBV	828586	1194362	100.00%	9.605%
44	19.786	2848	2851	2852	rBV	81872	87547	7.33%	0.704%
45	19.821	2853	2857	2864	rVB	744158	1109840	92.92%	8.925%
46	20.009	2884	2889	2894	rBV	742425	1001437	83.85%	8.054%
47	21.671	3166	3172	3178	rBV2	379915	996533	83.44%	8.014%
48	21.730	3179	3182	3189	rVB	296218	471553	39.48%	3.792%




Sum of corrected areas: 12434528

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049924.D
Acq On : 21 Aug 2021 00:56
Operator : CG/JU
Sample : M3434-35
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-15-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

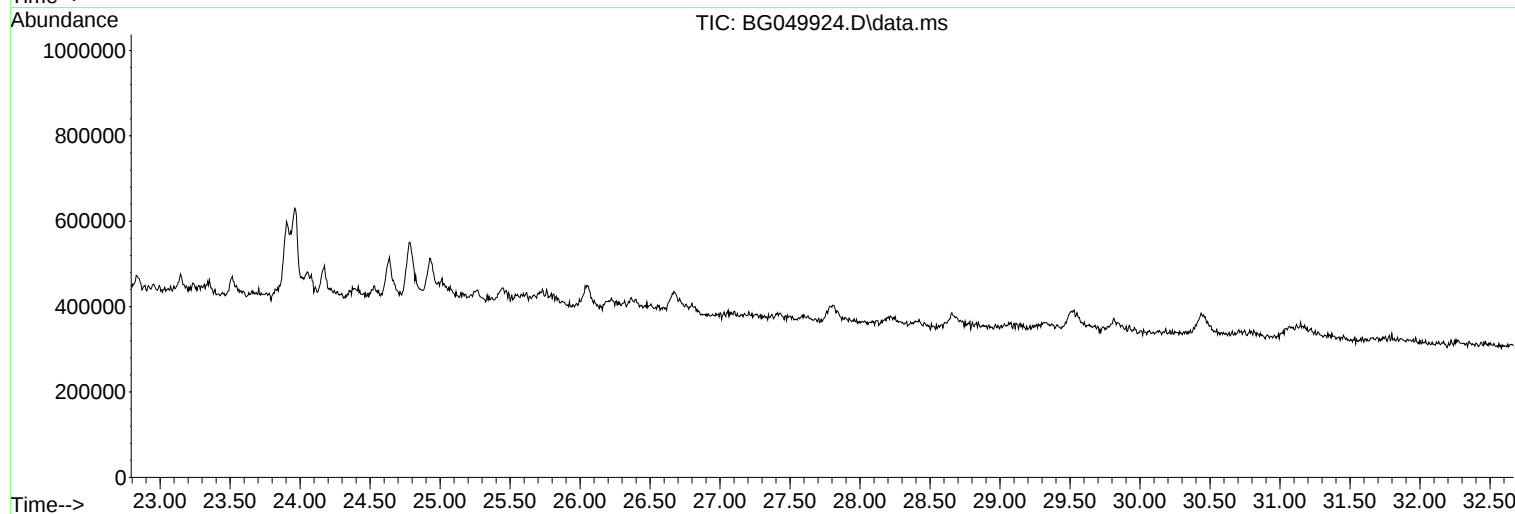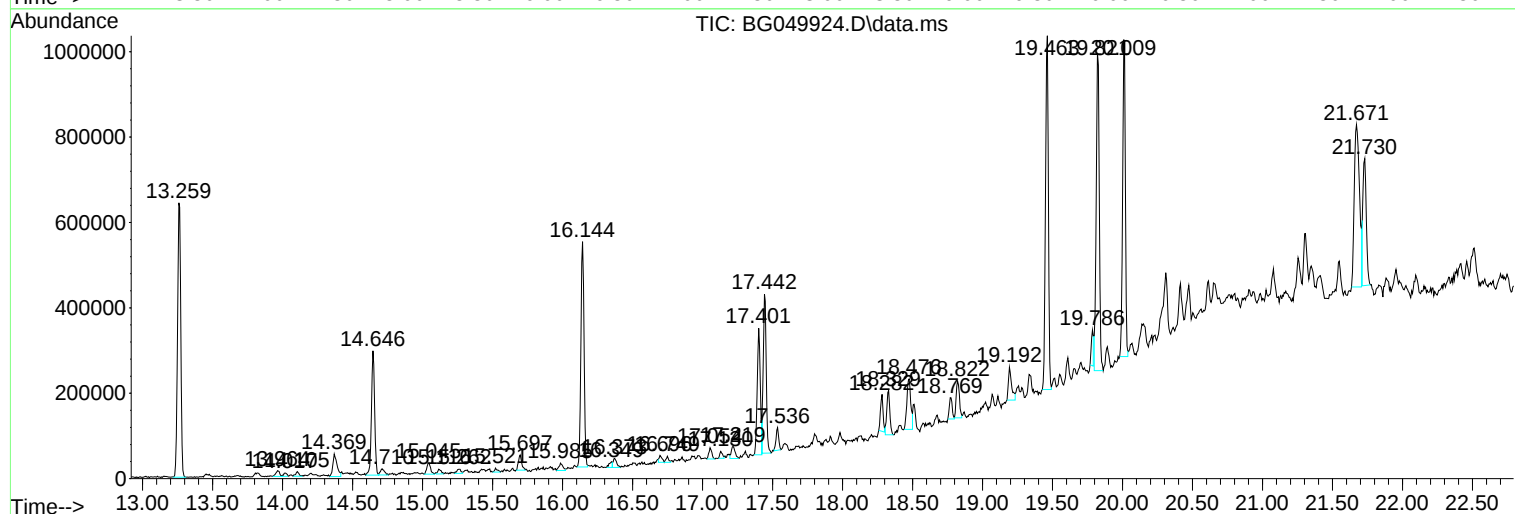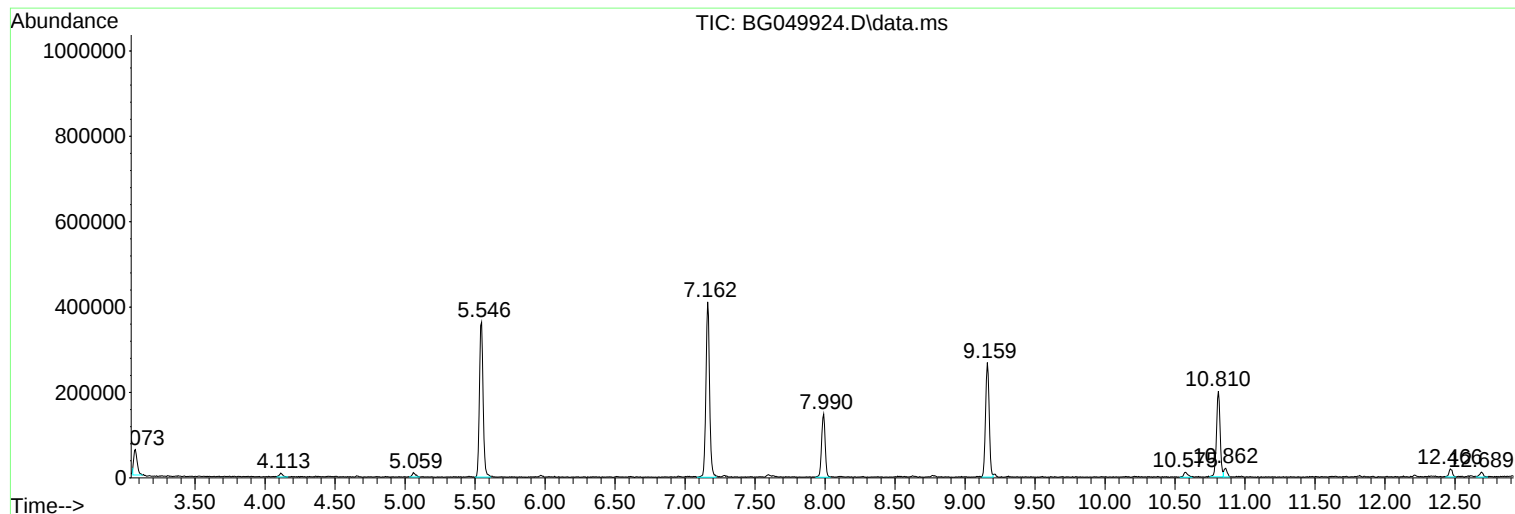

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049924.D
Acq On : 21 Aug 2021 00:56
Operator : CG/JU
Sample : M3434-35
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-15-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049924.D
Acq On : 21 Aug 2021 00:56
Operator : CG/JU
Sample : M3434-35
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-15-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------