

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049925.D
 Acq On : 21 Aug 2021 1:37
 Operator : CG/JU
 Sample : M3394-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-02-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.074	3	6	21	rVB	74137	143289	4.18%	0.484%
2	5.547	420	427	437	rBV	380800	679221	19.83%	2.293%
3	7.162	692	702	715	rBV	403009	762371	22.26%	2.574%
4	7.990	835	843	852	rVB	213498	378686	11.06%	1.278%
5	9.159	1035	1042	1051	rBV	275794	511972	14.95%	1.728%
6	10.810	1316	1323	1329	rBV	288776	533956	15.59%	1.802%
7	12.473	1599	1606	1612	rVB2	24694	44182	1.29%	0.149%
8	12.690	1637	1643	1650	rVB2	29073	54269	1.58%	0.183%
9	13.266	1733	1741	1752	rBV	712594	1121203	32.74%	3.785%
10	13.454	1769	1773	1784	rVB9	15400	36349	1.06%	0.123%
11	13.818	1829	1835	1842	rVB4	22608	56223	1.64%	0.190%
12	13.965	1854	1860	1865	rBV	57493	105415	3.08%	0.356%
13	14.018	1865	1869	1873	rVB2	31288	41444	1.21%	0.140%
14	14.106	1879	1884	1890	rBV3	23809	40482	1.18%	0.137%
15	14.206	1896	1901	1904	rBV3	27921	42367	1.24%	0.143%
16	14.370	1923	1929	1942	rBV	117095	289597	8.46%	0.978%
17	14.646	1966	1976	1983	rVV	396294	694729	20.29%	2.345%
18	14.717	1983	1988	1994	rVB3	24845	45721	1.33%	0.154%
19	14.858	2007	2012	2019	rBV6	17708	46106	1.35%	0.156%
20	15.046	2038	2044	2052	rVB3	59836	99512	2.91%	0.336%
21	15.122	2052	2057	2065	rVB	47337	77475	2.26%	0.262%
22	15.263	2075	2081	2085	rBV3	43102	80862	2.36%	0.273%
23	15.316	2087	2090	2094	rVB	30910	43250	1.26%	0.146%
24	15.427	2102	2109	2110	rBV6	35219	57618	1.68%	0.195%
25	15.474	2114	2117	2121	rVB4	32074	45210	1.32%	0.153%
26	15.527	2121	2126	2130	rBV	25538	43576	1.27%	0.147%
27	15.698	2149	2155	2167	rVB2	88965	186163	5.44%	0.628%
28	15.909	2185	2191	2196	rBV10	19470	41385	1.21%	0.140%
29	15.991	2199	2205	2211	rVB3	37153	75069	2.19%	0.253%
30	16.144	2225	2231	2238	rVB	547774	841432	24.57%	2.840%
31	16.367	2266	2269	2274	rVB5	62872	97126	2.84%	0.328%
32	16.702	2318	2326	2331	rBV4	59826	129779	3.79%	0.438%
33	16.755	2331	2335	2340	rVB2	52517	74421	2.17%	0.251%
34	16.855	2348	2352	2356	rVB3	41033	61526	1.80%	0.208%
35	17.055	2382	2386	2391	rBV3	74392	113406	3.31%	0.383%
36	17.137	2396	2400	2405	rVB4	43760	72181	2.11%	0.244%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049925.D
 Acq On : 21 Aug 2021 1:37
 Operator : CG/JU
 Sample : M3394-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-02-0002

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.219	2411	2414	2420	rVB	87633	131518	3.84%	0.444%
38	17.407	2440	2446	2449	rBV	395469	663077	19.36%	2.238%
39	17.448	2449	2453	2460	rVV	1338114	2025239	59.13%	6.837%
40	17.536	2464	2468	2472	rBV	91566	135694	3.96%	0.458%
41	17.589	2473	2477	2483	rVB2	44077	94972	2.77%	0.321%
42	17.807	2509	2514	2523	rBV3	69674	179761	5.25%	0.607%
43	17.918	2530	2533	2537	rVB	61255	71905	2.10%	0.243%
44	17.983	2541	2544	2550	rVB	104015	160494	4.69%	0.542%
45	18.282	2590	2595	2599	rBV	385487	565937	16.52%	1.910%
46	18.329	2599	2603	2609	rVB	434192	650645	19.00%	2.196%
47	18.412	2614	2617	2622	rVV2	52291	82511	2.41%	0.279%
48	18.476	2622	2628	2632	rVV2	432037	871024	25.43%	2.940%
49	18.512	2632	2634	2639	rVB	295921	383171	11.19%	1.293%
50	18.776	2675	2679	2683	rBV	218345	315320	9.21%	1.064%
51	18.829	2683	2688	2697	rVB	361674	552827	16.14%	1.866%
52	19.075	2726	2730	2733	rBV	118231	141216	4.12%	0.477%
53	19.117	2734	2737	2741	rVB2	79305	94974	2.77%	0.321%
54	19.199	2746	2751	2755	rBV	317477	542830	15.85%	1.832%
55	19.346	2771	2776	2782	rBV4	192554	399747	11.67%	1.349%
56	19.469	2790	2797	2802	rVB	2213661	3424833	100.00%	11.561%
57	19.616	2818	2822	2825	rBV	103532	156312	4.56%	0.528%
58	19.833	2854	2859	2865	rVB	2254391	3361364	98.15%	11.347%
59	19.892	2866	2869	2875	rVB2	168791	249988	7.30%	0.844%
60	20.015	2885	2890	2894	rVB	882478	1167439	34.09%	3.941%
61	20.156	2908	2914	2920	rBV3	187064	422733	12.34%	1.427%
62	20.415	2955	2958	2961	rBV	232330	252171	7.36%	0.851%
63	20.474	2965	2968	2973	rVB	258006	353351	10.32%	1.193%
64	20.615	2989	2992	2996	rBV	226161	295777	8.64%	0.998%
65	20.662	2997	3000	3010	rVB2	227394	401110	11.71%	1.354%
66	21.079	3069	3071	3080	rVB	216515	320546	9.36%	1.082%
67	21.678	3167	3173	3179	rBV3	675724	1863918	54.42%	6.292%
68	21.737	3180	3183	3195	rVB	827323	1523264	44.48%	5.142%




Sum of corrected areas: 29623241

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049925.D
Acq On : 21 Aug 2021 1:37
Operator : CG/JU
Sample : M3394-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-02-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

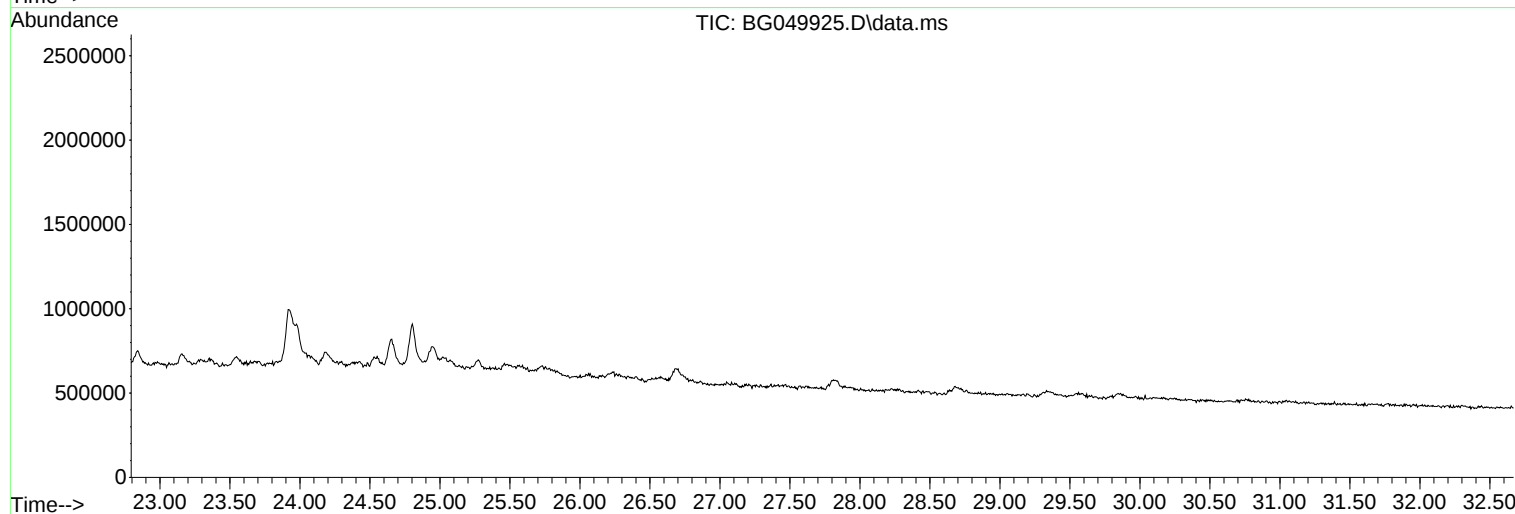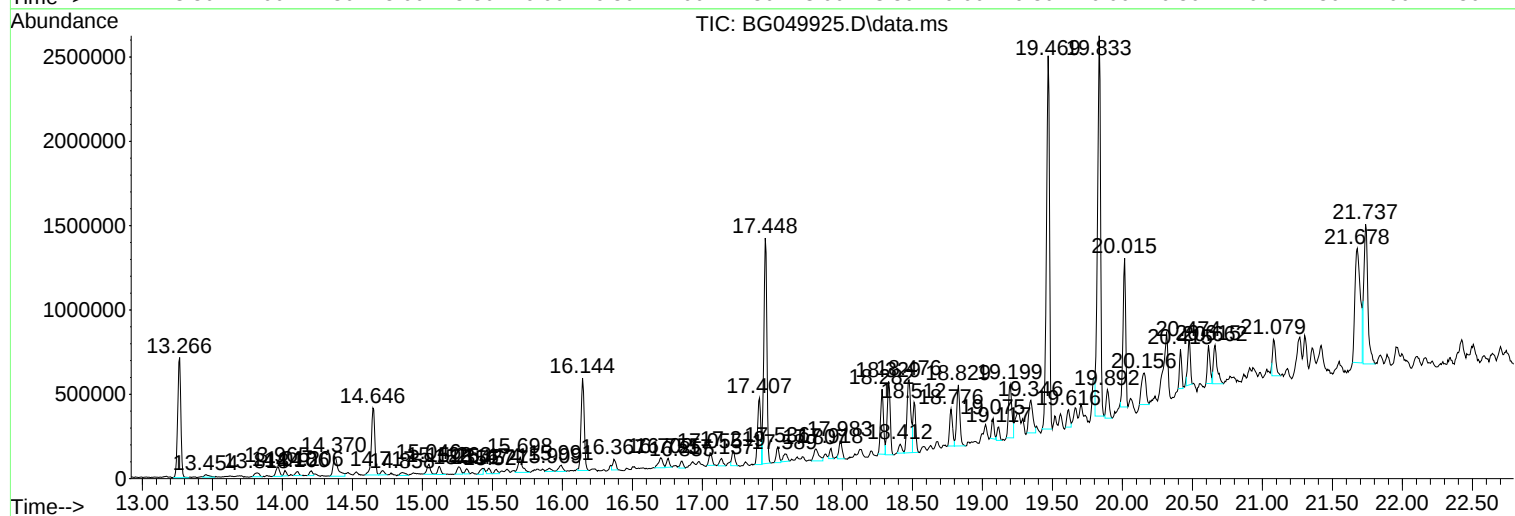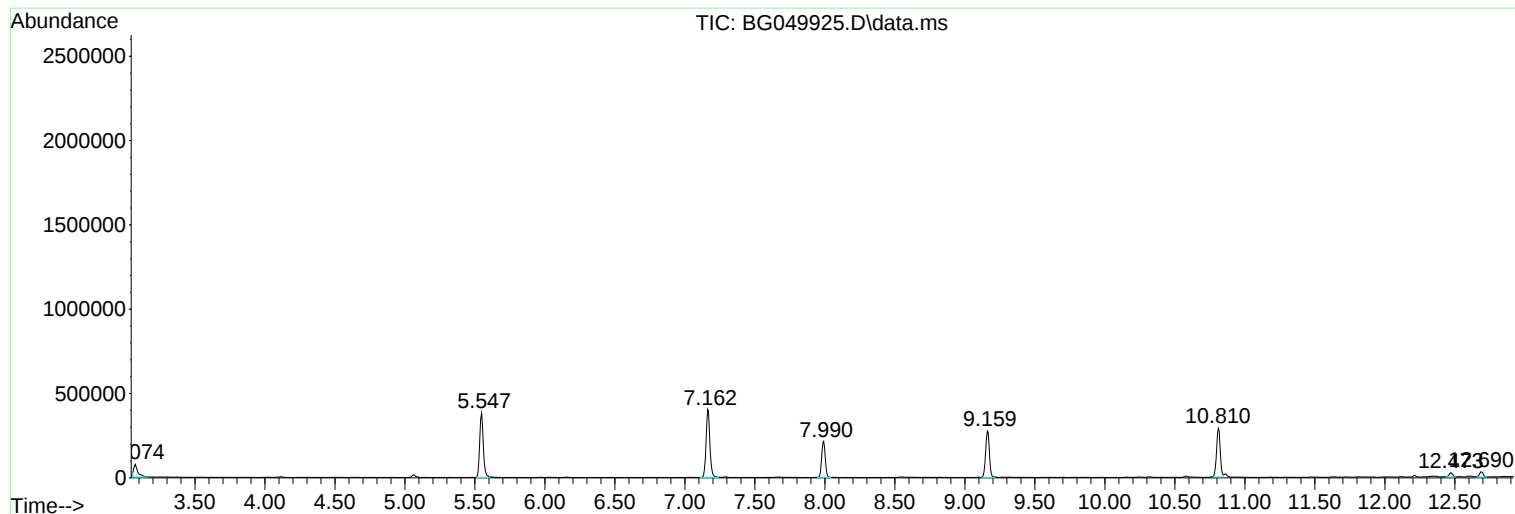

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049925.D
Acq On : 21 Aug 2021 1:37
Operator : CG/JU
Sample : M3394-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-02-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049925.D
Acq On : 21 Aug 2021 1:37
Operator : CG/JU
Sample : M3394-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-02-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------