

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049926.D
 Acq On : 21 Aug 2021 2:18
 Operator : CG/JU
 Sample : M3419-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.074	3	6	15	rVB	85368	141508	13.74%	1.809%
2	5.060	337	344	350	rBV2	11825	22499	2.18%	0.288%
3	5.547	419	427	438	rBV	380633	660643	64.15%	8.445%
4	7.169	694	703	714	rVB	424613	792529	76.96%	10.131%
5	7.991	835	843	853	rBV2	132425	242675	23.56%	3.102%
6	8.120	858	865	872	rVB2	17050	27936	2.71%	0.357%
7	8.208	875	880	885	rBV4	12520	20717	2.01%	0.265%
8	9.166	1035	1043	1055	rBV	283338	544483	52.87%	6.960%
9	10.576	1277	1283	1290	rBV3	23779	45021	4.37%	0.576%
10	10.811	1316	1323	1330	rBV	182412	333545	32.39%	4.264%
11	11.621	1454	1461	1465	rBV7	5865	16296	1.58%	0.208%
12	13.266	1731	1741	1751	rBV	667467	1029837	100.00%	13.165%
13	14.377	1926	1930	1934	rBV5	8005	16086	1.56%	0.206%
14	14.647	1969	1976	1983	rBV	259944	420978	40.88%	5.381%
15	14.711	1983	1987	1992	rVB6	8487	12684	1.23%	0.162%
16	16.145	2225	2231	2238	rBV	541860	859809	83.49%	10.991%
17	16.344	2262	2265	2268	rBV4	10225	15940	1.55%	0.204%
18	17.408	2440	2446	2449	rBV	256807	407029	39.52%	5.203%
19	17.449	2449	2453	2460	rVB	135930	205236	19.93%	2.624%
20	19.017	2717	2720	2725	rVB3	90601	119930	11.65%	1.533%
21	19.464	2792	2796	2801	rVB	346653	448548	43.56%	5.734%
22	19.828	2854	2858	2866	rVB	308150	452786	43.97%	5.788%
23	20.016	2885	2890	2895	rBV	735716	986064	95.75%	12.605%




Sum of corrected areas: 7822779

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049926.D
Acq On : 21 Aug 2021 2:18
Operator : CG/JU
Sample : M3419-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

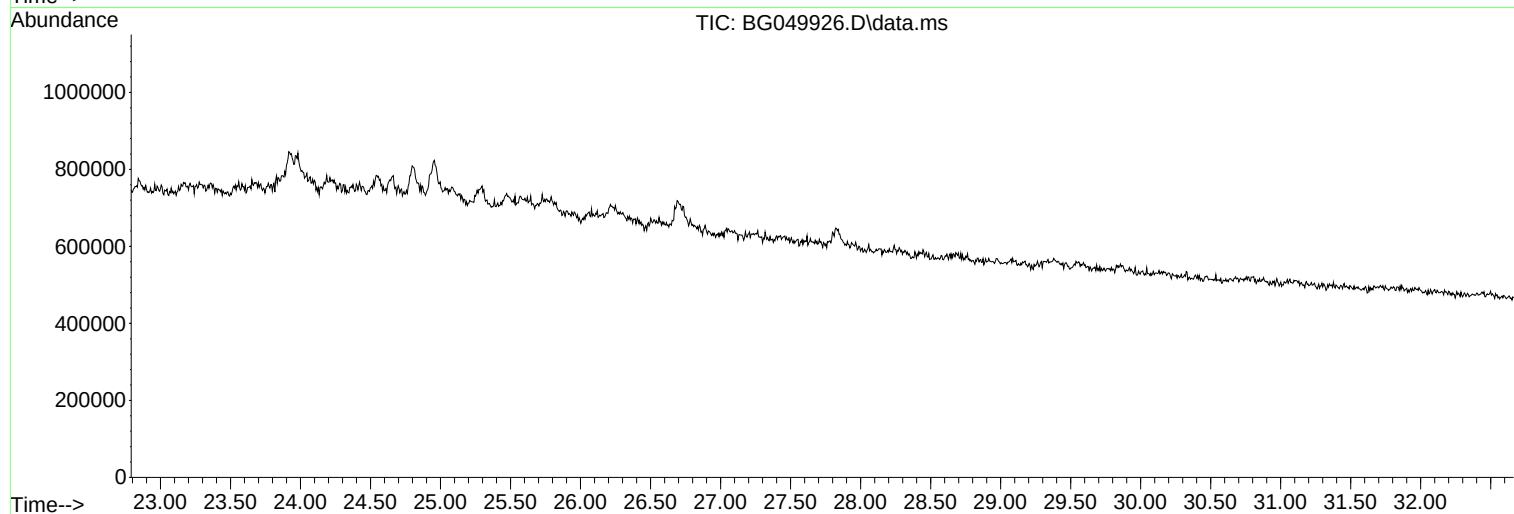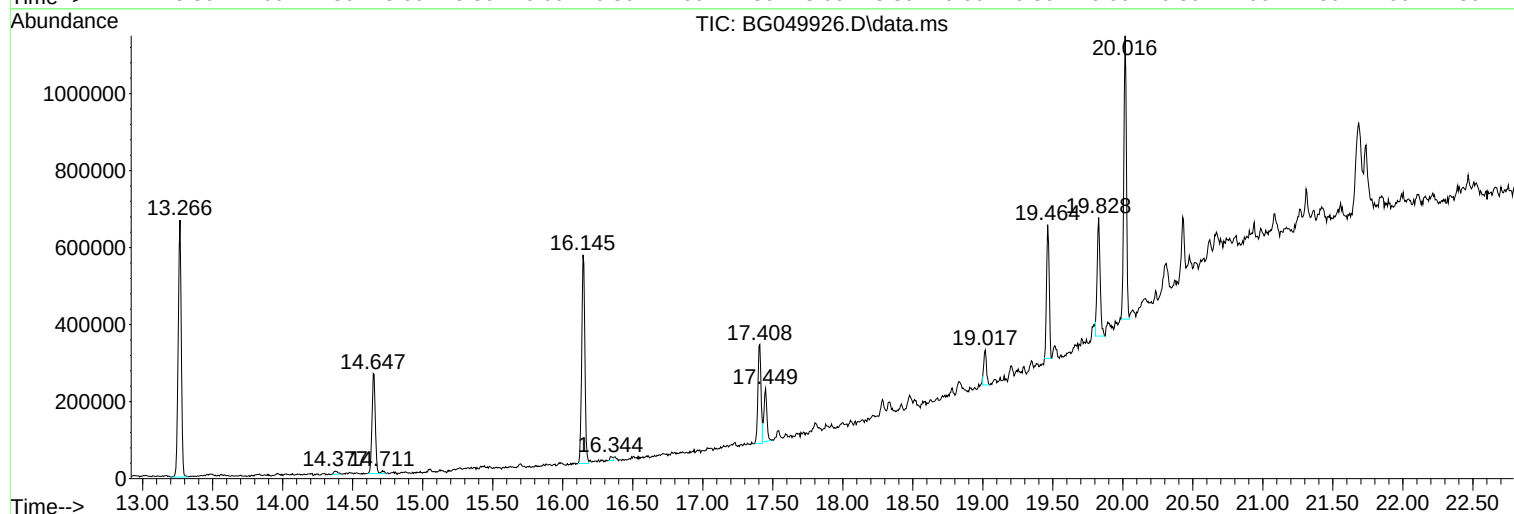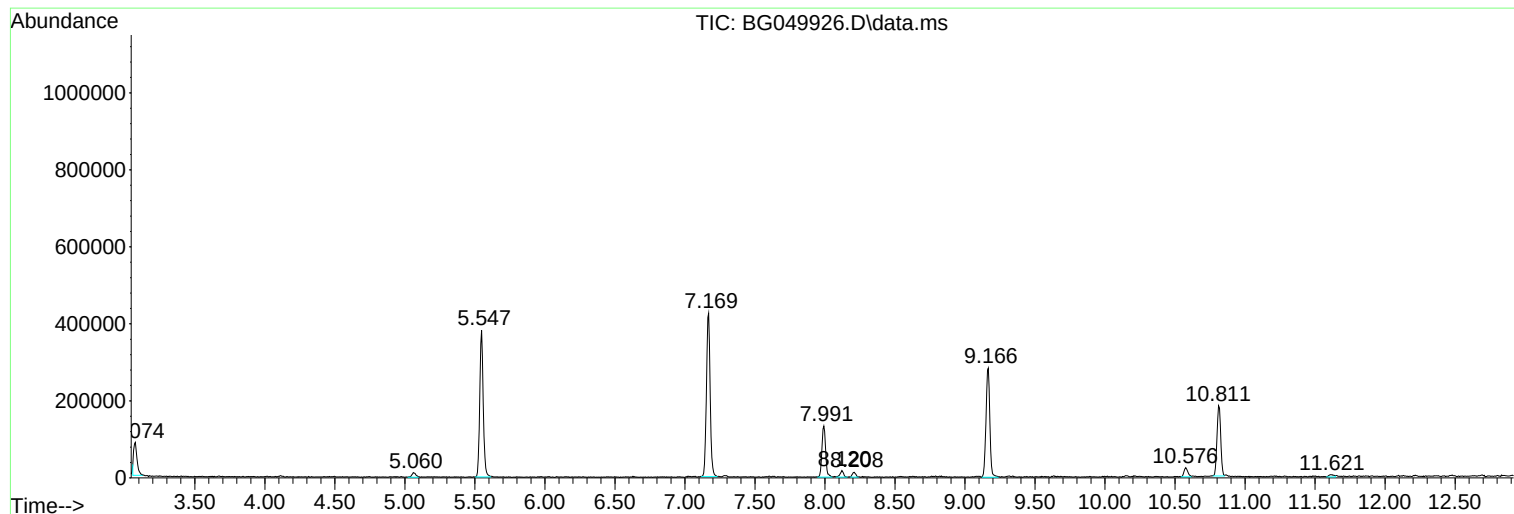

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049926.D
Acq On : 21 Aug 2021 2:18
Operator : CG/JU
Sample : M3419-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049926.D
Acq On : 21 Aug 2021 2:18
Operator : CG/JU
Sample : M3419-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------