

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049927.D
 Acq On : 21 Aug 2021 2:59
 Operator : CG/JU
 Sample : M3419-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-09-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.071	3	5	19	rVB	106102	169873	12.44%	1.732%
2	4.116	177	183	188	rBV4	7991	16208	1.19%	0.165%
3	5.062	337	344	354	rVB2	13126	27248	2.00%	0.278%
4	5.550	419	427	446	rVB	495460	909842	66.63%	9.276%
5	5.972	495	499	506	rBV3	11912	22678	1.66%	0.231%
6	7.065	679	685	691	rBV	16641	25393	1.86%	0.259%
7	7.171	691	703	716	rVV	534339	1014157	74.27%	10.339%
8	7.288	718	723	730	rVB4	8345	17051	1.25%	0.174%
9	7.635	777	782	792	rVB2	22320	41605	3.05%	0.424%
10	7.993	836	843	854	rBV2	127212	228731	16.75%	2.332%
11	8.105	857	862	867	rBV3	9804	14678	1.07%	0.150%
12	8.540	930	936	942	rBV5	10180	21033	1.54%	0.214%
13	8.628	946	951	957	rBV4	15426	27139	1.99%	0.277%
14	9.098	1026	1031	1035	rBV3	11406	19021	1.39%	0.194%
15	9.168	1035	1043	1051	rVV	346138	634692	46.48%	6.471%
16	9.685	1127	1131	1138	rVB4	9606	16491	1.21%	0.168%
17	10.578	1275	1283	1291	rBV2	139598	268669	19.67%	2.739%
18	10.813	1312	1323	1330	rBV	171623	326534	23.91%	3.329%
19	12.475	1601	1606	1613	rVB3	16198	26981	1.98%	0.275%
20	12.693	1638	1643	1649	rVB3	10105	16384	1.20%	0.167%
21	13.268	1734	1741	1748	rBV	891378	1365591	100.00%	13.922%
22	13.639	1800	1804	1808	rVB2	22223	30481	2.23%	0.311%
23	13.838	1831	1838	1843	rVB5	14373	27856	2.04%	0.284%
24	14.385	1925	1931	1937	rBV2	15712	33655	2.46%	0.343%
25	14.655	1971	1977	1984	rVB	242948	392290	28.73%	3.999%
26	16.153	2225	2232	2240	rBV	669590	1058076	77.48%	10.787%
27	16.370	2263	2269	2273	rBV9	9584	24797	1.82%	0.253%
28	17.410	2440	2446	2450	rBV	245346	380343	27.85%	3.878%
29	17.451	2450	2453	2460	rVB	50168	78325	5.74%	0.799%
30	18.802	2678	2683	2690	rBV5	206130	332215	24.33%	3.387%
31	19.466	2792	2796	2802	rVB	128059	171498	12.56%	1.748%
32	19.824	2855	2857	2865	rVB	110662	140786	10.31%	1.435%
33	20.018	2885	2890	2897	rVB	1012837	1323366	96.91%	13.492%
34	20.118	2903	2907	2912	rBV	478242	605164	44.32%	6.170%

Sum of corrected areas: 9808851

Instrument :

BNA_G

ClientSampleId :




SWCS-09-0002

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049927.D
Acq On : 21 Aug 2021 2:59
Operator : CG/JU
Sample : M3419-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

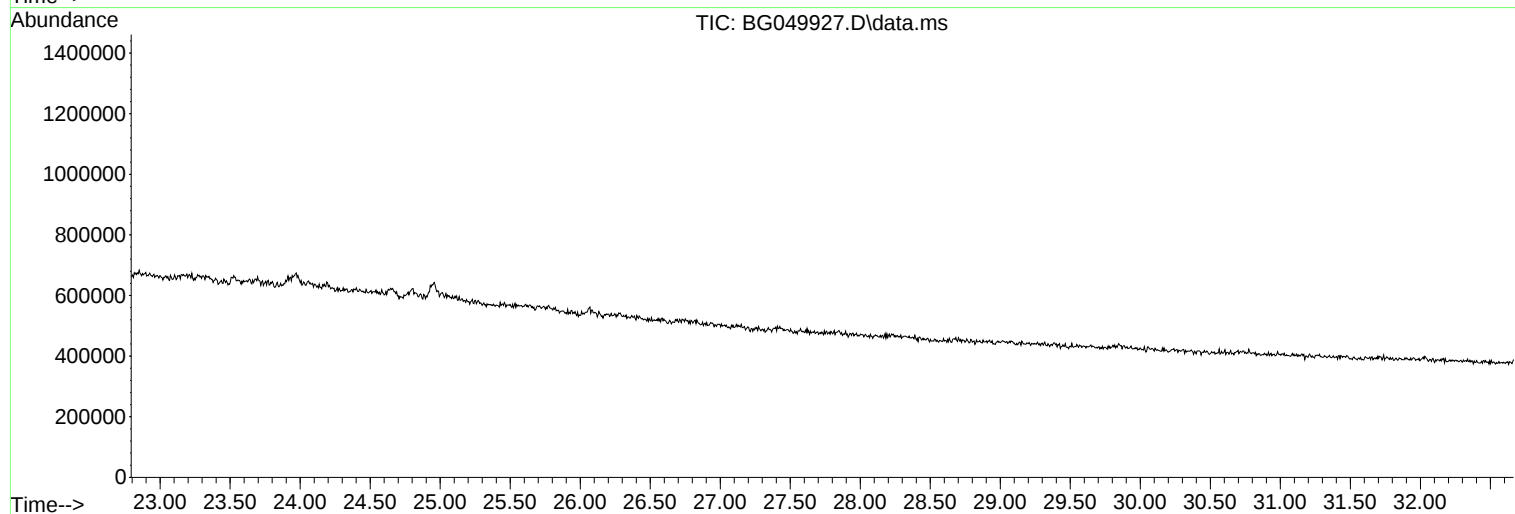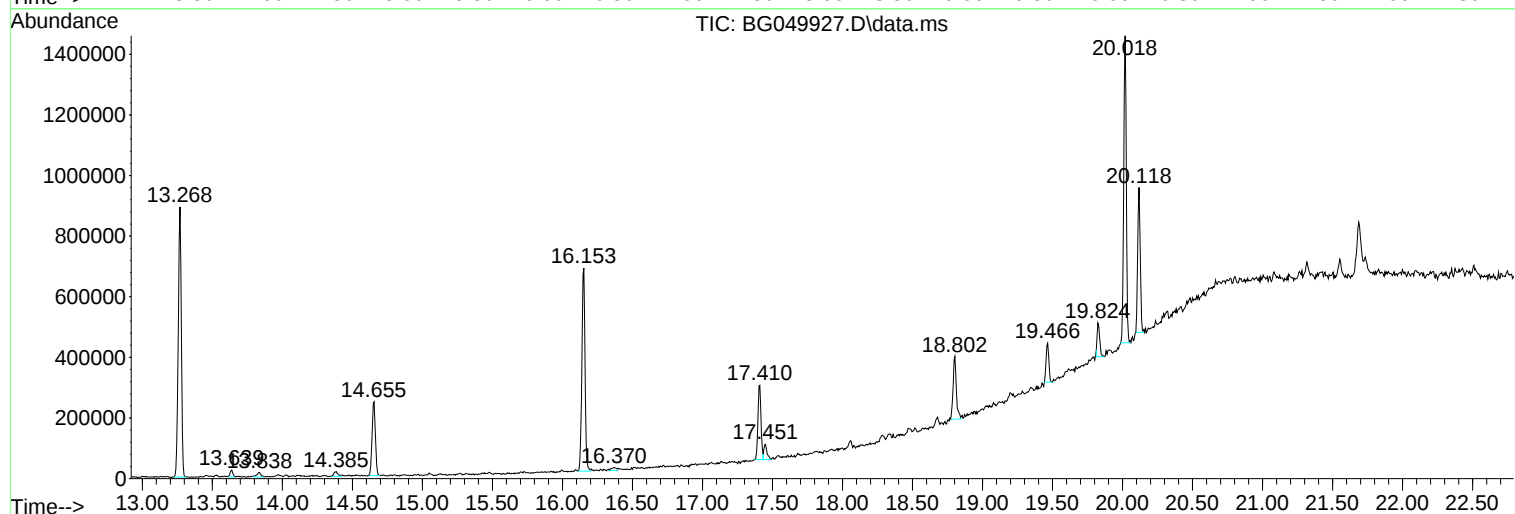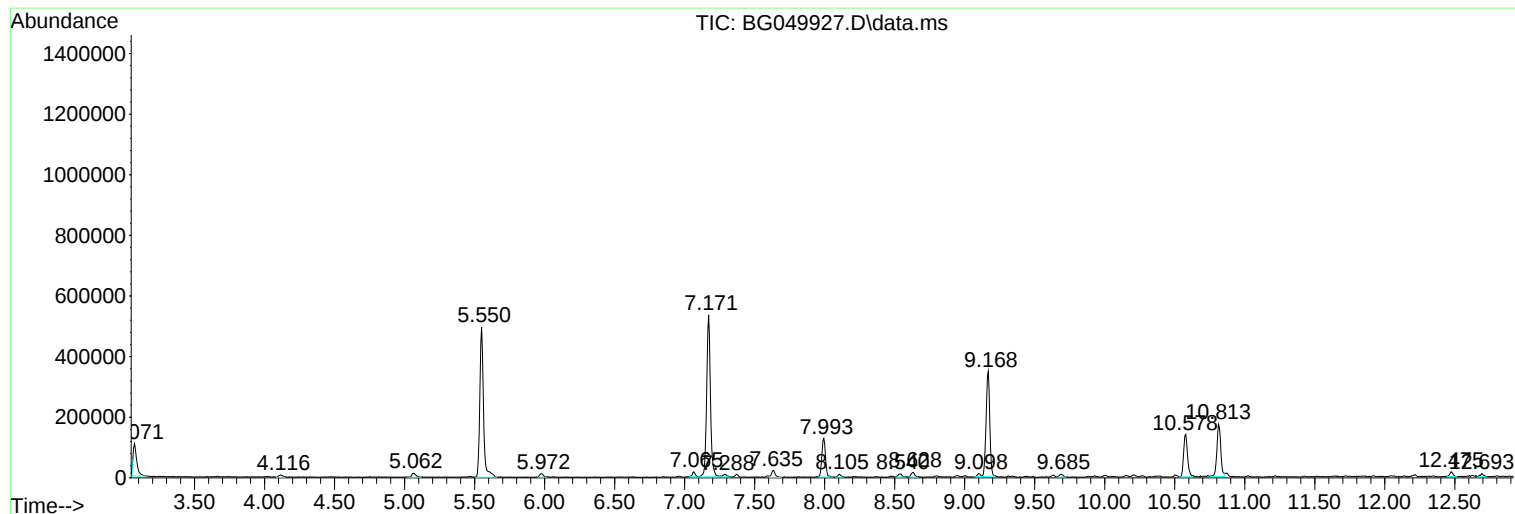

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049927.D
Acq On : 21 Aug 2021 2:59
Operator : CG/JU
Sample : M3419-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049927.D
Acq On : 21 Aug 2021 2:59
Operator : CG/JU
Sample : M3419-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------