

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049928.D
 Acq On : 21 Aug 2021 3:40
 Operator : CG/JU
 Sample : M3419-23
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-09-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.068	3	5	17	rVB	95590	154088	13.81%	1.950%
2	4.114	178	183	190	rVB4	10476	14776	1.32%	0.187%
3	5.060	340	344	353	rBV3	13788	28799	2.58%	0.364%
4	5.547	420	427	435	rBV	383878	689888	61.82%	8.731%
5	5.976	495	500	507	rVB	21209	37335	3.35%	0.473%
6	6.951	659	666	672	rBV6	5613	11735	1.05%	0.149%
7	7.069	680	686	690	rVB	20940	32882	2.95%	0.416%
8	7.169	690	703	715	rVV	430049	843281	75.56%	10.673%
9	7.286	717	723	731	rVV2	7612	17014	1.52%	0.215%
10	7.374	731	738	744	rVB3	11404	20806	1.86%	0.263%
11	7.633	777	782	789	rVB2	29818	49991	4.48%	0.633%
12	7.991	834	843	851	rBV	128895	231630	20.75%	2.932%
13	8.103	858	862	868	rVB2	11297	18440	1.65%	0.233%
14	8.537	930	936	941	rBV2	13033	21501	1.93%	0.272%
15	8.631	946	952	960	rVB5	19696	38065	3.41%	0.482%
16	8.943	1002	1005	1010	rBV3	7725	11761	1.05%	0.149%
17	9.101	1027	1032	1036	rBV4	11464	19833	1.78%	0.251%
18	9.166	1036	1043	1052	rVV2	287042	514525	46.10%	6.512%
19	9.630	1117	1122	1126	rBV	8556	12702	1.14%	0.161%
20	9.689	1128	1132	1139	rVB2	11039	17770	1.59%	0.225%
21	10.499	1265	1270	1277	rBV3	10496	19921	1.78%	0.252%
22	10.576	1277	1283	1294	rVV2	108786	204180	18.30%	2.584%
23	10.817	1314	1324	1330	rBV	176296	334327	29.96%	4.231%
24	12.215	1558	1562	1568	rVB6	5890	11675	1.05%	0.148%
25	12.479	1602	1607	1612	rVB	13827	25309	2.27%	0.320%
26	12.632	1625	1633	1637	rVB7	5682	12347	1.11%	0.156%
27	12.697	1637	1644	1651	rVB5	9111	18058	1.62%	0.229%
28	13.266	1731	1741	1749	rBV	732556	1116025	100.00%	14.124%
29	13.636	1800	1804	1808	rVB	10802	16976	1.52%	0.215%
30	13.824	1832	1836	1844	rVB8	9347	19878	1.78%	0.252%
31	14.382	1925	1931	1936	rBV3	12220	29347	2.63%	0.371%
32	14.653	1970	1977	1984	rBV	266649	416072	37.28%	5.266%
33	15.052	2041	2045	2053	rVB9	6468	14358	1.29%	0.182%
34	16.151	2226	2232	2239	rBV	541948	867323	77.72%	10.977%
35	16.345	2262	2265	2269	rBV4	15620	20585	1.84%	0.261%
36	17.408	2440	2446	2450	rBV	271002	410548	36.79%	5.196%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049928.D
Acq On : 21 Aug 2021 3:40
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0205

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.449	2450	2453	2458	rVB	75342	107618	9.64%	1.362%
38	17.807	2512	2514	2517	rBV4	10075	11236	1.01%	0.142%
39	18.054	2553	2556	2560	rBV5	21115	30159	2.70%	0.382%
40	19.464	2792	2796	2803	rBV	152437	213018	19.09%	2.696%
41	19.828	2854	2858	2863	rVB	124350	185655	16.64%	2.350%
42	20.016	2885	2890	2895	rBV	808502	1029921	92.28%	13.035%




Sum of corrected areas: 7901358

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049928.D
Acq On : 21 Aug 2021 3:40
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

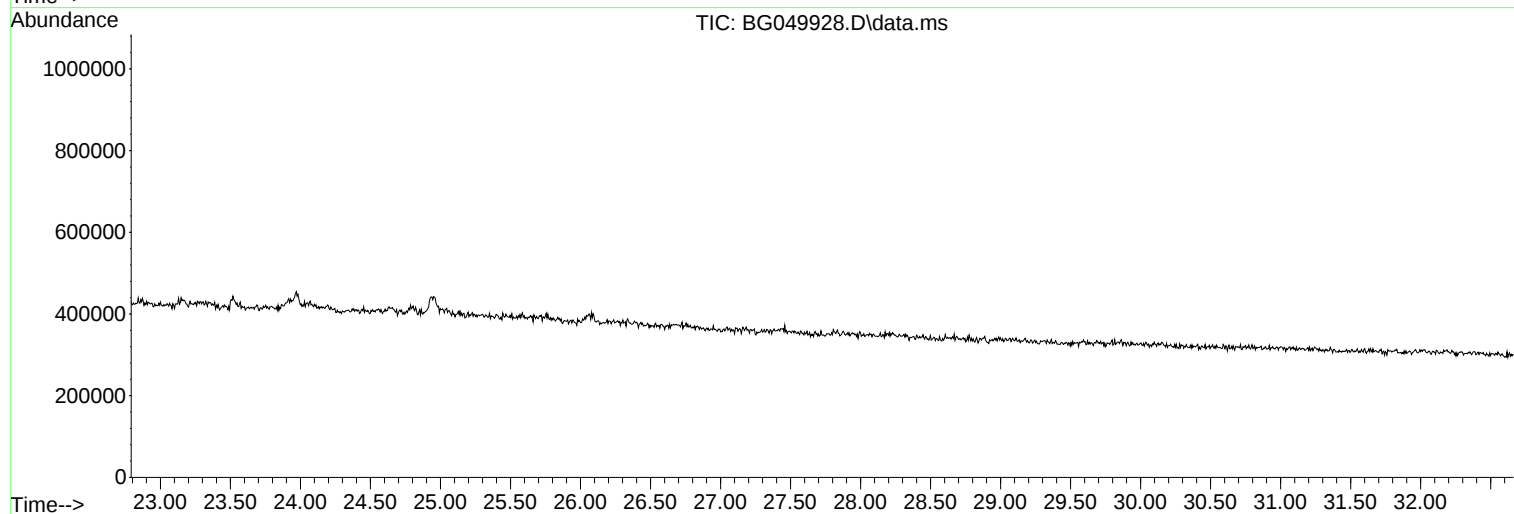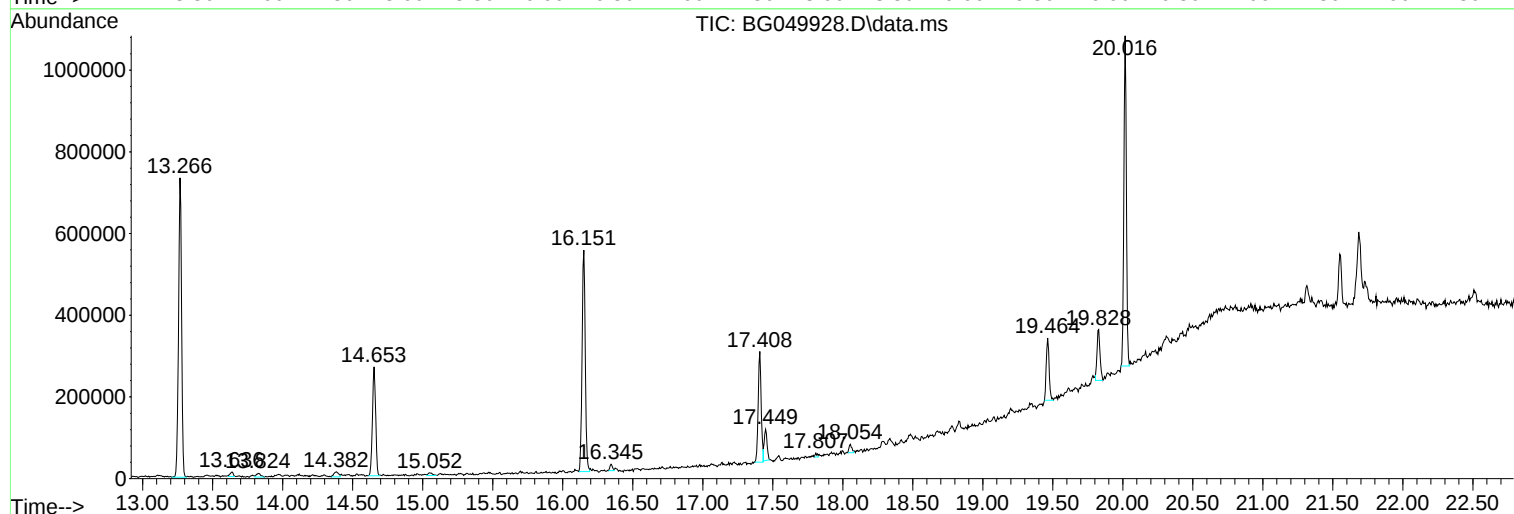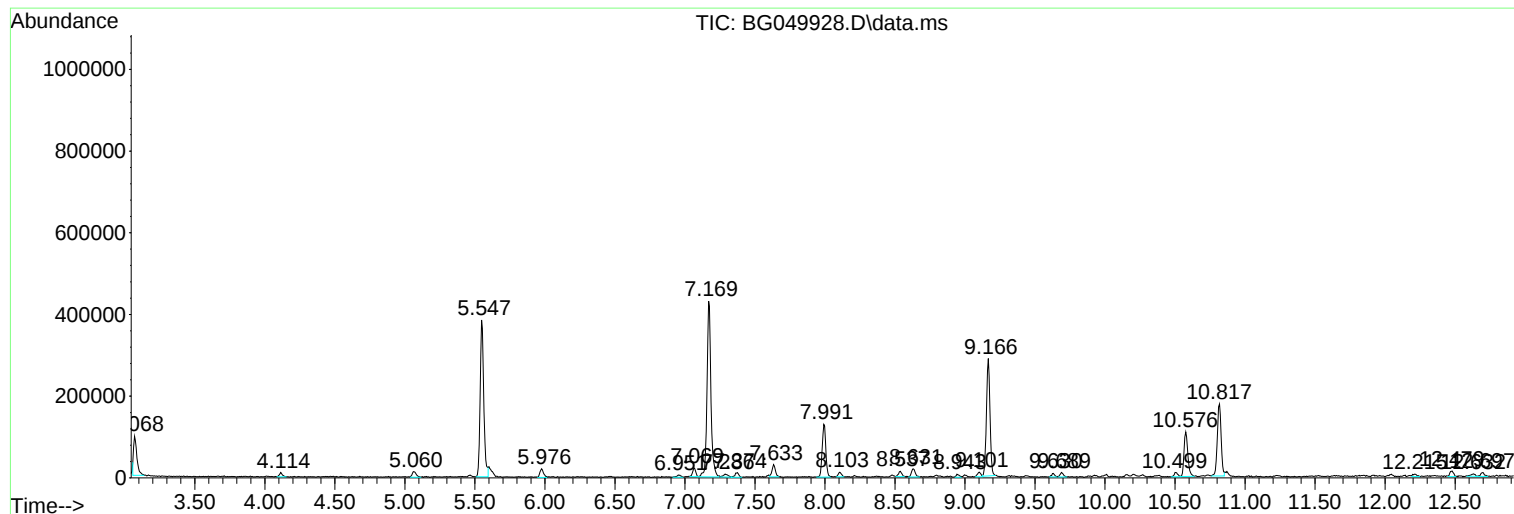

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049928.D
Acq On : 21 Aug 2021 3:40
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049928.D
Acq On : 21 Aug 2021 3:40
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-09-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------