


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049913.D
 Acq On : 20 Aug 2021 17:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 23 16:13:24 2021

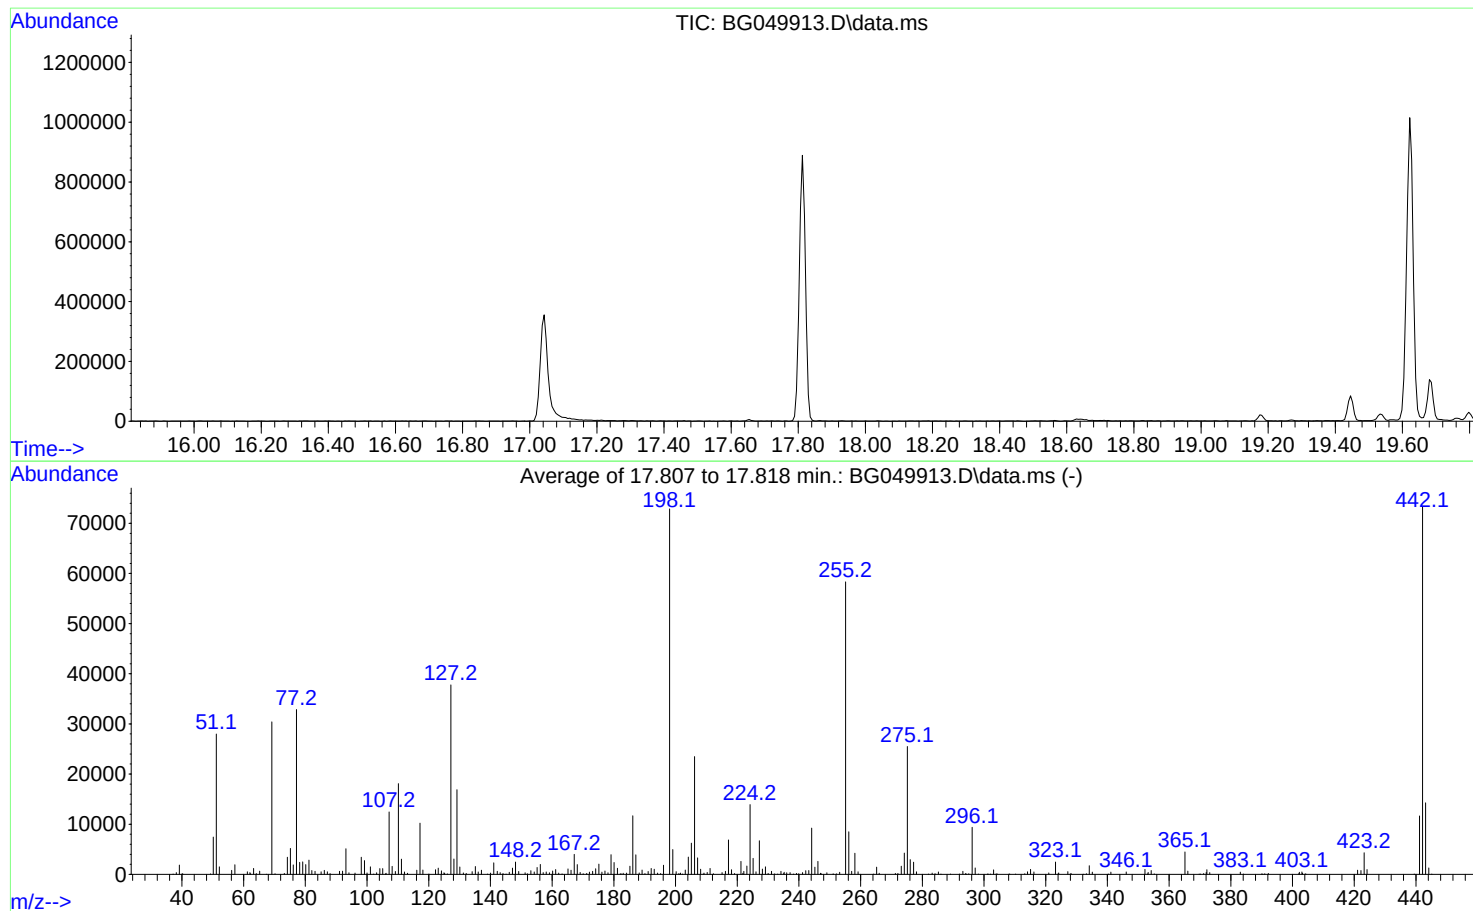

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	27979	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.7	30400	PASS
70	69	0.00	2	0.4	125	PASS
127	198	10	80	51.9	37784	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72867	PASS
199	198	5	9	6.8	4939	PASS
275	198	10	60	35.0	25496	PASS
365	198	1	100	6.1	4479	PASS
441	198	0.01	100	16.0	11645	PASS
442	442	50	100	100.0	73349	PASS
443	442	15	24	19.5	14273	PASS

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/21/2021	BNA_G	<u>BG049913.D</u>
Compound Name	Response	Retention Time
DDT	290911	20.849
DDD	8772	20.49
DDE	610	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9382	300293	3.12

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049913.D
Acq On : 20 Aug 2021 17:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 20 17:57:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

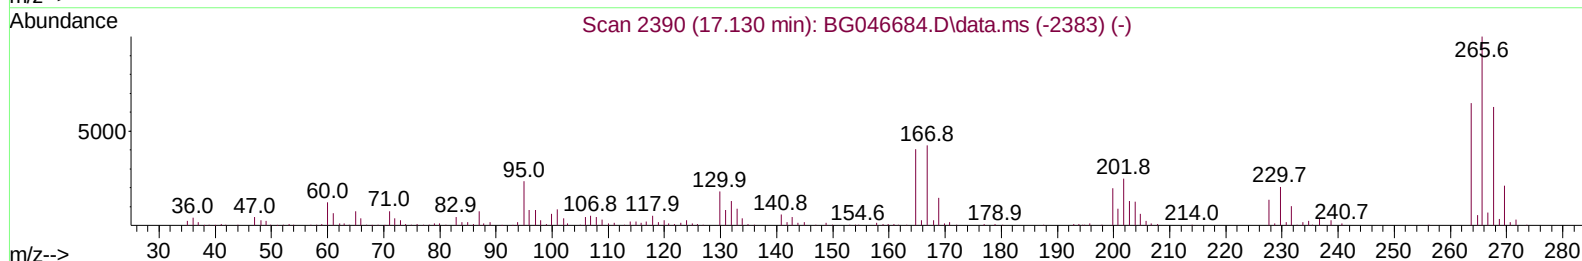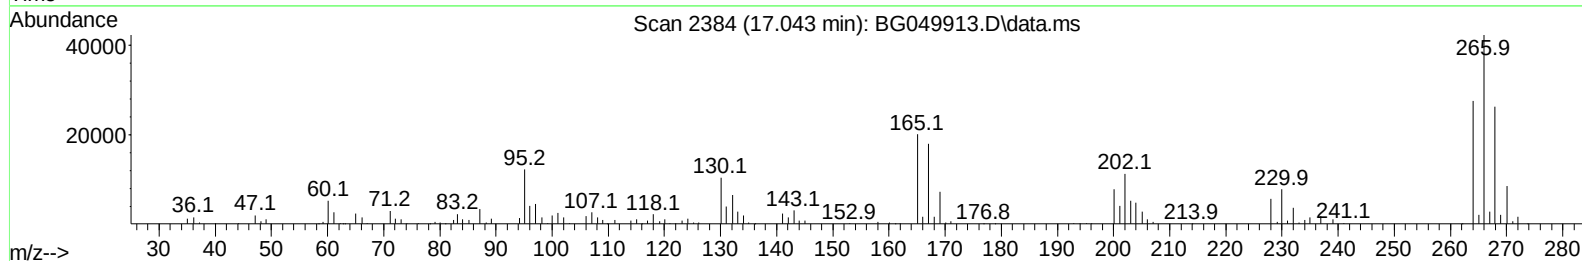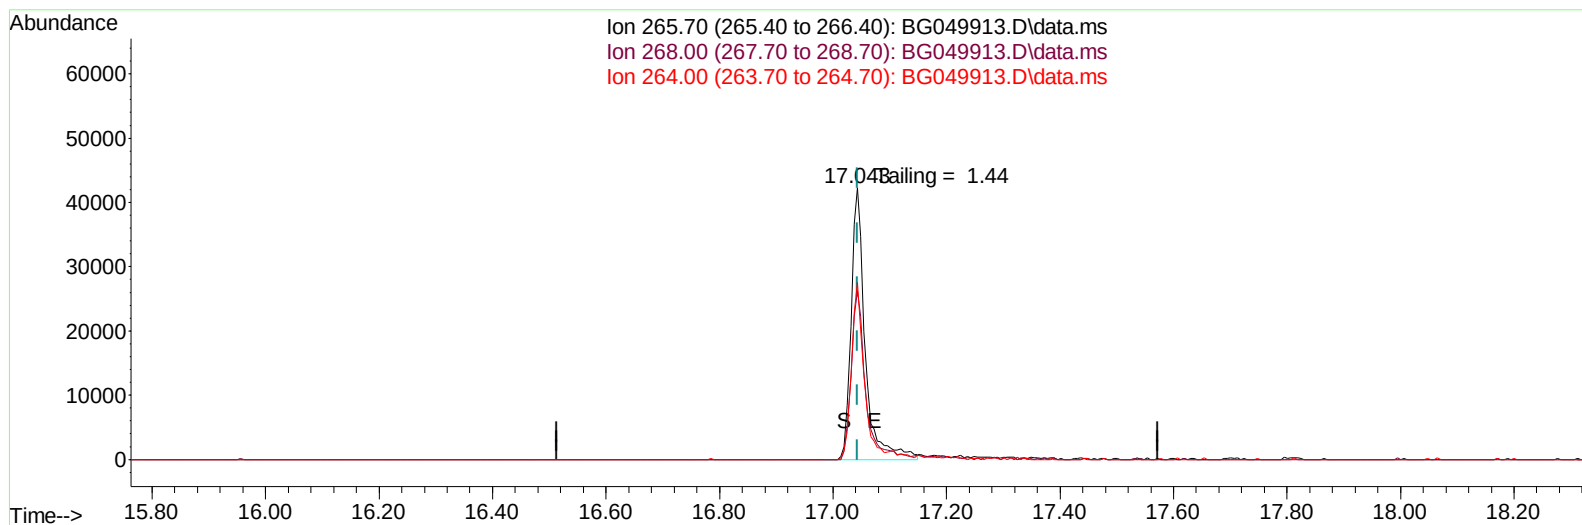

TIC: BG049913.D\data.ms

(70) Pentachlorophenol (C)

17.043min (0.000) 20776.74 ng




response 74025

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.12
264.00	61.60	65.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049913.D
Acq On : 20 Aug 2021 17:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 20 17:57:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

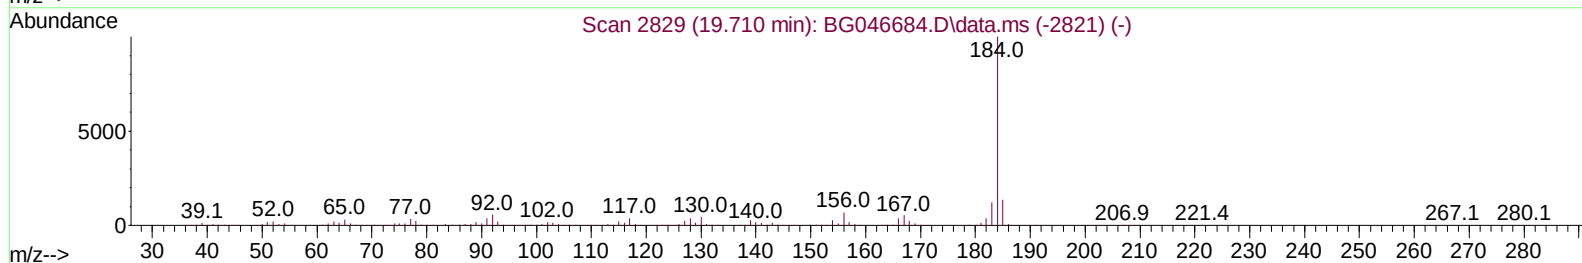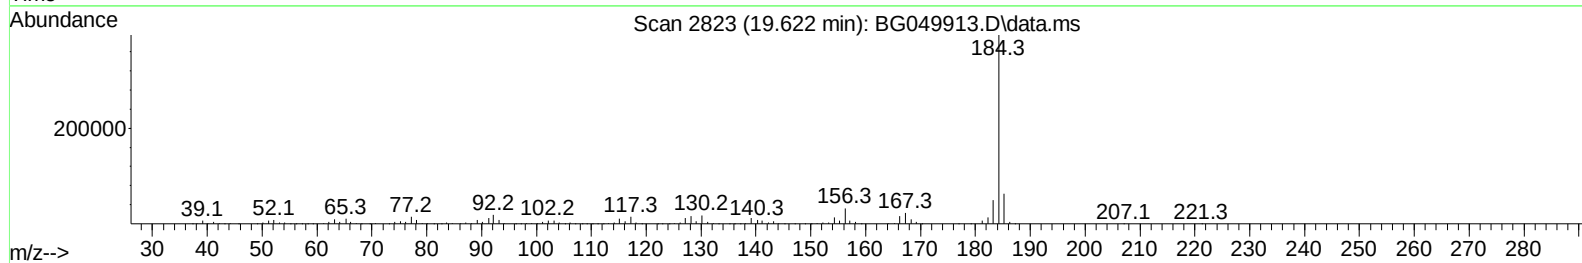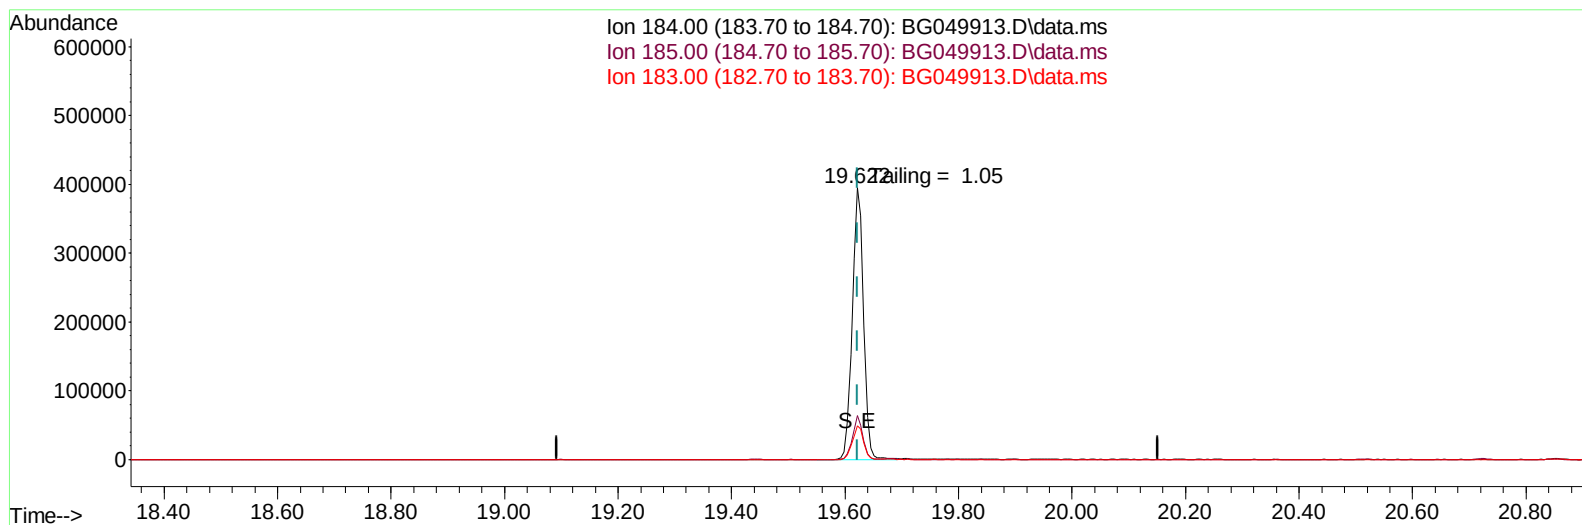

TIC: BG049913.D\data.ms

(77) Benzidine

19.622min (0.000) 300820.32 ng

response 547101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.12
183.00	13.20	12.47
0.00	0.00	0.00