
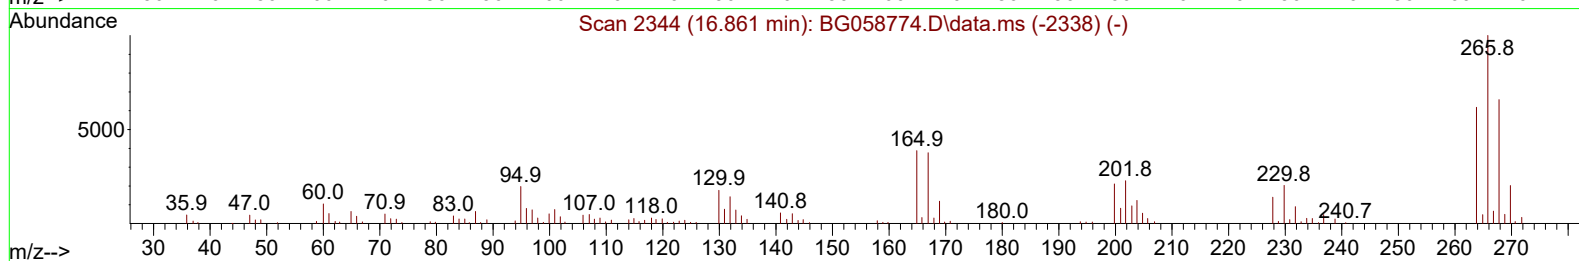
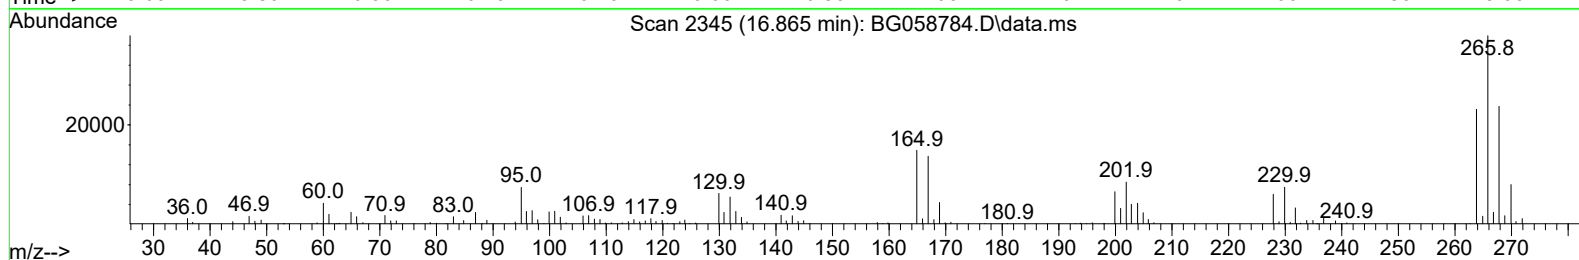


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082123\
Data File : BG058784.D
Acq On : 21 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 08:54:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

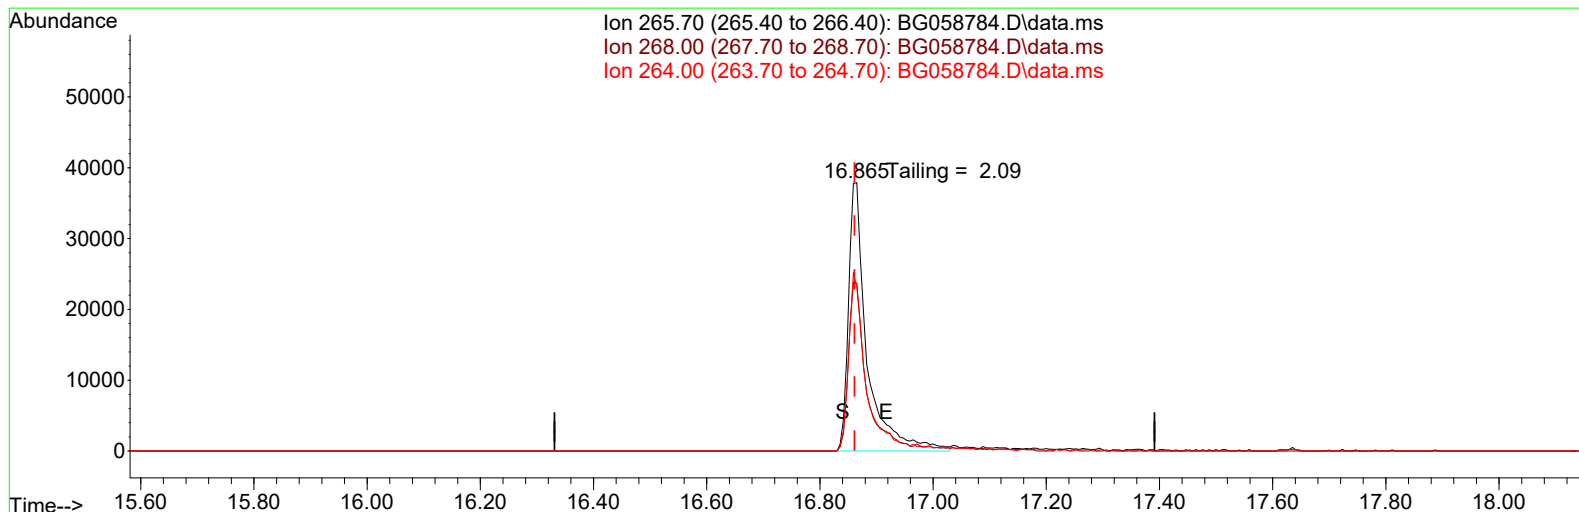

TIC: BG058784.D\data.ms

(70) Pentachlorophenol (C)




16.865min (+ 0.004) 21279.55 ng

response 86582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.59
264.00	61.90	61.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082123\
Data File : BG058784.D
Acq On : 21 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 08:54:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

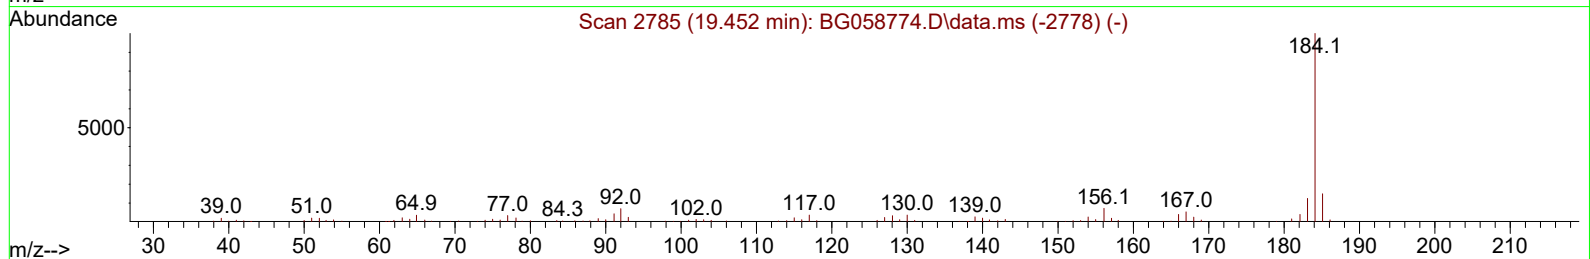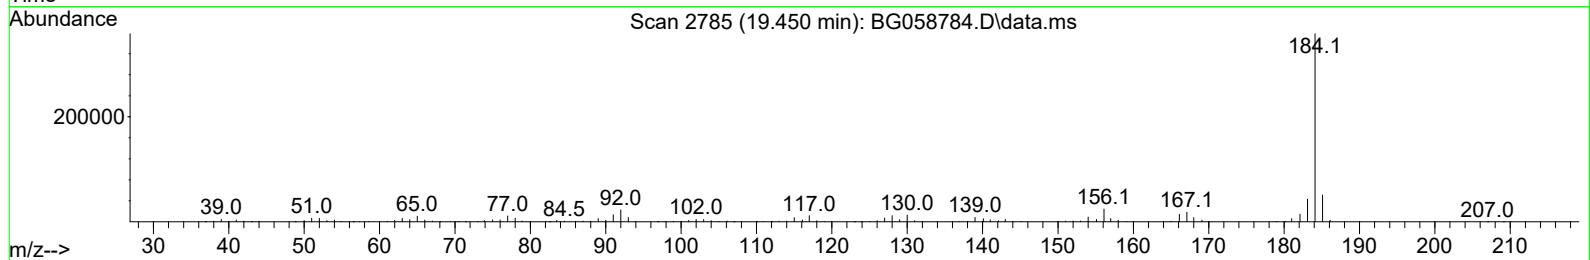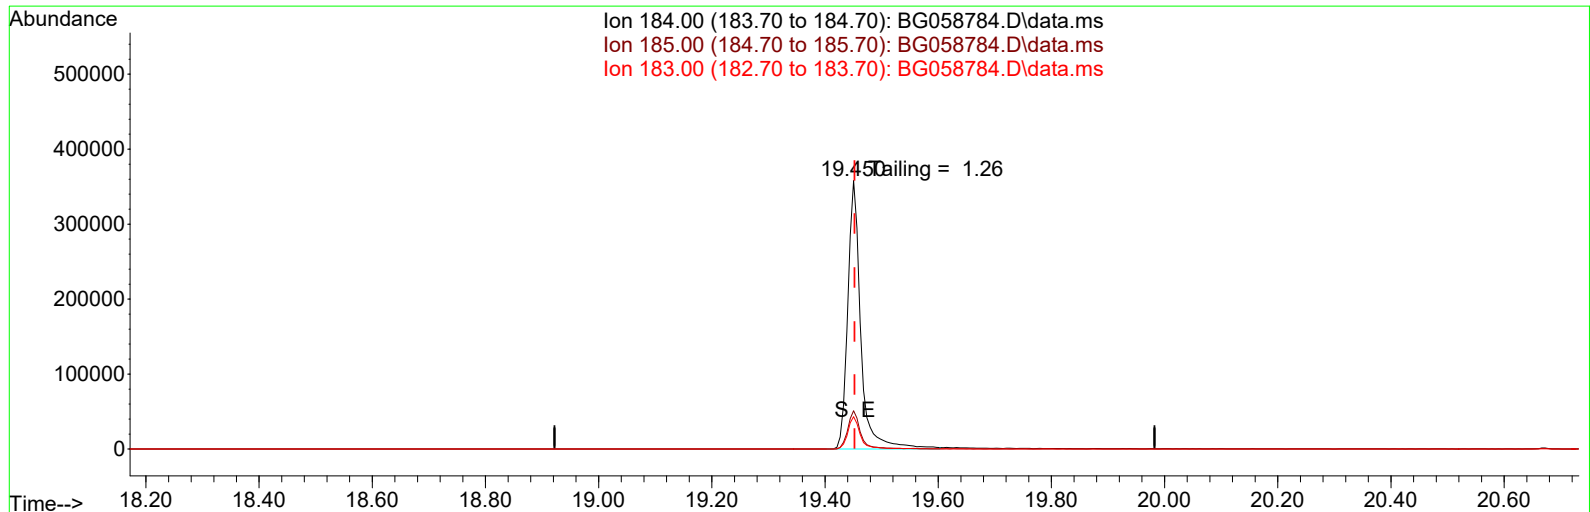

TIC: BG058784.D\data.ms

(77) Benzidine

19.450min (-0.002) 0.00 ng

response 575284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	12.50	12.04
0.00	0.00	0.00