


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082123\
Data File : BG058784.D
Acq On : 21 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 21 01:40:57 2023

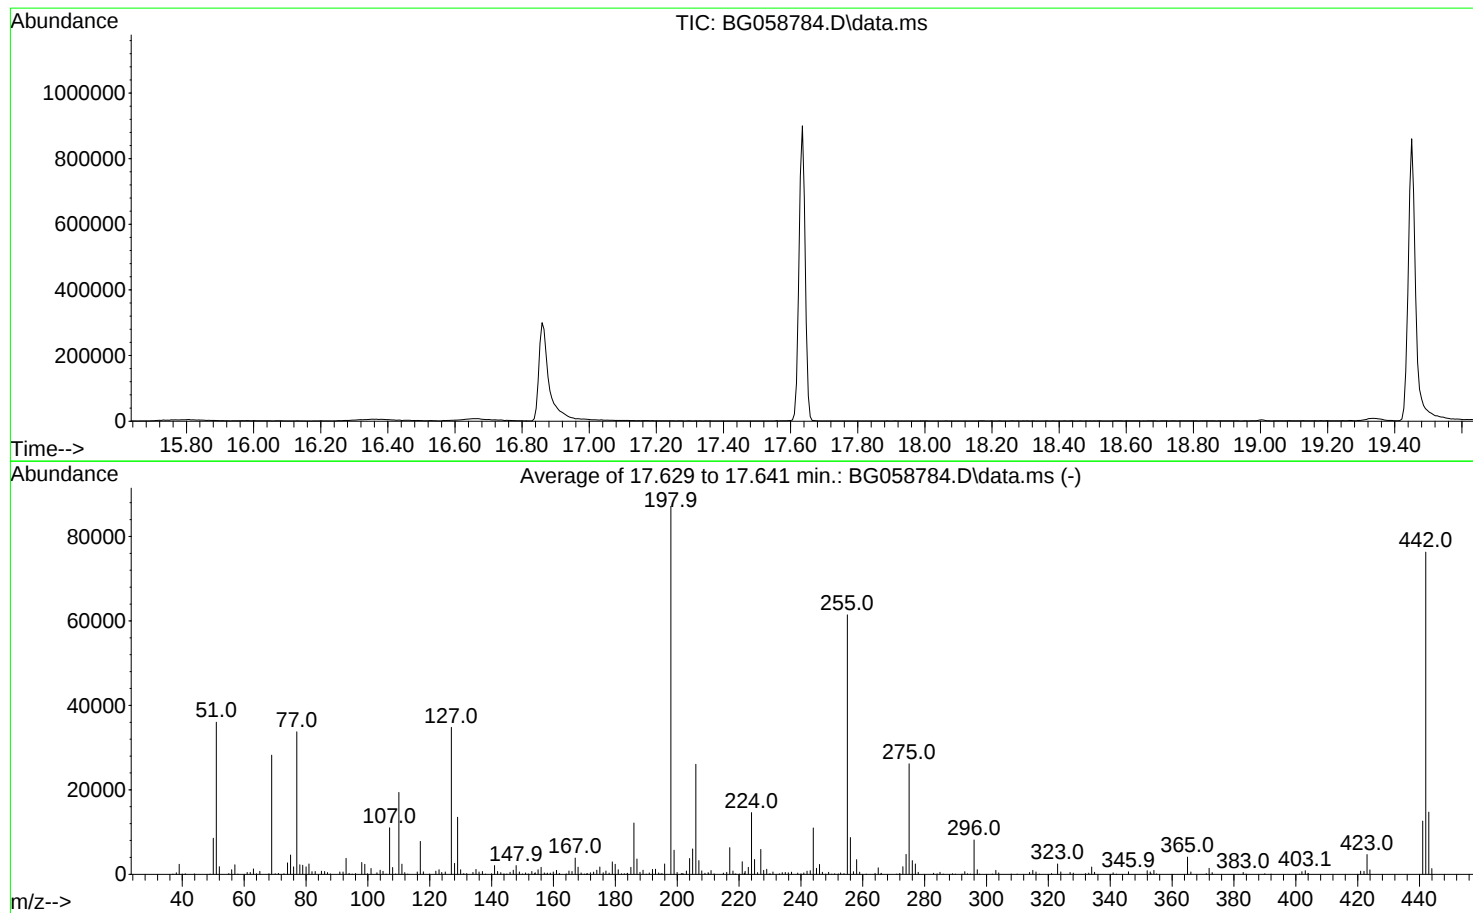




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	36029	PASS
68	69	0.00	2	0.4	117	PASS
69	198	0.00	100	32.4	28227	PASS
70	69	0.00	2	0.5	153	PASS
127	198	10	80	40.0	34824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87120	PASS
199	198	5	9	6.6	5710	PASS
275	198	10	60	30.0	26176	PASS
365	198	1	100	4.7	4094	PASS
441	198	0.01	100	14.5	12604	PASS
442	442	50	100	100.0	76288	PASS
443	442	15	24	19.3	14726	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082123\
Data File : BG058784.D
Acq On : 21 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 21 08:54:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

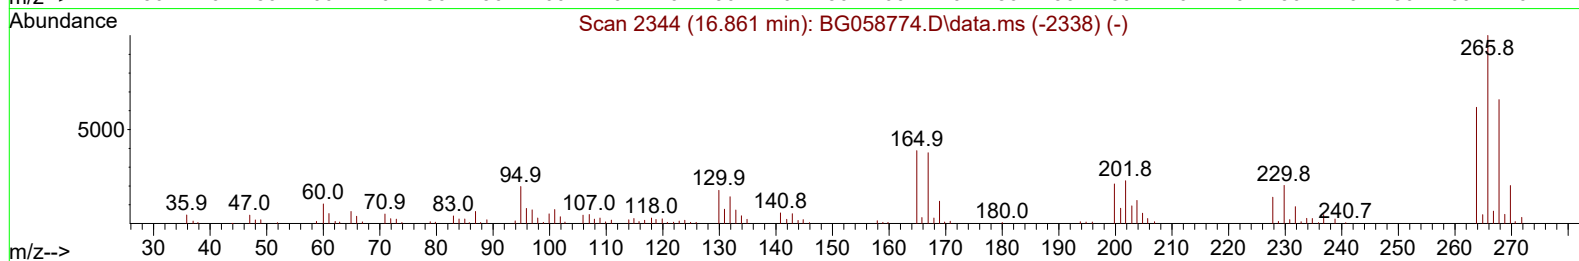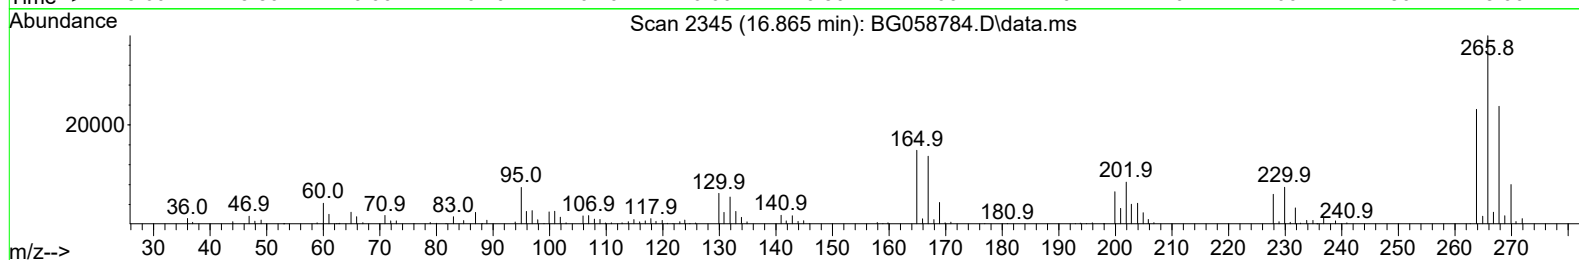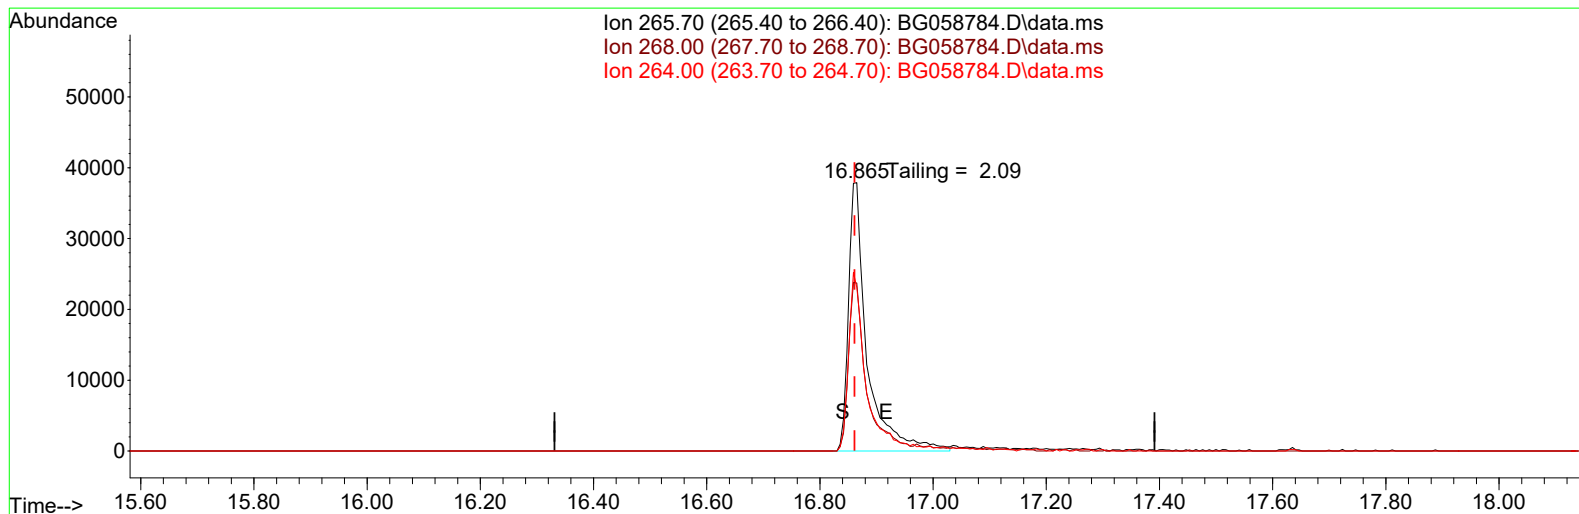

TIC: BG058784.D\data.ms

(70) Pentachlorophenol (C)

16.865min (+ 0.004) 21279.55 ng




response 86582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.59
264.00	61.90	61.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082123\
Data File : BG058784.D
Acq On : 21 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 21 08:54:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

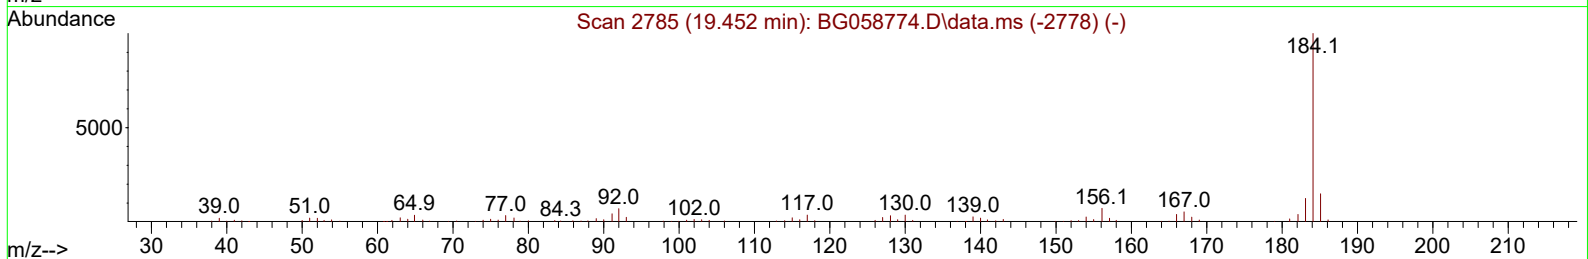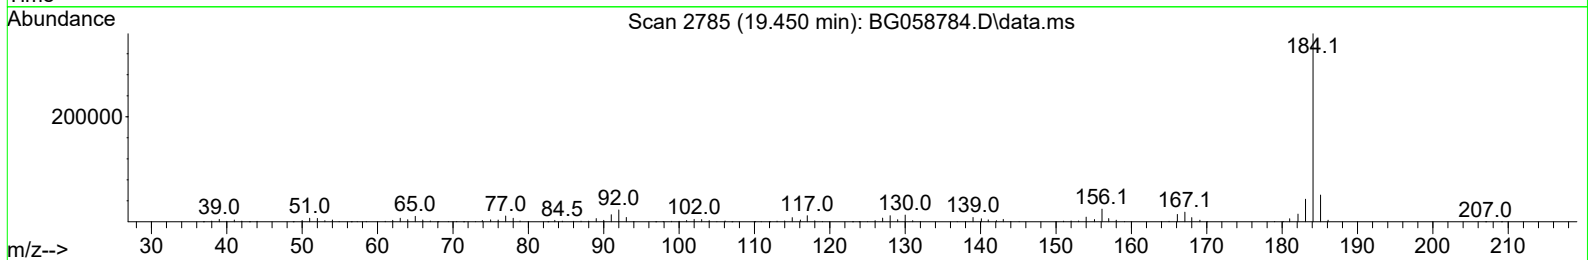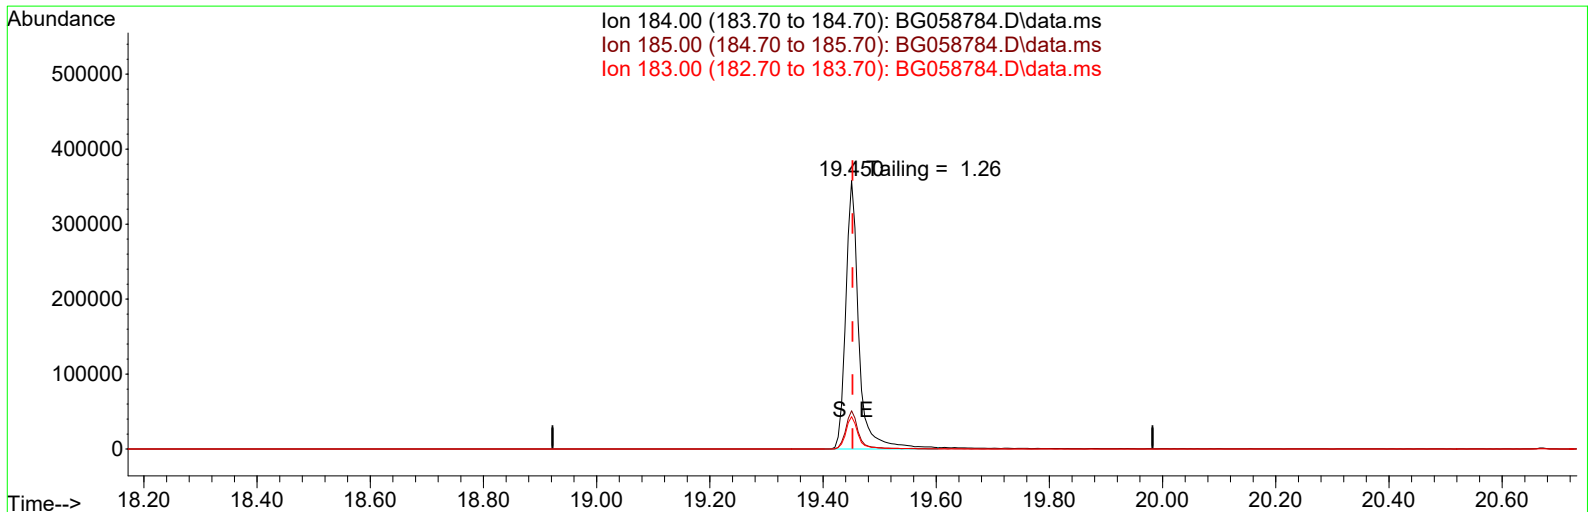

TIC: BG058784.D\data.ms

(77) Benzidine

19.450min (-0.002) 0.00 ng

response 575284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	12.50	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/21/2023	BNA_G	<u>BG058784.D</u>
Compound Name	Response	Retention Time
DDT	296602	20.672
DDD	6819	20.238
DDE	556	19.738
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7375	303977	2.43

Instrument :
BNA_G
ClientSampleId :
DFTPP