


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082223\
Data File : BG058800.D
Acq On : 22 Aug 2023 8:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 21 01:40:57 2023

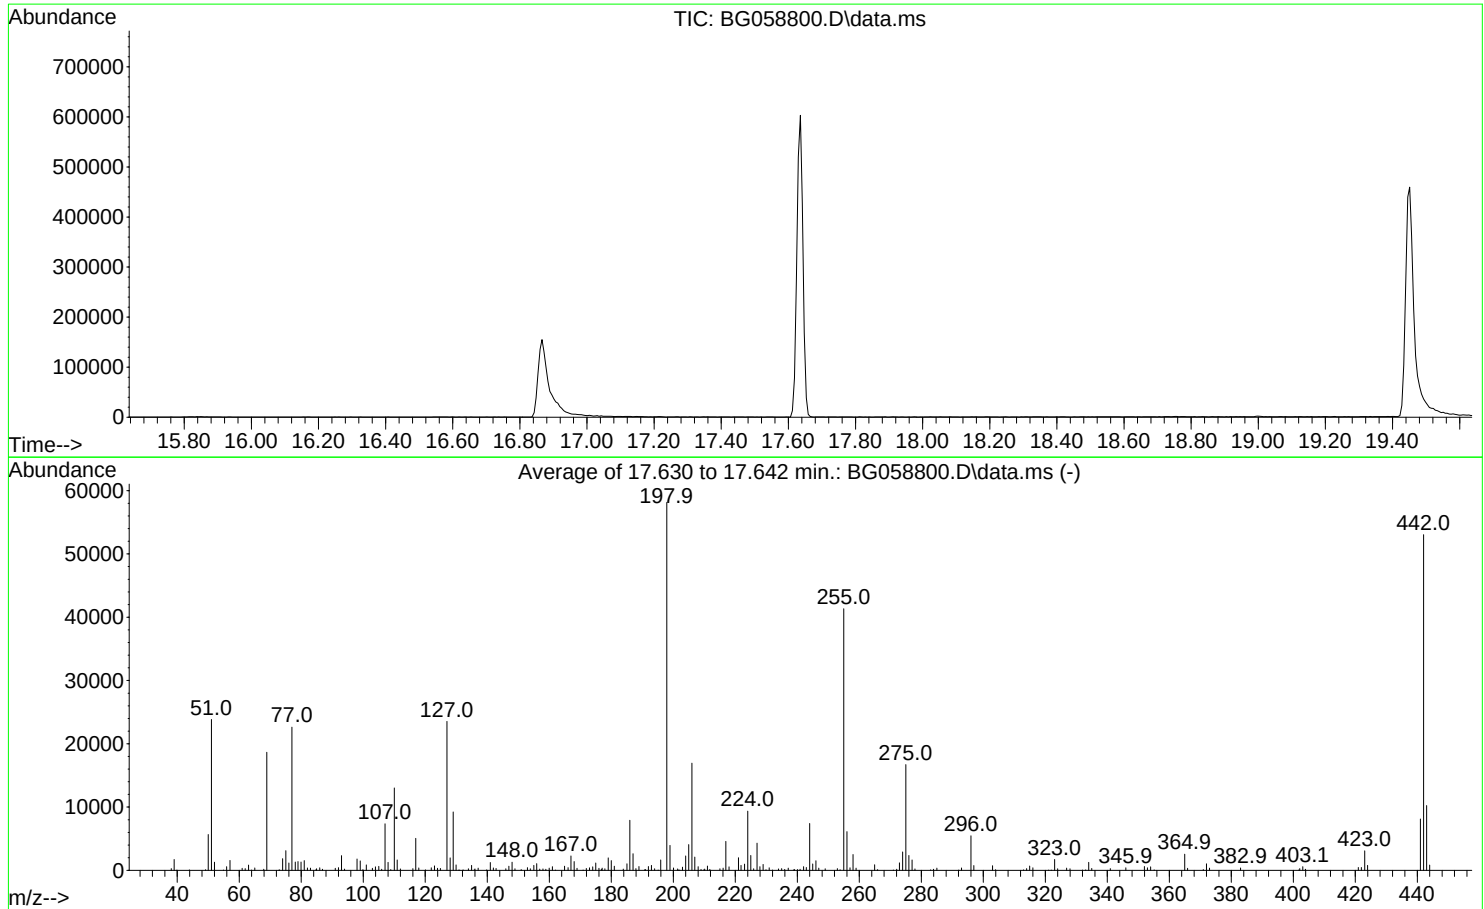




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	23849	PASS
68	69	0.00	2	1.0	187	PASS
69	198	0.00	100	32.1	18669	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.5	23531	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58125	PASS
199	198	5	9	6.8	3950	PASS
275	198	10	60	28.8	16720	PASS
365	198	1	100	4.4	2549	PASS
441	198	0.01	100	14.0	8116	PASS
442	442	50	100	100.0	53048	PASS
443	442	15	24	19.3	10242	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082223\
Data File : BG058800.D
Acq On : 22 Aug 2023 8:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:26:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

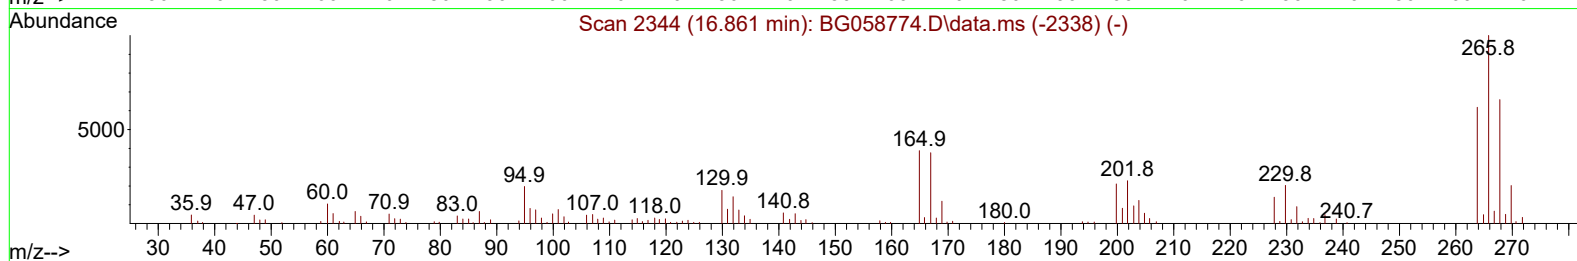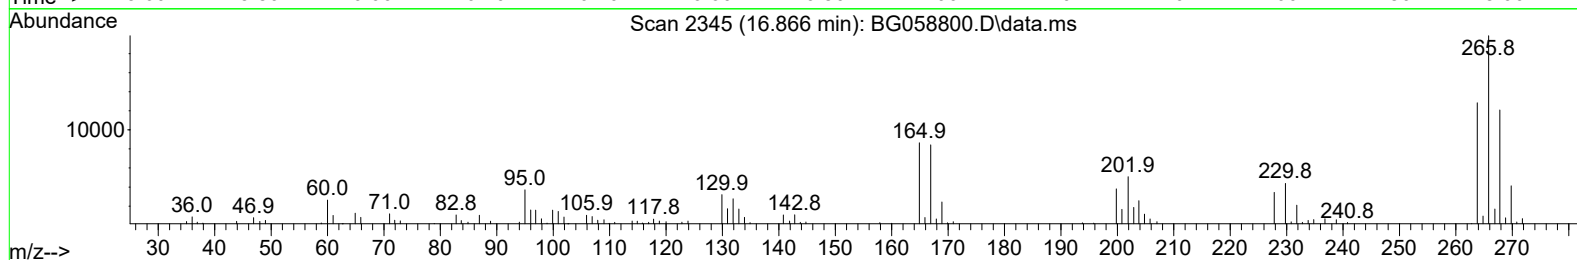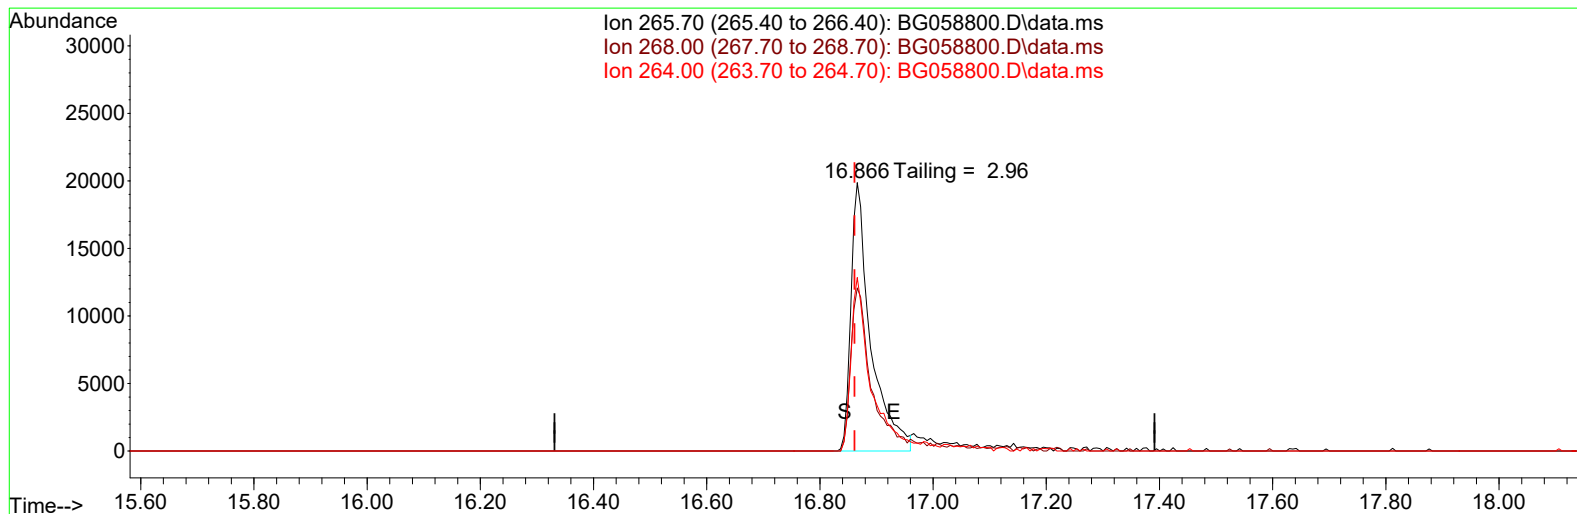

TIC: BG058800.D\data.ms

(70) Pentachlorophenol (C)

16.866min (+ 0.005) 26025.88 ng




response 48031

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	60.79
264.00	61.90	64.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082223\
Data File : BG058800.D
Acq On : 22 Aug 2023 8:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:26:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

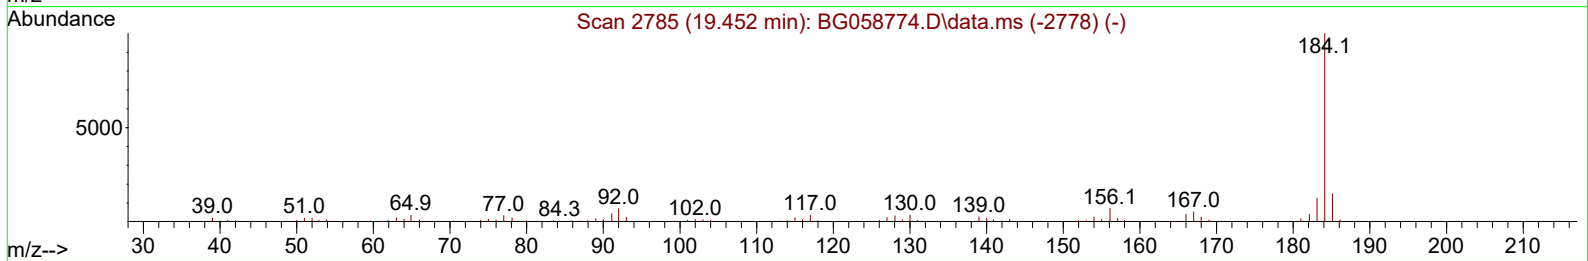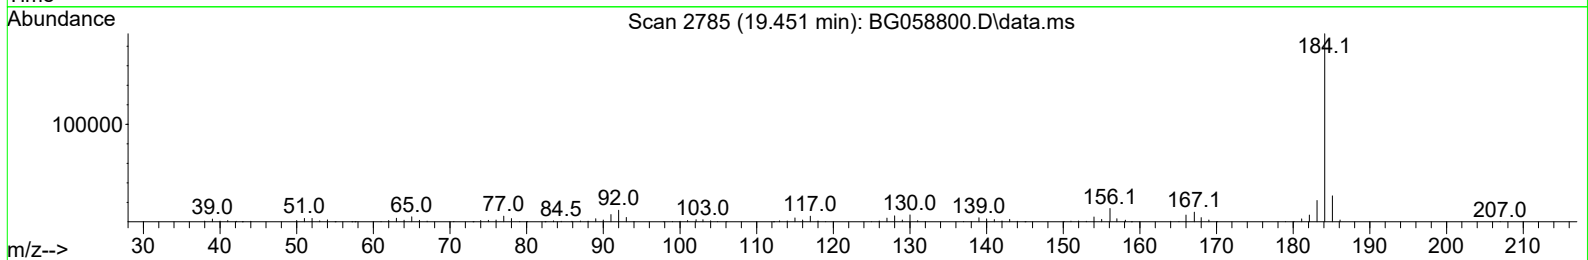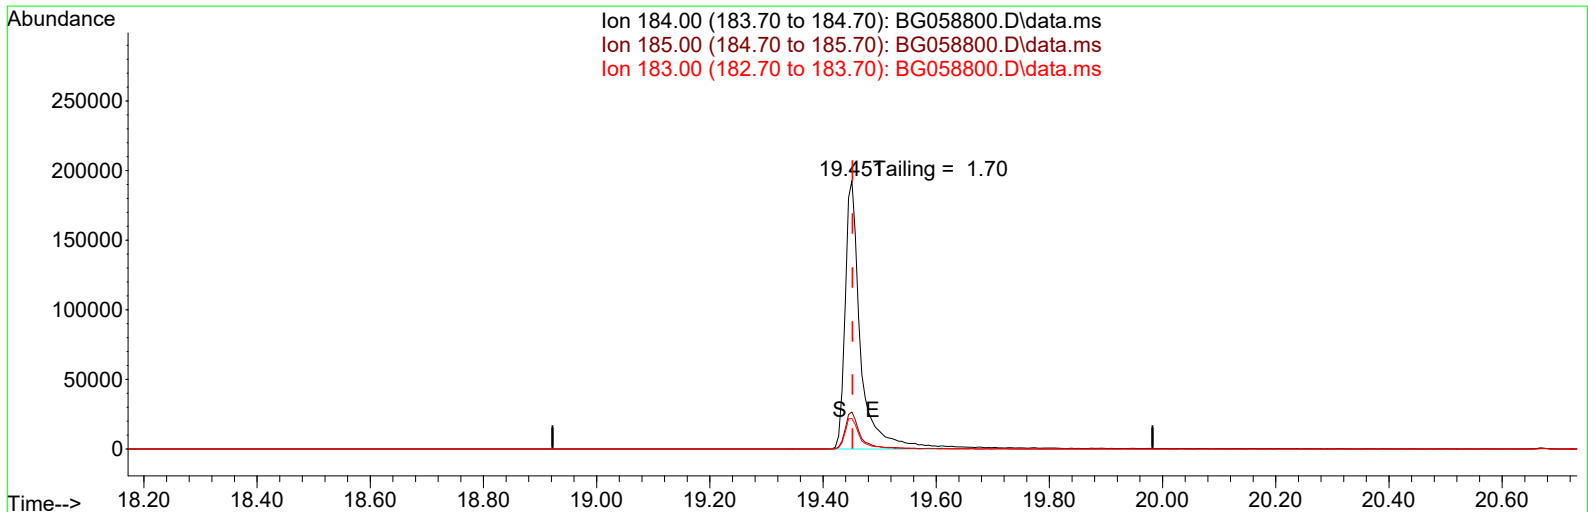

TIC: BG058800.D\data.ms

(77) Benzidine

19.451min (-0.001) 0.00 ng

response 364600

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.85
183.00	12.50	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/21/2023	BNA_G	<u>BG058800.D</u>
Compound Name	Response	Retention Time
DDT	190826	20.673
DDD	6597	20.238
DDE	864	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7461	198287	3.76

Instrument :
BNA_G
ClientSampleId :
DFTPP