
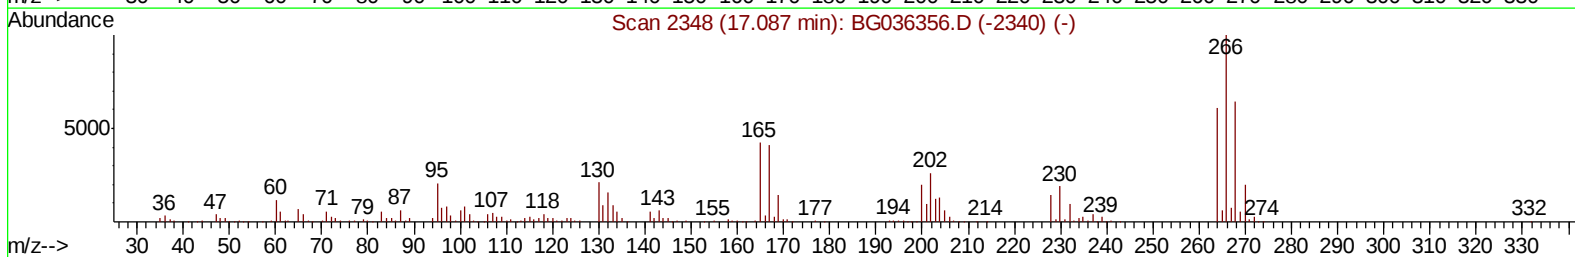
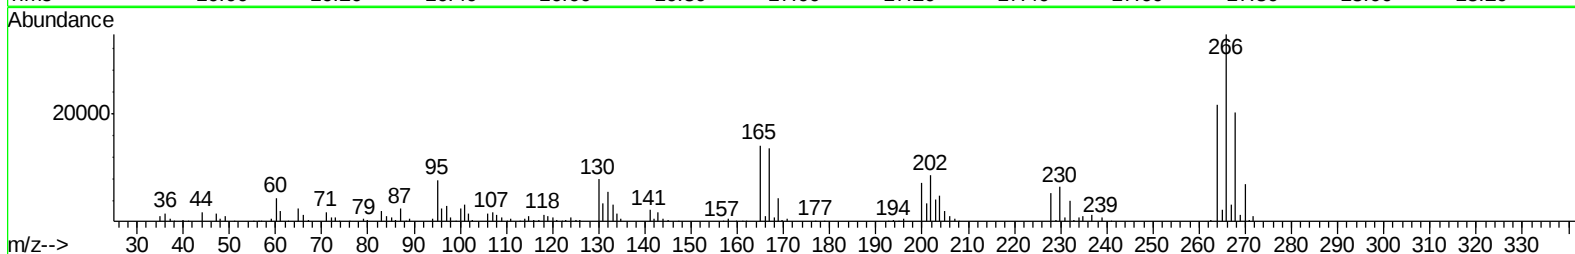


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082318\
Data File : BG036352.D
Acq On : 22 Aug 2018 21:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:19:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 08:52:32 2018
Response via : Initial Calibration

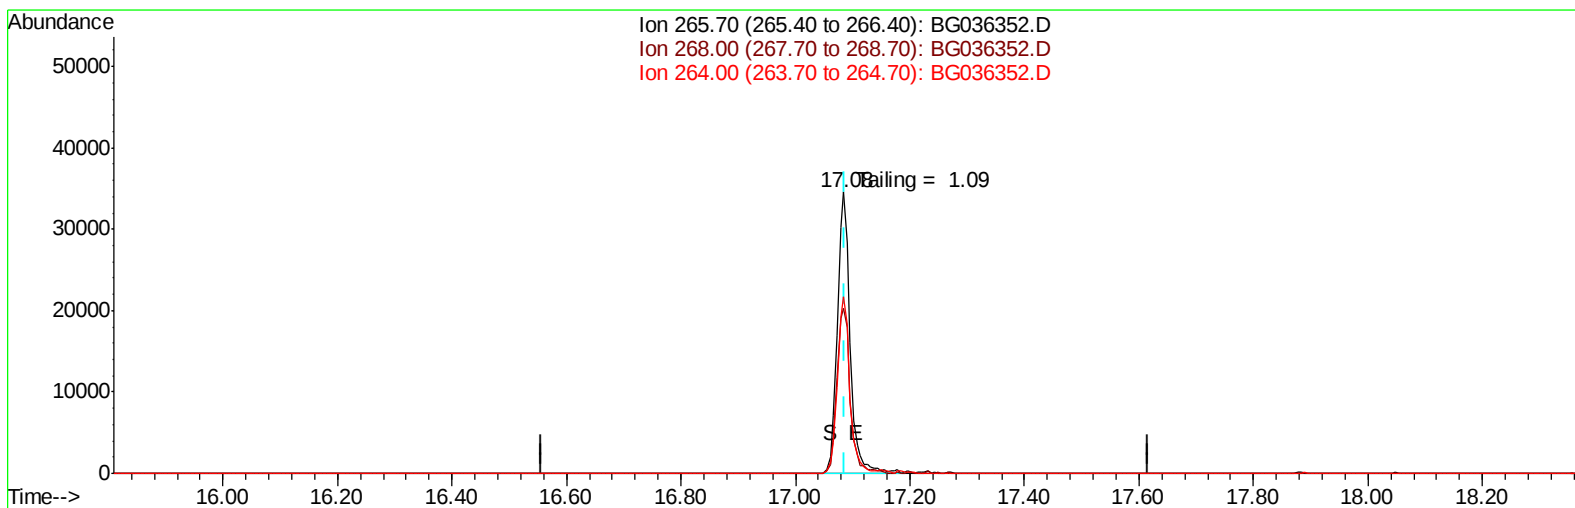

TIC: BG036352.D

(69) Pentachlorophenol (C)




17.084min (-0.003) 50706.93ng

response 54460

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	58.43
264.00	61.10	62.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082318\
 Data File : BG036352.D
 Acq On : 22 Aug 2018 21:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:19:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 08:52:32 2018
 Response via : Initial Calibration

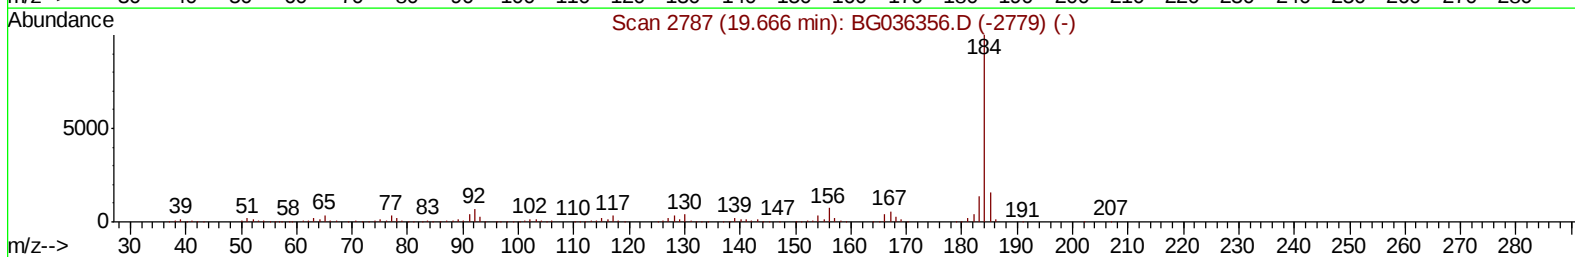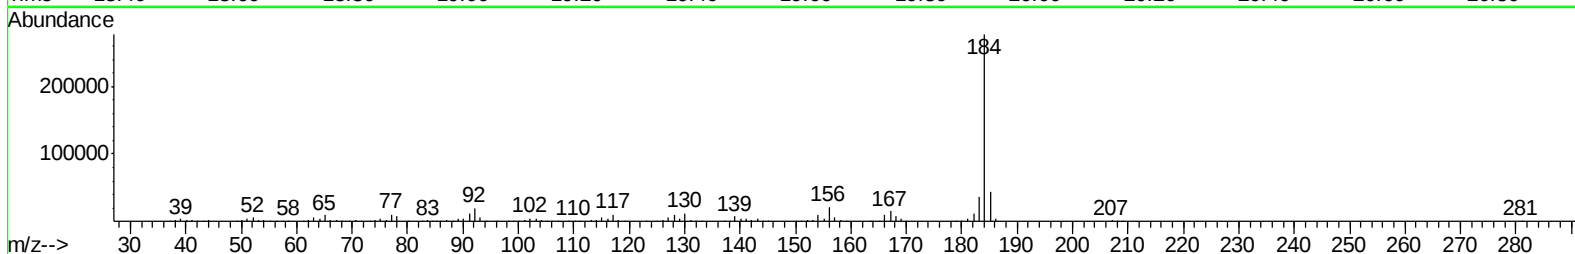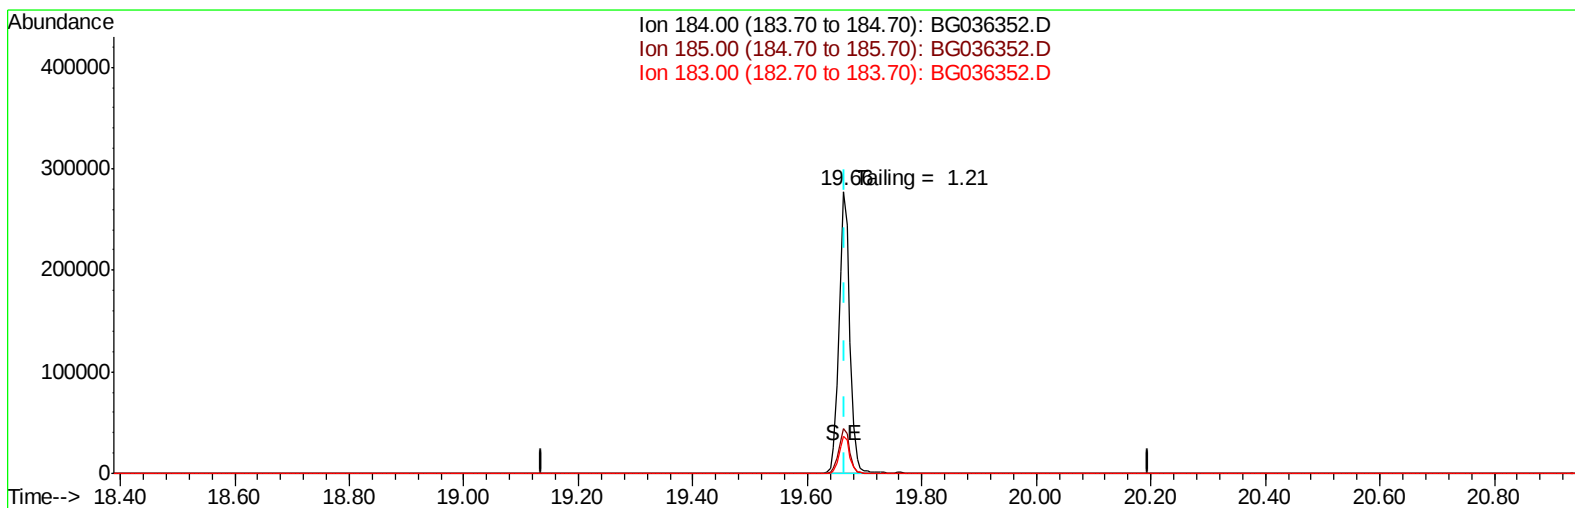

TIC: BG036352.D

(76) Benzidine

19.663min (-0.003) 0.00ng

response 369773

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.79
183.00	13.60	13.11
0.00	0.00	0.00