
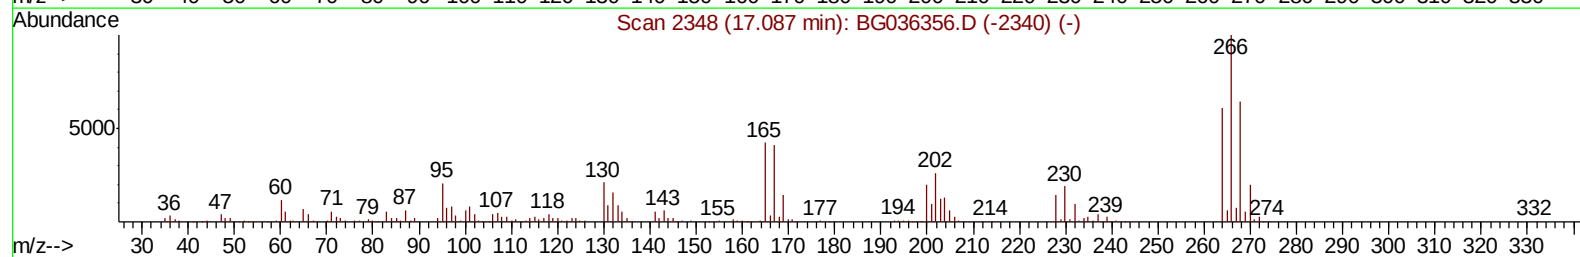
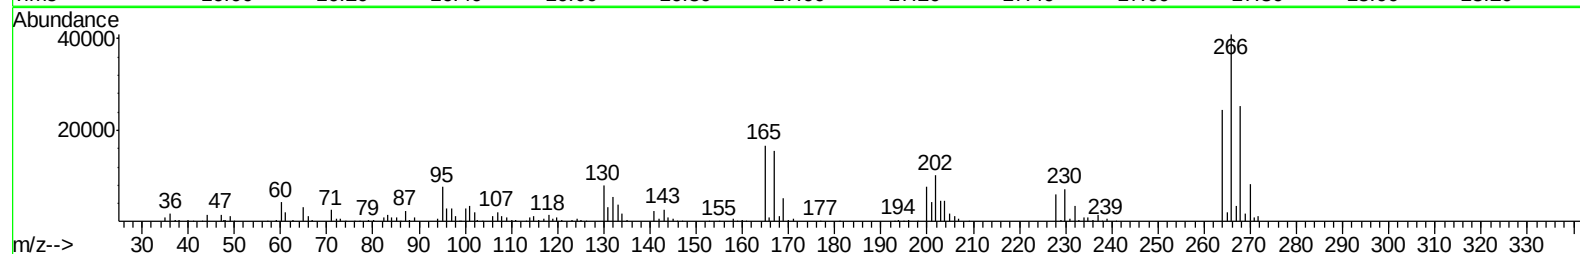


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082318\
Data File : BG036361.D
Acq On : 23 Aug 2018 3:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:21:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 08:52:32 2018
Response via : Initial Calibration

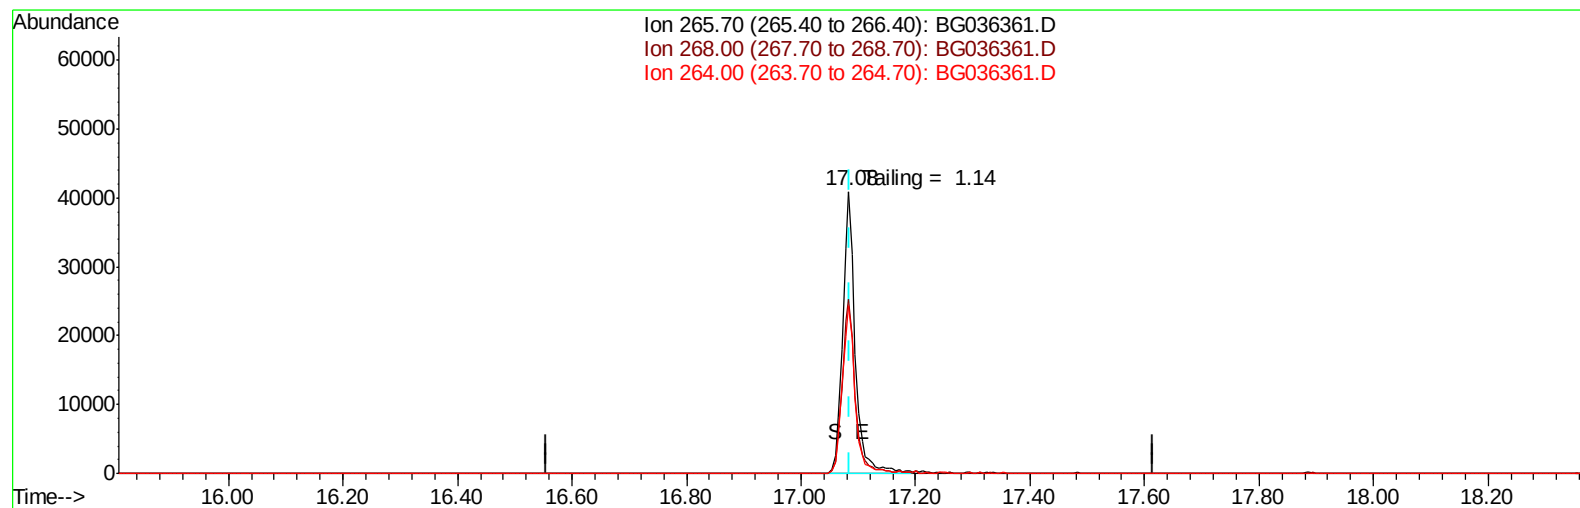

TIC: BG036361.D

(69) Pentachlorophenol (C)




17.083min (-0.003) 22780.15ng

response 62463

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.82
264.00	61.10	59.51
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082318\
 Data File : BG036361.D
 Acq On : 23 Aug 2018 3:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:21:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 08:52:32 2018
 Response via : Initial Calibration

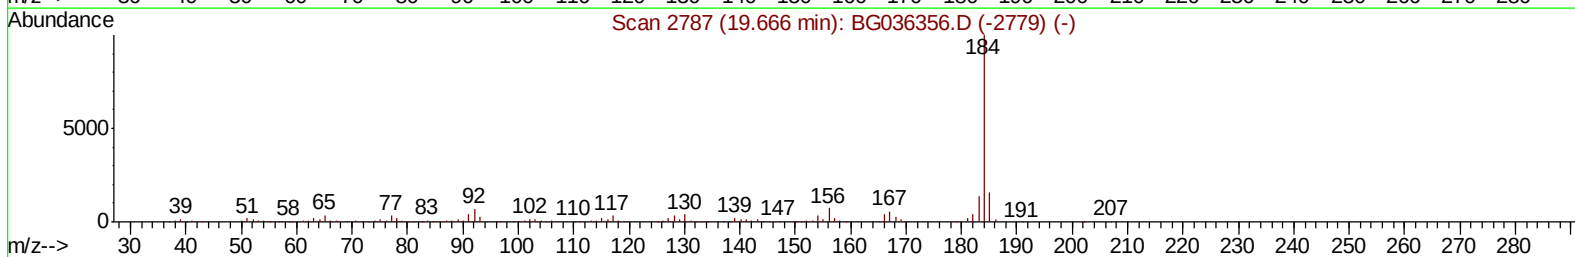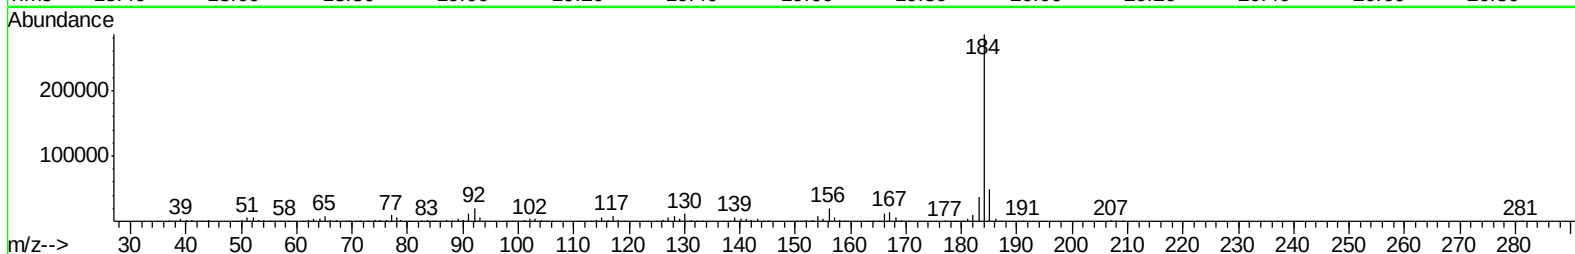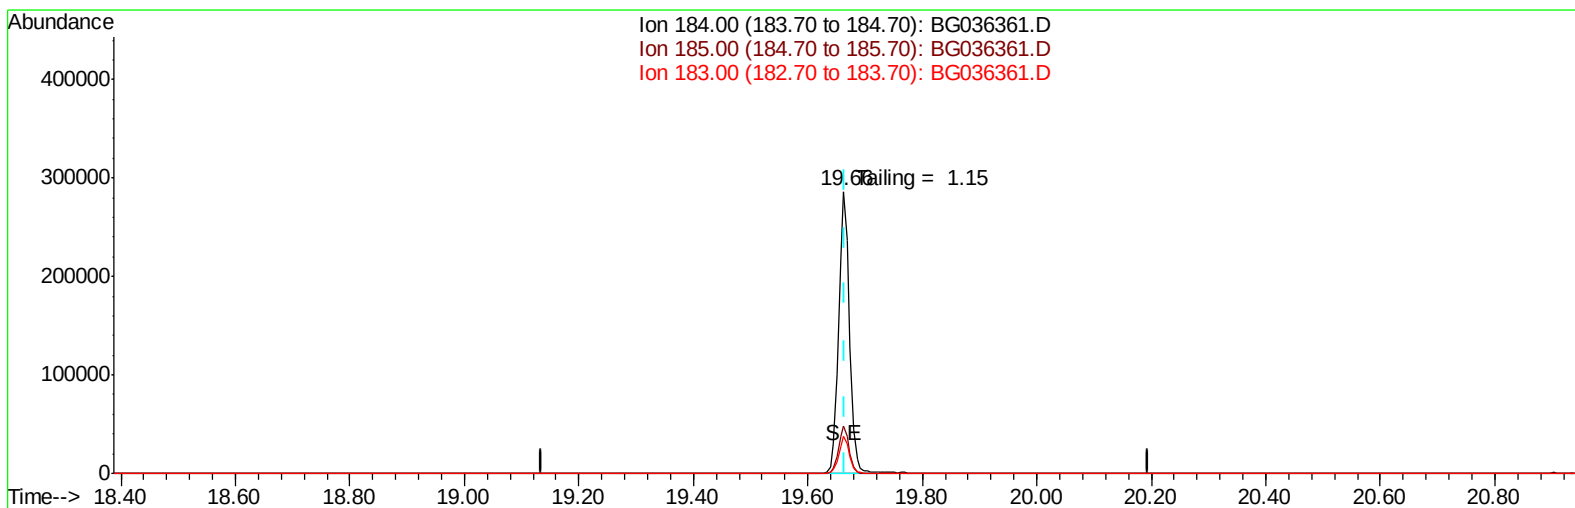

TIC: BG036361.D

(76) Benzidine

19.663min (-0.003) 0.00ng

response 383218

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.86
183.00	13.60	13.40
0.00	0.00	0.00