

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082318\
 Data File : BG036375.D
 Acq On : 23 Aug 2018 12:12
 Operator : JU/SJ
 Sample : J4540-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 081618-TIPC-E-U-M

Quant Time: Aug 23 12:54:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 12:07:02 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	47890	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	194667	20.00	ng	0.00
38) Acenaphthene-d10	14.69	164	125906	20.00	ng	0.00
63) Phenanthrene-d10	17.44	188	331896	20.00	ng	0.00
75) Chrysene-d12	21.70	240	378247	20.00	ng	0.00
86) Perylene-d12	24.93	264	378479	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	103752	34.37	ng	0.00
7) Phenol-d6	7.21	99	98183	22.71	ng	0.00
23) Nitrobenzene-d5	9.23	82	376260	104.87	ng	0.00
41) 2,4,6-Tribromophenol	16.18	330	64799	43.13	ng	0.00
44) 2-Fluorobiphenyl	13.32	172	890703	101.01	ng	0.00
78) Terphenyl-d14	20.05	244	1534793	94.84	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.14	163	38961	3.790	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082318\
Data File : BG036375.D
Acq On : 23 Aug 2018 12:12
Operator : JU/SJ
Sample : J4540-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
081618-TIPC-E-U-M

Quant Time: Aug 23 12:54:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

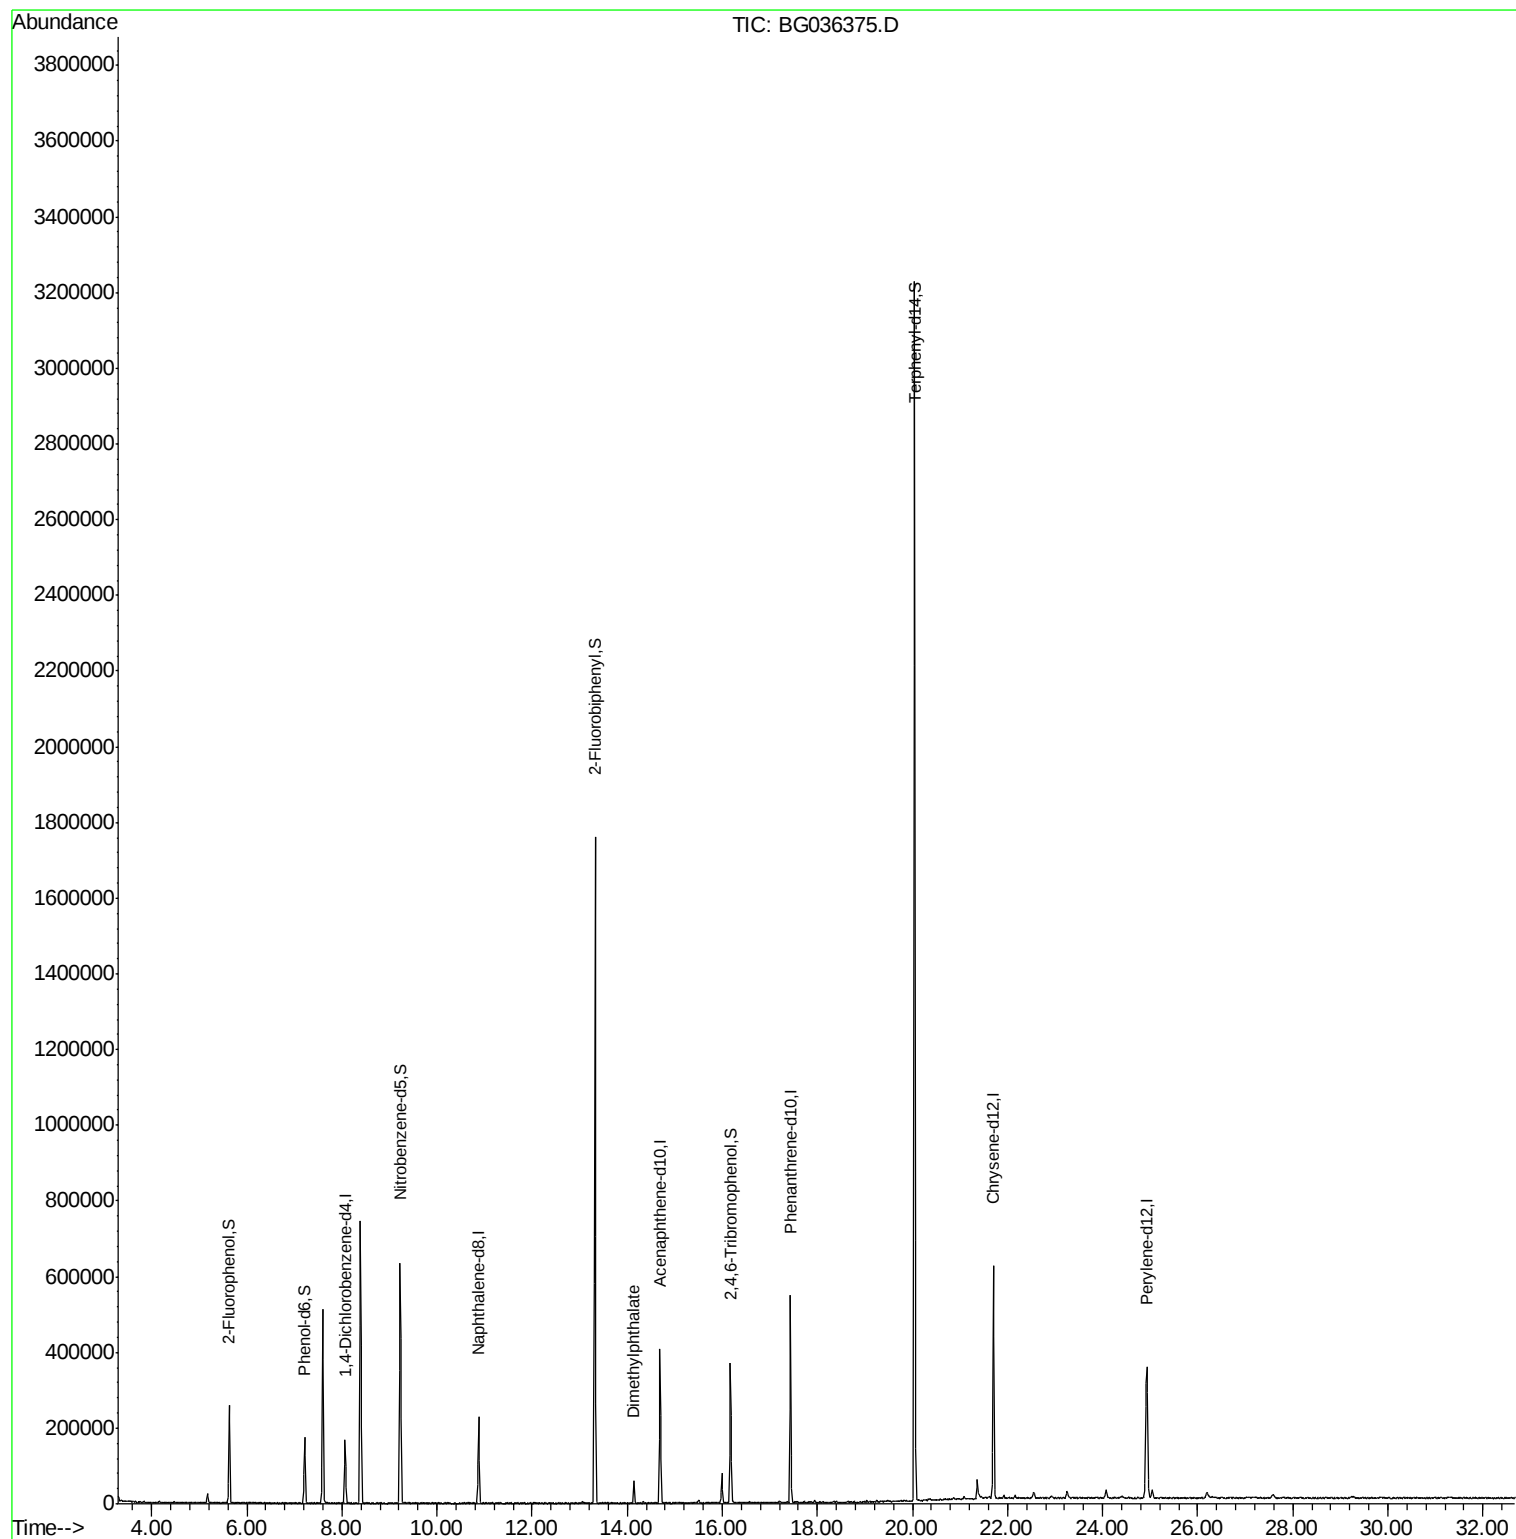




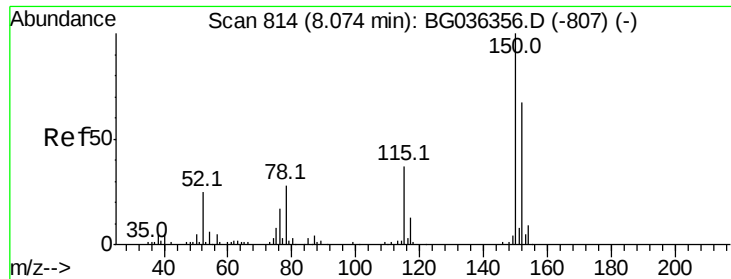


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 814
Delta R.T. -0.00 min
Lab File: BG036375.D
Acq: 23 Aug 2018 12:12

Instrument :
BNA_G
ClientSampleId :
081618-TIPC-E-U-M




Tot Ion:152 Resp: 47890
Ion Ratio Lower Upper
152 100
150 144.2 119.5 179.3
115 57.4 44.5 66.7

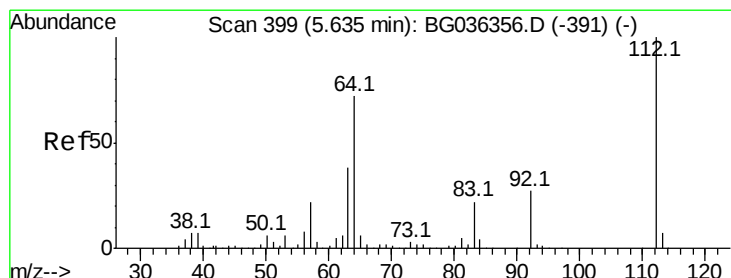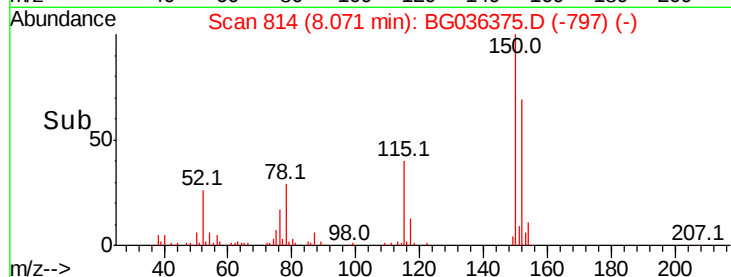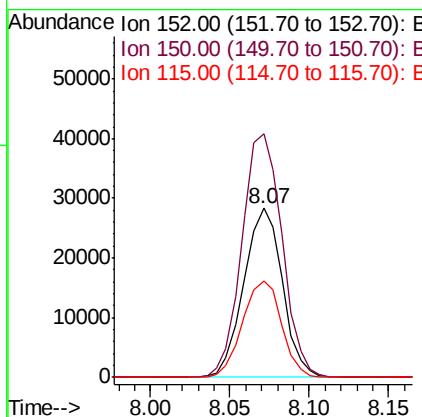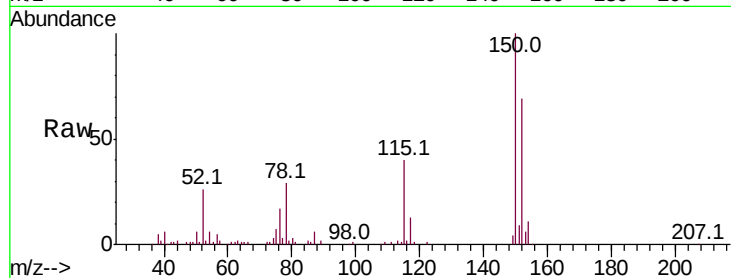

#5

2-Fluorophenol
Concen: 34.367 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.00 min
Lab File: BG036375.D
Acq: 23 Aug 2018 12:12

Tgt Ion:112 Resp: 103752
Ion Ratio Lower Upper
112 100
64 68.9 57.2 85.8
63 35.1 30.8 46.2

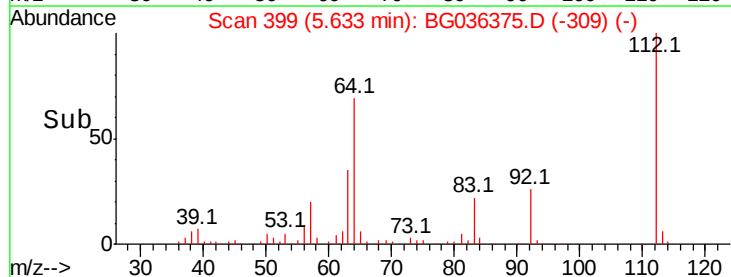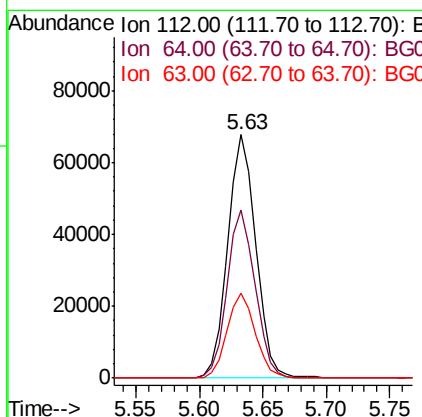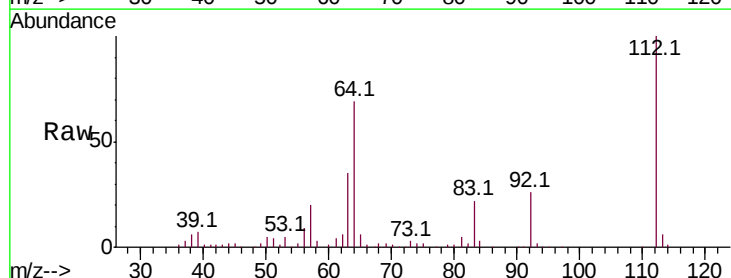



#7

Phenol-d6

Concen: 22.715 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG036375.D

Acq: 23 Aug 2018 12:12

Instrument :

BNA_G

ClientSampleId :

081618-TIPC-E-U-M


Tot Ion: 99 Resp: 98183

Ion Ratio Lower Upper



99 100

42 20.9 16.5 24.7

71 34.8 29.4 44.2

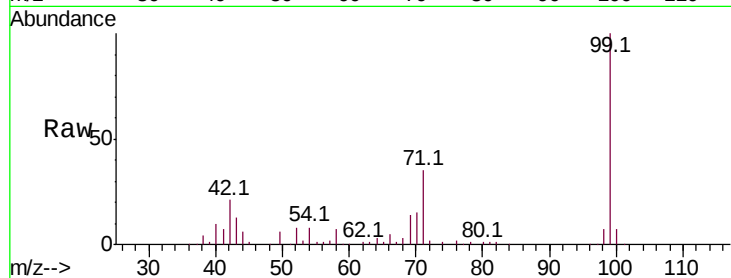

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

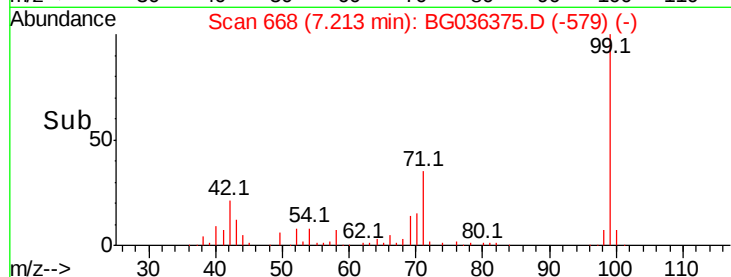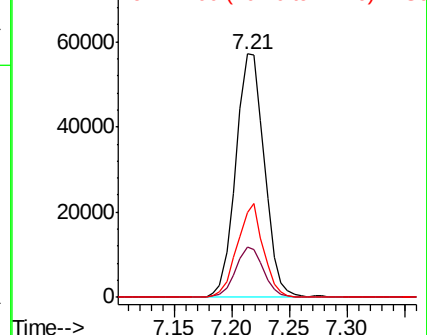

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.88 min Scan# 1292

Delta R.T. -0.00 min

Lab File: BG036375.D

Acq: 23 Aug 2018 12:12

Tgt Ion: 136 Resp: 194667


Ion Ratio Lower Upper

136 100



137 11.2 8.8 13.2


54 10.3 9.2 13.8

68 5.7 5.8 8.6#

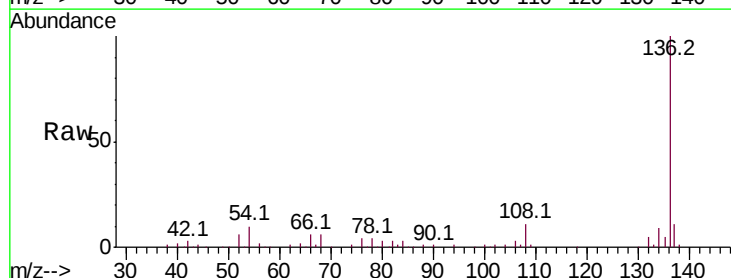

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



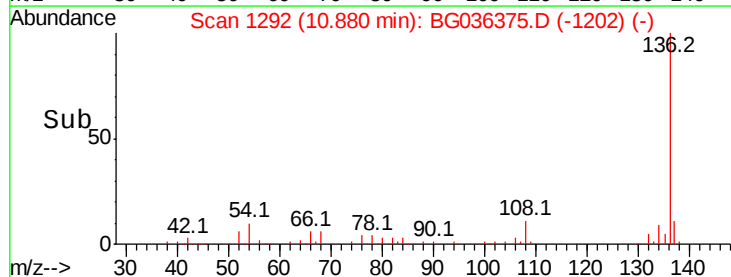
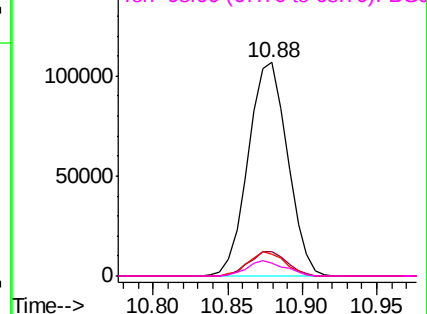


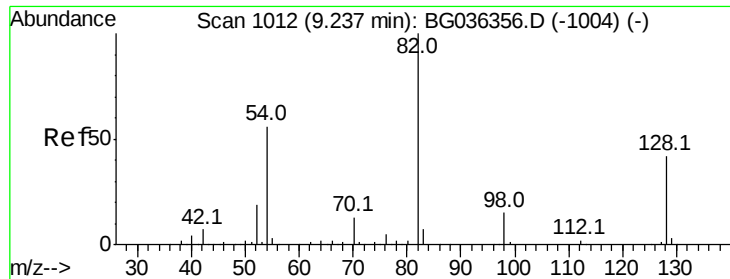

#23
 Nitrobenzene-d5
 Concen: 104.869 ng
 RT: 9.23 min Scan# 1011
 Delta R.T. -0.01 min
 Lab File: BG036375.D
 Acq: 23 Aug 2018 12:12




Instrument :
 BNA_G
 ClientSampleId :
 081618-TIPC-E-U-M

Tot Ion	Ratio	Lower	Upper
82	100		
128	41.3	33.3	49.9
54	57.7	45.1	67.7

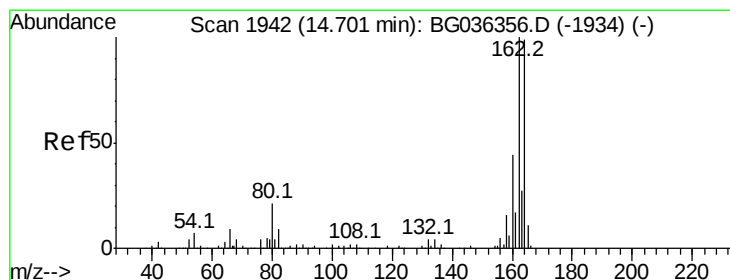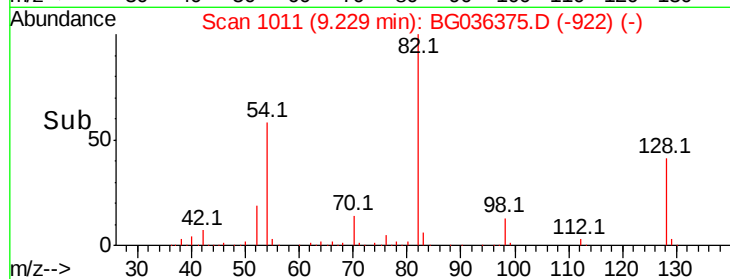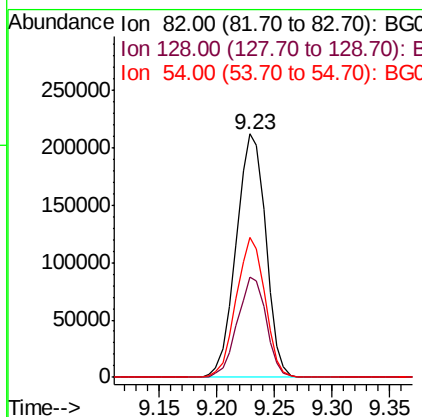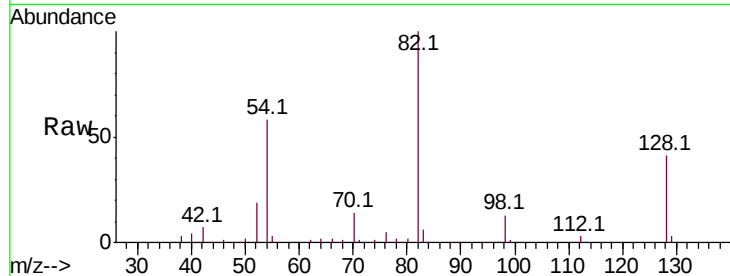

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.69 min Scan# 1941
 Delta R.T. -0.01 min
 Lab File: BG036375.D
 Acq: 23 Aug 2018 12:12

Tgt Ion	Ratio	Lower	Upper
164	100		
162	100.3	80.7	121.1
160	43.3	35.3	52.9

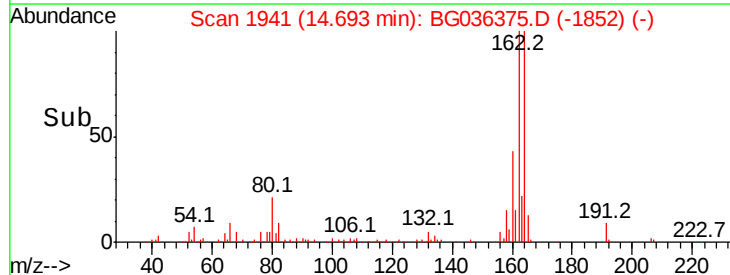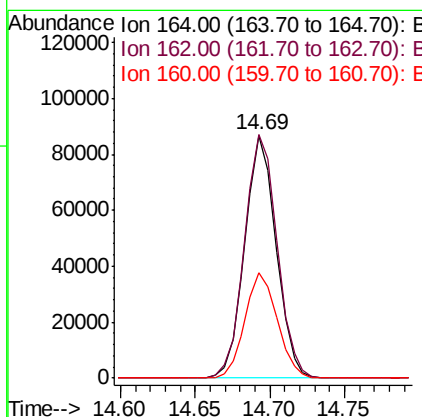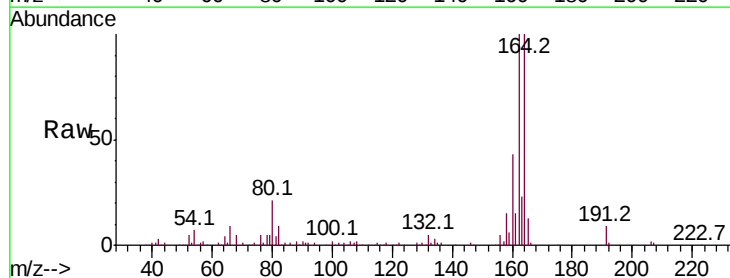




#41
 2,4,6-Tribromophenol
 Concen: 43.132 ng
 RT: 16.18 min Scan# 2194
 Delta R.T. -0.00 min
 Lab File: BG036375.D
 Acq: 23 Aug 2018 12:12

Instrument :
 BNA_G
 ClientSampleId :
 081618-TIPC-E-U-M

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.3	75.4	113.2
141	39.0	30.7	46.1



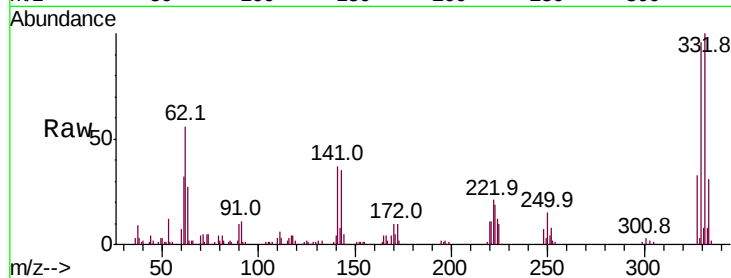


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

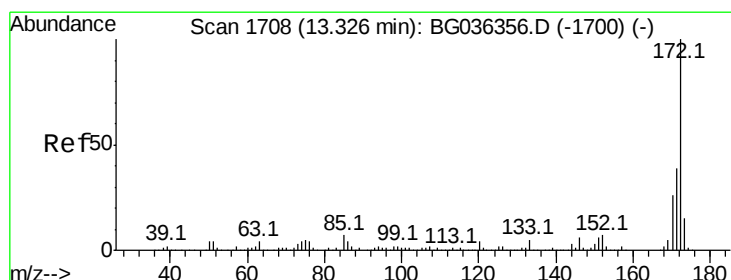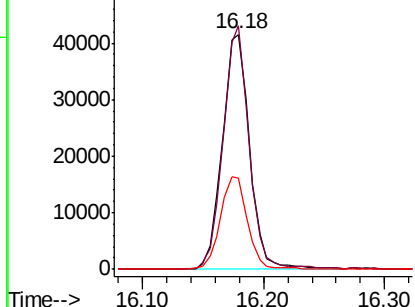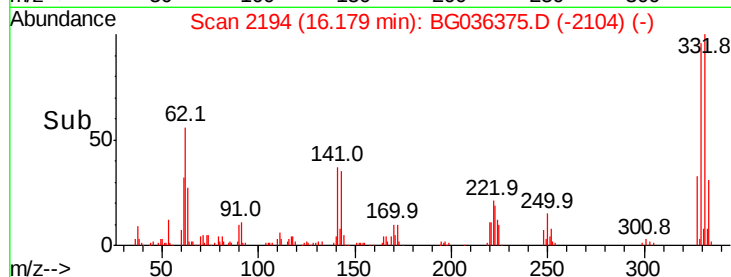

#44
 2-Fluorobiphenyl
 Concen: 101.009 ng
 RT: 13.32 min Scan# 1708
 Delta R.T. -0.00 min
 Lab File: BG036375.D
 Acq: 23 Aug 2018 12:12

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.8	31.3	46.9
170	25.9	21.0	31.6


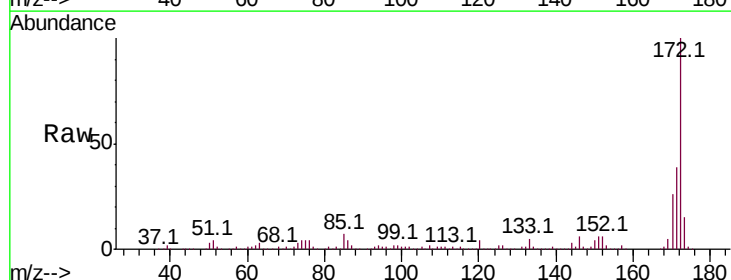



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



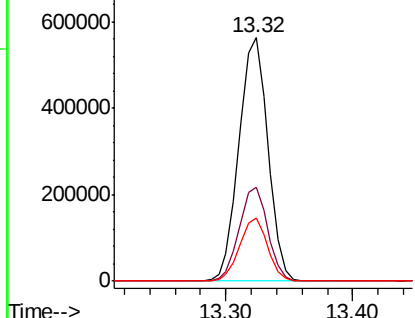
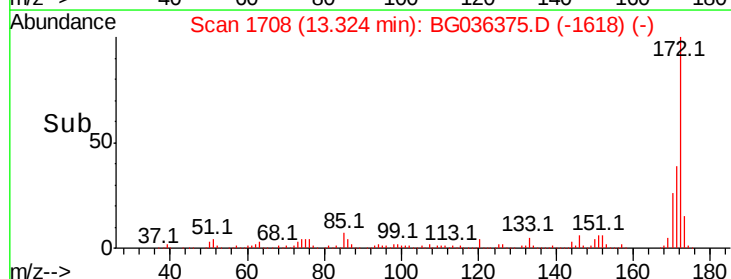


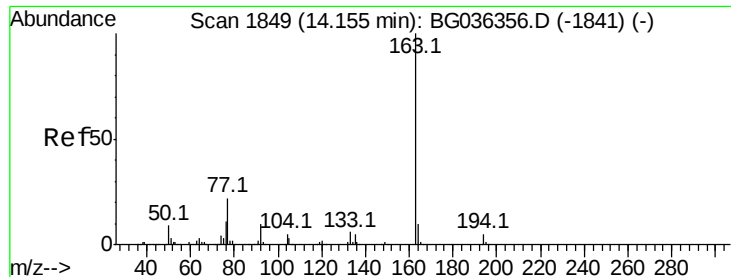

#49
Dimethylphthalate
Concen: 3.790 ng
RT: 14.14 min Scan# 1847
Delta R.T. -0.01 min
Lab File: BG036375.D
Acq: 23 Aug 2018 12:12




Instrument :
BNA_G
ClientSampleId :
081618-TIPC-E-U-M


Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	4.0	6.0
164	10.9	8.1	12.1

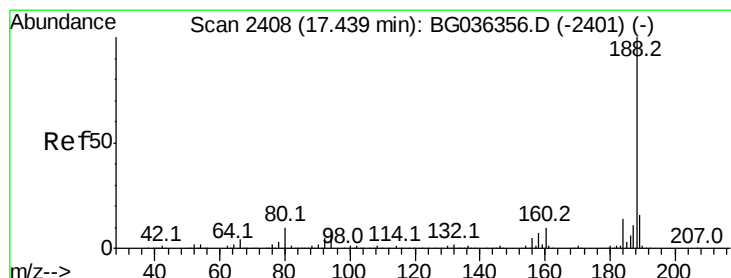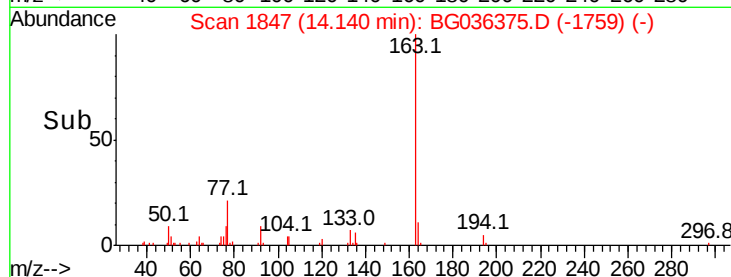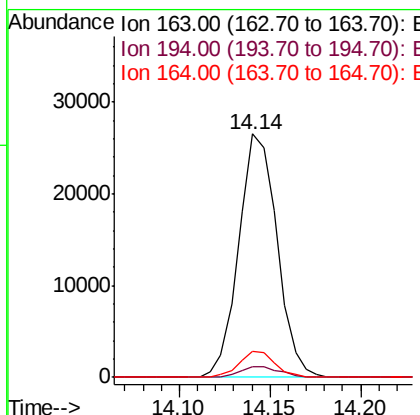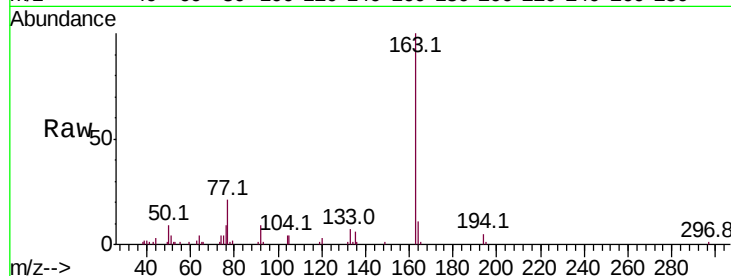

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.44 min Scan# 2408
Delta R.T. -0.00 min
Lab File: BG036375.D
Acq: 23 Aug 2018 12:12

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.6	6.7	10.1
80	9.4	8.1	12.1

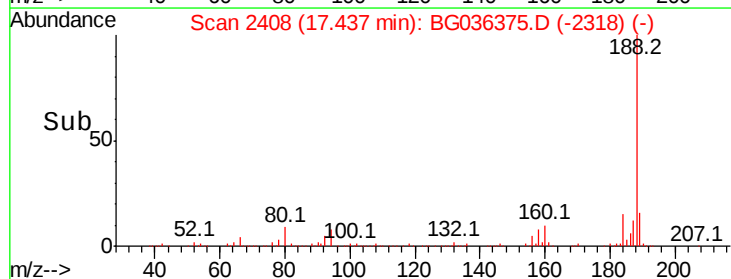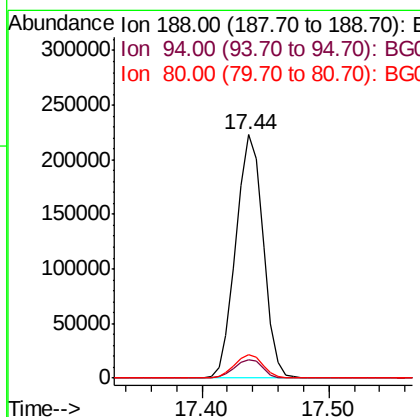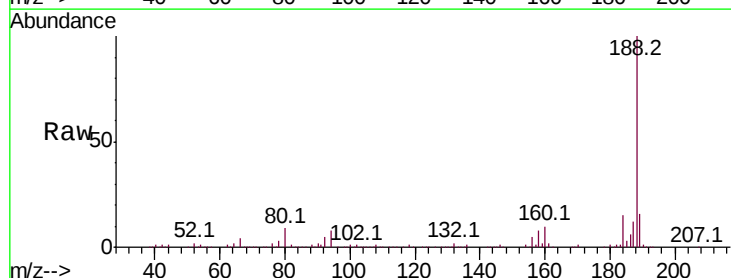

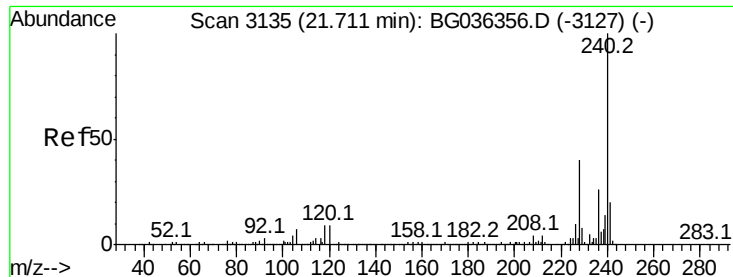

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.70 min Scan# 3134

Delta R.T. -0.01 min

Lab File: BG036375.D

Acq: 23 Aug 2018 12:12

Instrument :

BNA_G

ClientSampleId :

081618-TIPC-E-U-M


Tot Ion:240 Resp: 378247

Ion Ratio Lower Upper

240 100

120 8.4 6.9 10.3




236 26.3 21.2 31.8

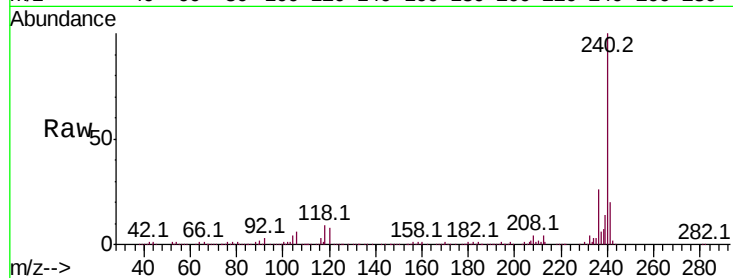

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

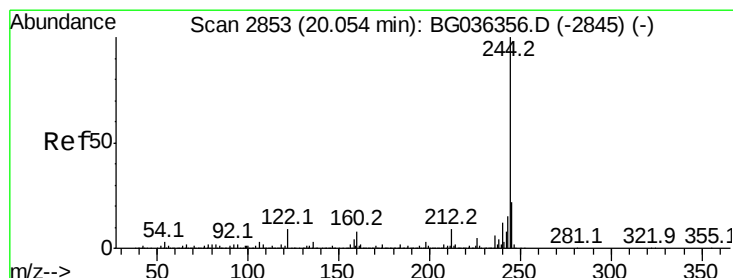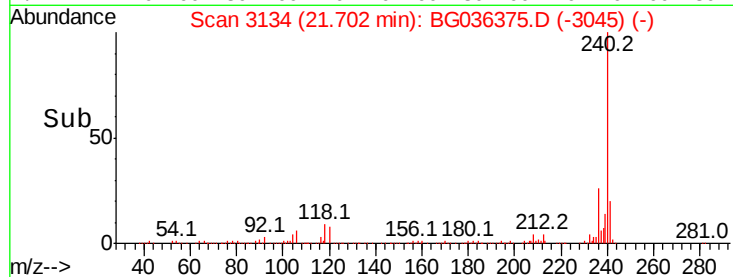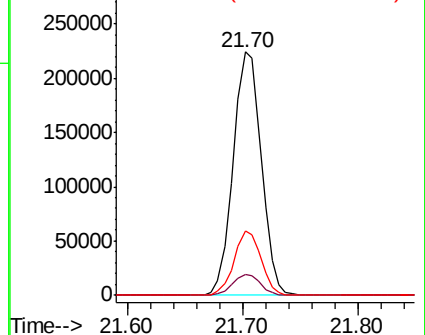

#78

Terphenyl-d14

Concen: 94.841 ng

RT: 20.05 min Scan# 2852

Delta R.T. -0.01 min

Lab File: BG036375.D

Acq: 23 Aug 2018 12:12


Tgt Ion:244 Resp: 1534793

Ion Ratio Lower Upper

244 100

212 9.2 7.0 10.6



122 10.2 7.1 10.7

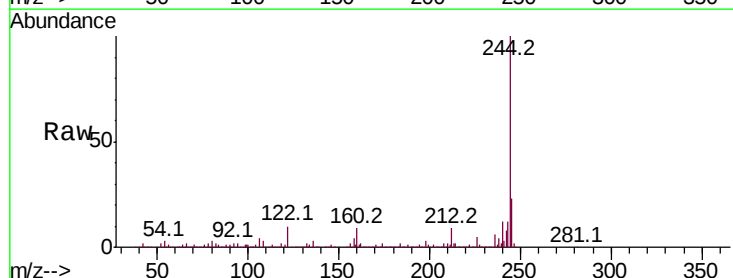


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

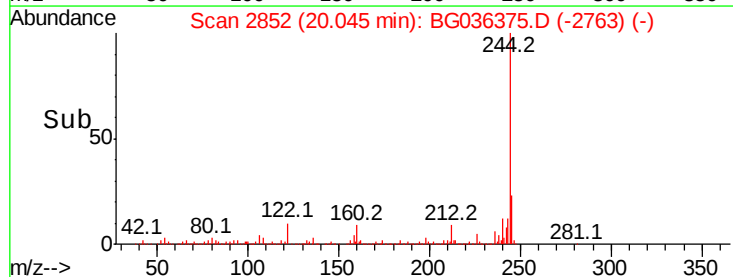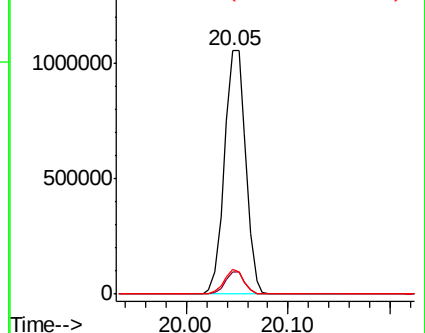


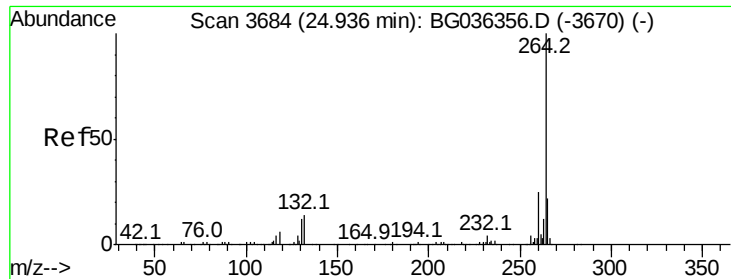

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.93 min Scan# 3683
Delta R.T. -0.01 min
Lab File: BG036375.D
Acq: 23 Aug 2018 12:12

Instrument :
BNA_G
ClientSampleId :
081618-TIPC-E-U-M

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.6	29.4
265	21.0	17.4	26.0

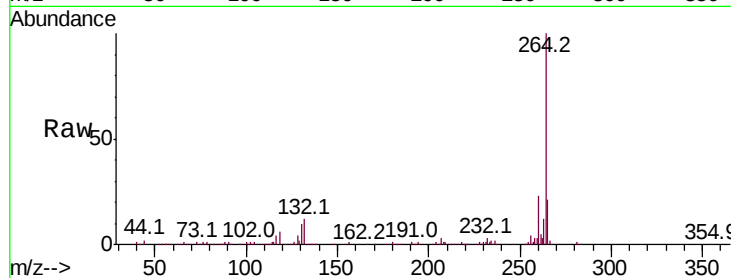

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

