


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082318\
 Data File : BG036352.D
 Acq On : 22 Aug 2018 21:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

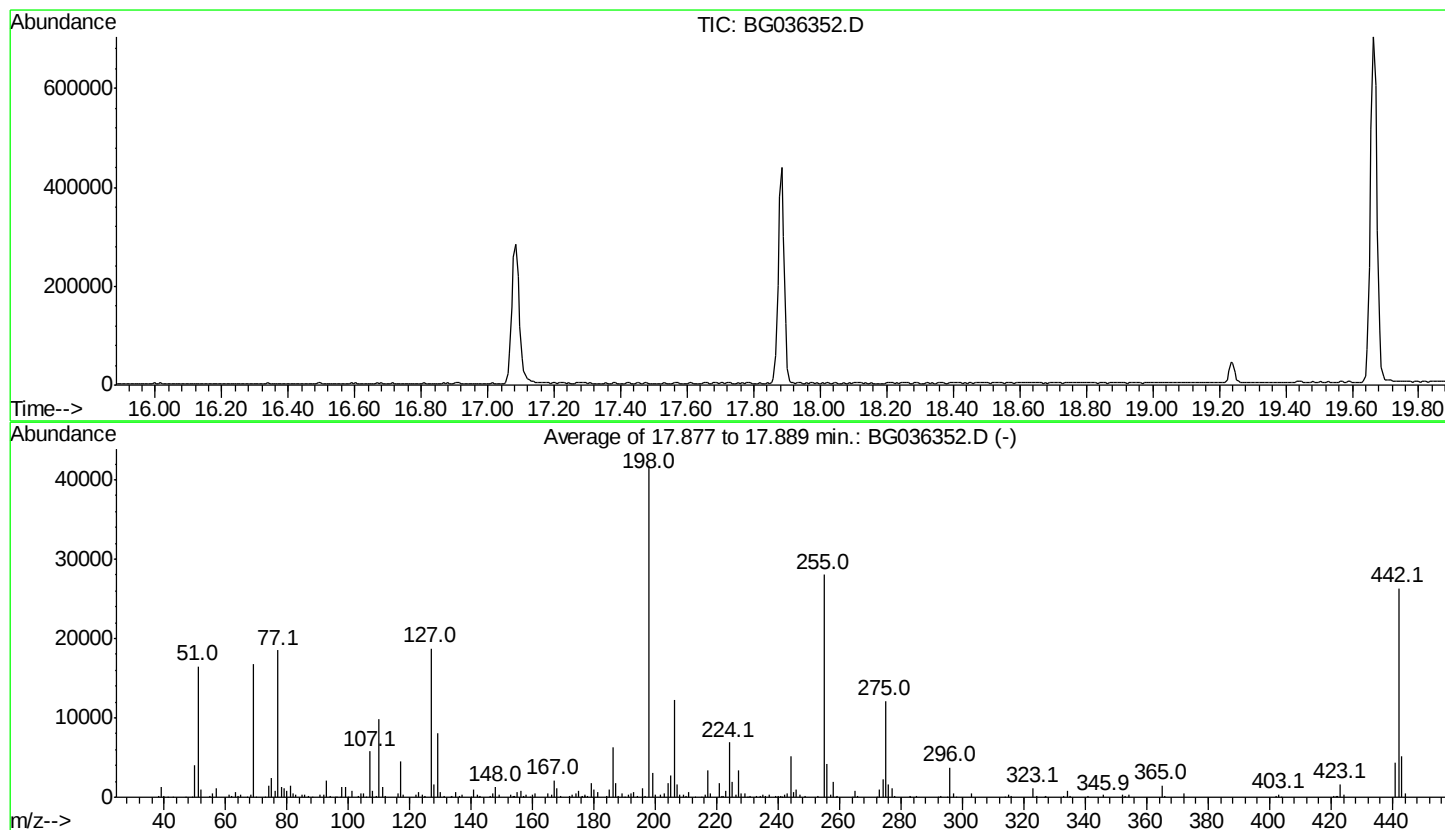

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	16530	PASS
68	69	0.00	2	1.9	320	PASS
69	198	0.00	100	40.0	16726	PASS
70	69	0.00	2	0.4	61	PASS
127	198	10	80	44.9	18733	PASS
197	198	0.00	2	0.3	130	PASS
198	198	100	100	100.0	41768	PASS
199	198	5	9	7.2	3021	PASS
275	198	10	60	29.0	12113	PASS
365	198	1	100	3.6	1520	PASS
441	198	0.01	100	10.3	4297	PASS
442	198	50	100	63.1	26341	PASS
443	442	15	24	19.4	5104	PASS