


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082318\
 Data File : BG036361.D
 Acq On : 23 Aug 2018 3:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

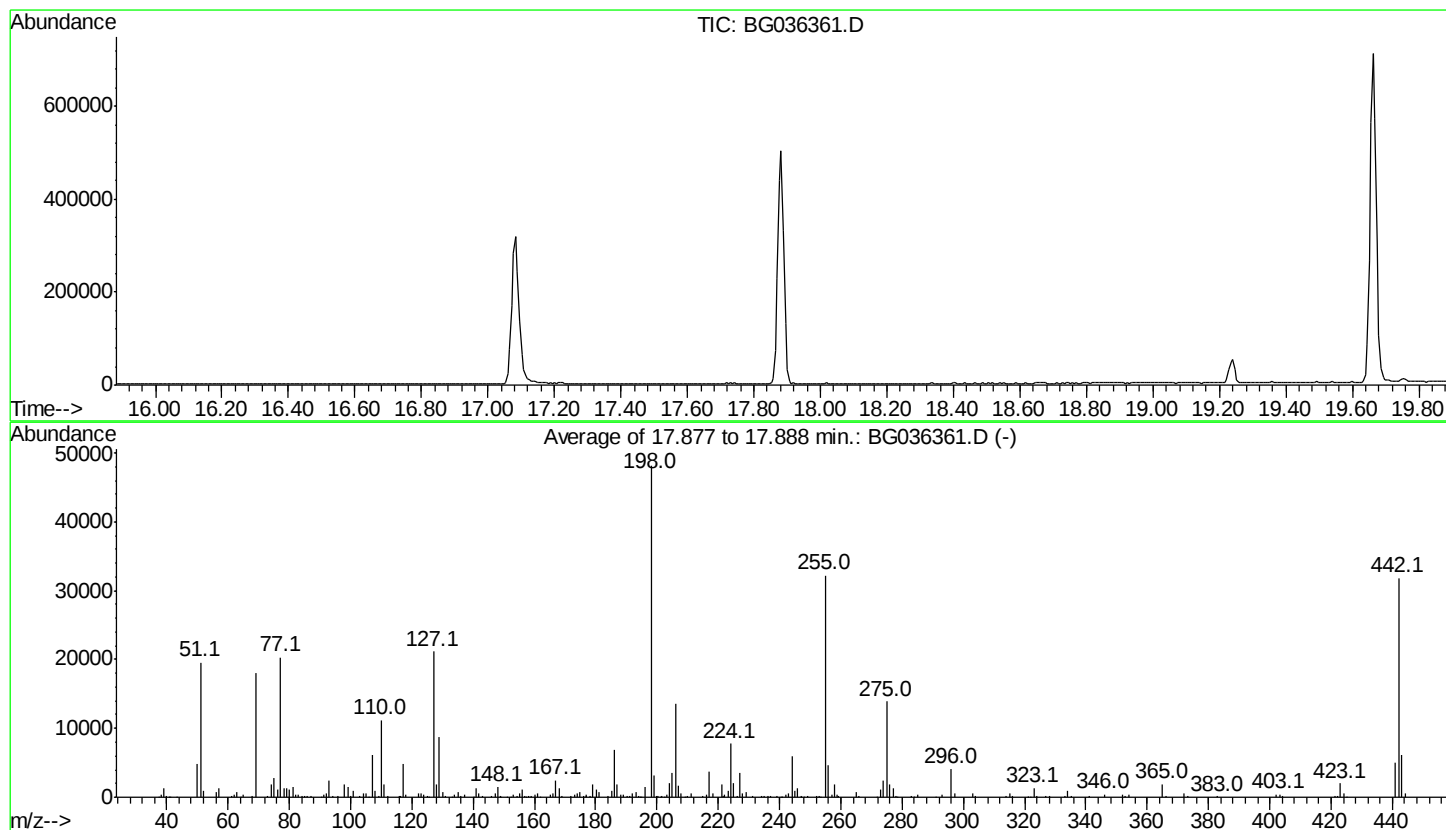

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	19583	PASS
68	69	0.00	2	1.3	237	PASS
69	198	0.00	100	37.5	18052	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	21129	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48170	PASS
199	198	5	9	6.7	3251	PASS
275	198	10	60	28.8	13862	PASS
365	198	1	100	4.1	1955	PASS
441	198	0.01	100	10.6	5108	PASS
442	198	50	100	66.1	31842	PASS
443	442	15	24	19.1	6068	PASS