
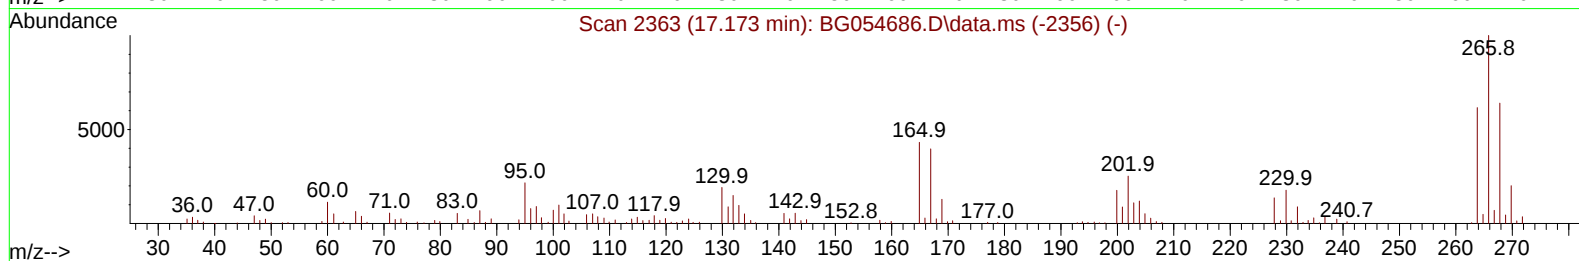
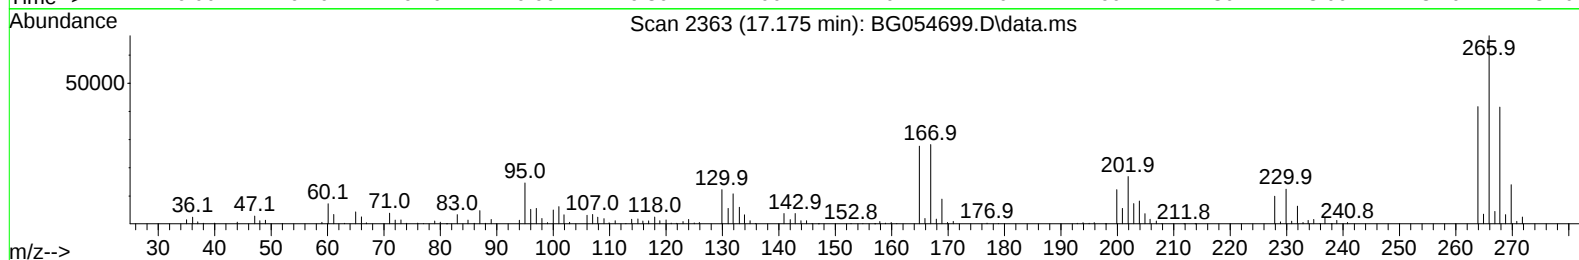


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082322\
Data File : BG054699.D
Acq On : 23 Aug 2022 9:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 03:56:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

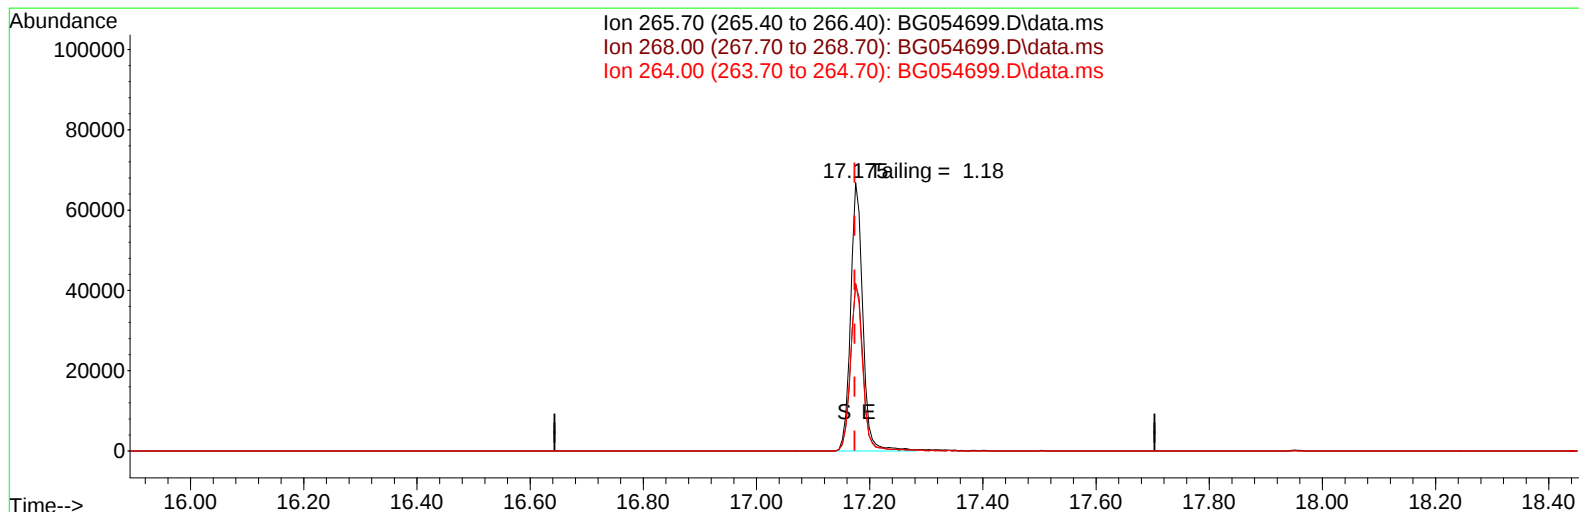

TIC: BG054699.D\data.ms

(70) Pentachlorophenol (C)




17.175min (+ 0.002) 245573.68 ng

response 100085

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.12
264.00	61.70	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082322\
Data File : BG054699.D
Acq On : 23 Aug 2022 9:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 03:56:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

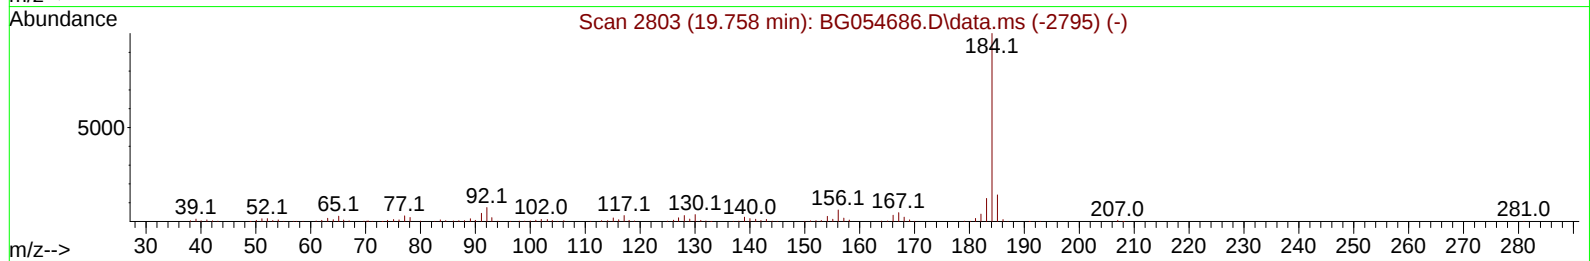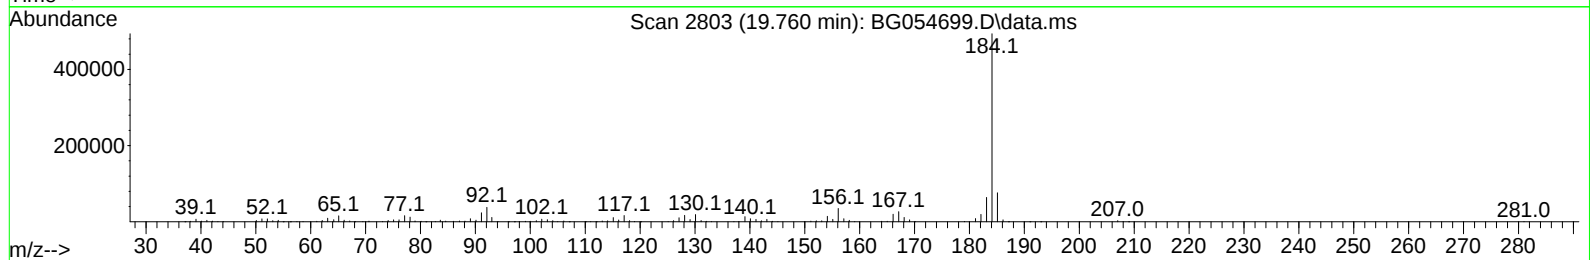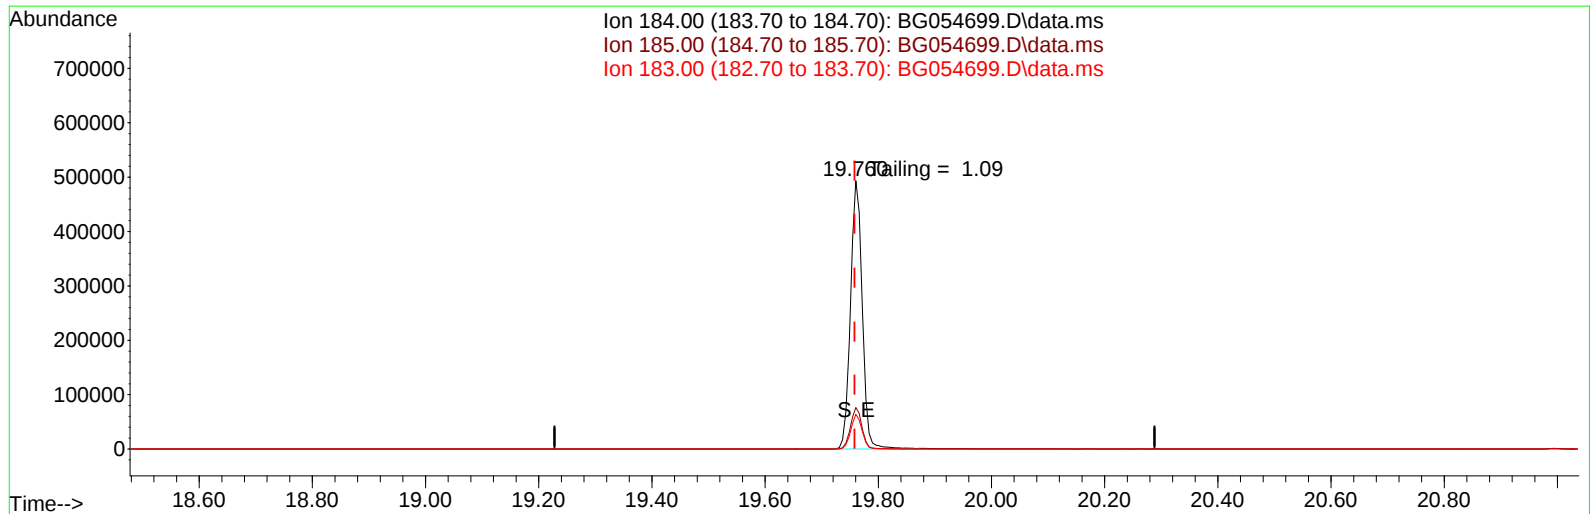

TIC: BG054699.D\data.ms

(77) Benzidine**19.760min (+ 0.003) 64583.56 ng****response 713748**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.43
183.00	12.30	12.97
0.00	0.00	0.00