
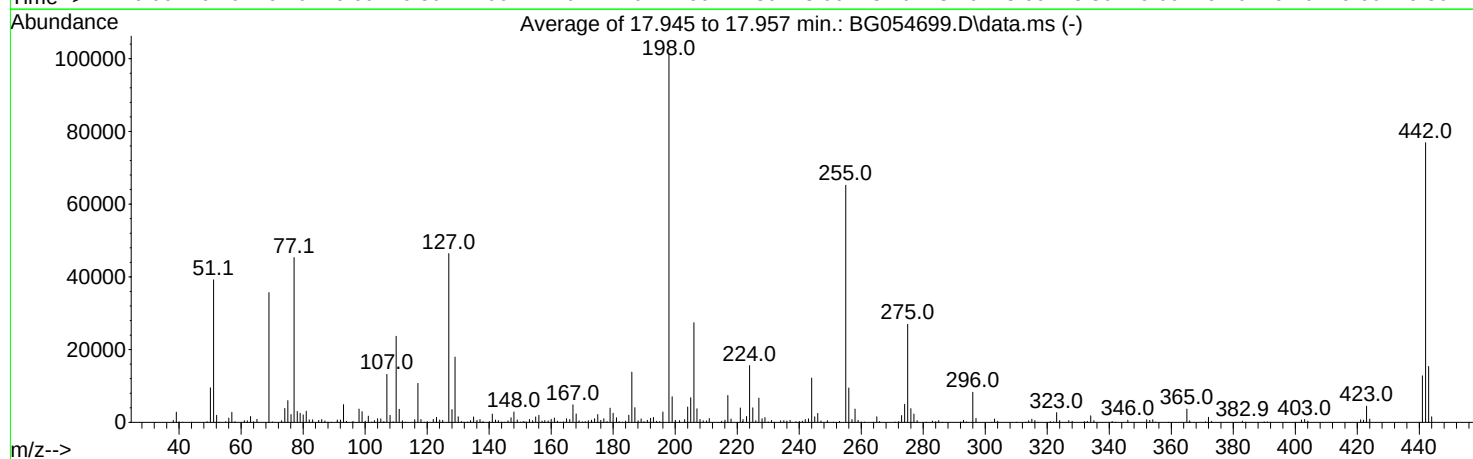


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082322\
 Data File : BG054699.D
 Acq On : 23 Aug 2022 9:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 23 03:09:46 2022

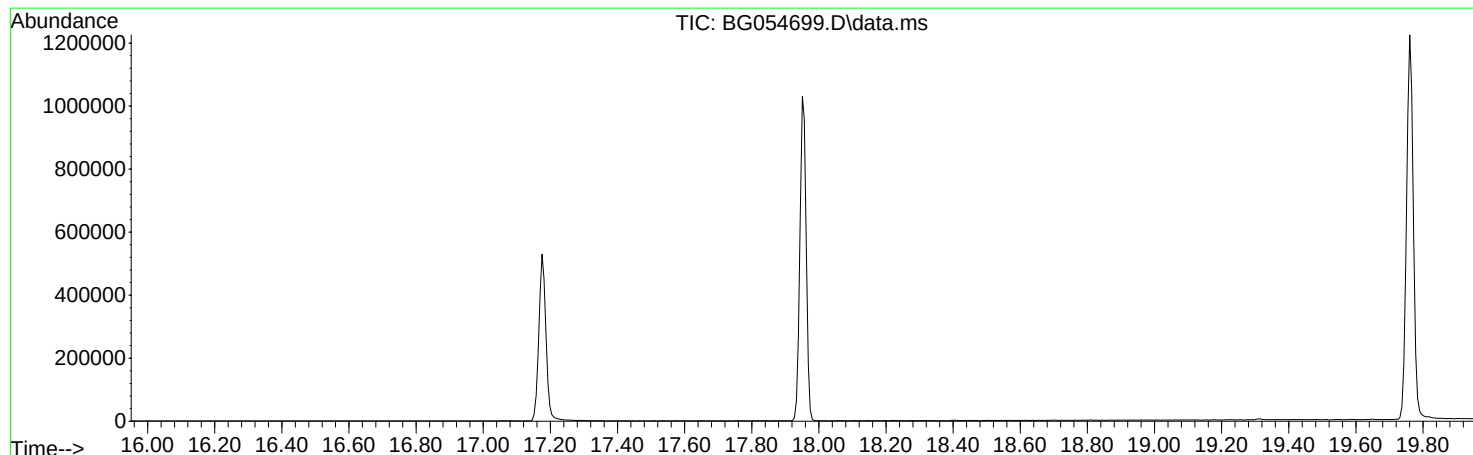




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	39181	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	35701	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	45.9	46424	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101147	PASS
199	198	5	9	7.0	7034	PASS
275	198	10	60	26.7	26992	PASS
365	198	1	100	3.6	3657	PASS
441	198	0.01	100	12.7	12812	PASS
442	442	50	100	100.0	76907	PASS
443	442	15	24	20.0	15362	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082322\
Data File : BG054699.D
Acq On : 23 Aug 2022 9:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 03:56:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

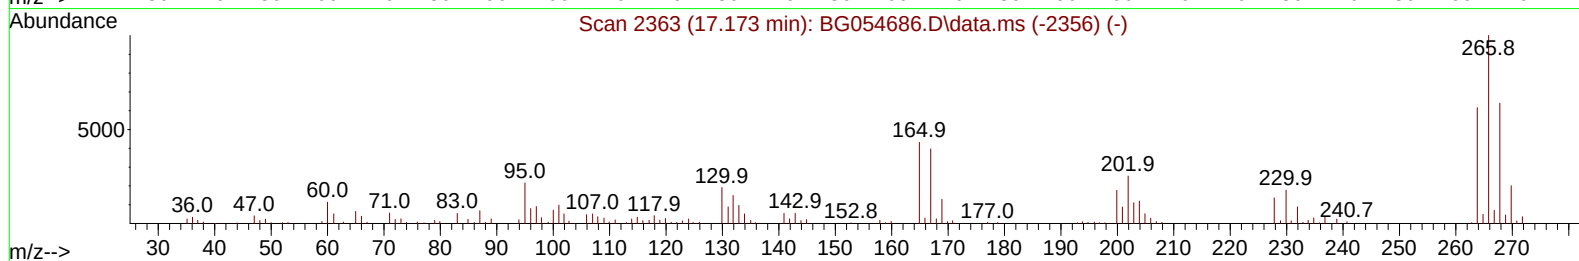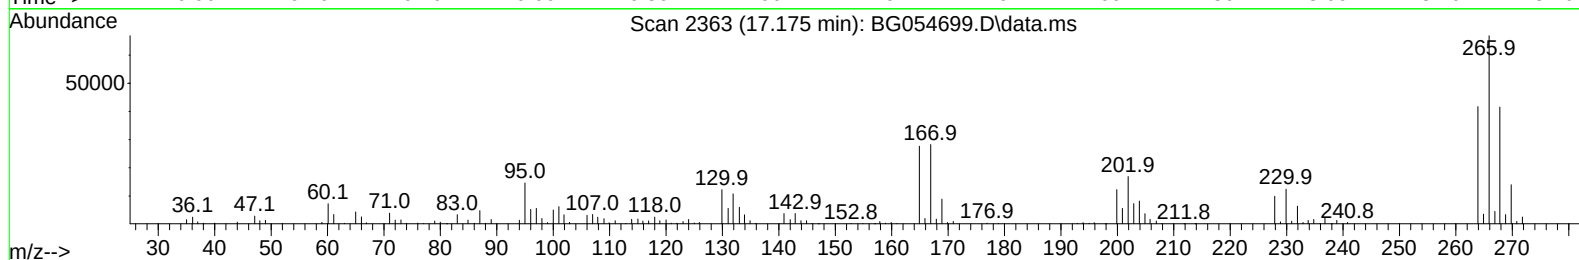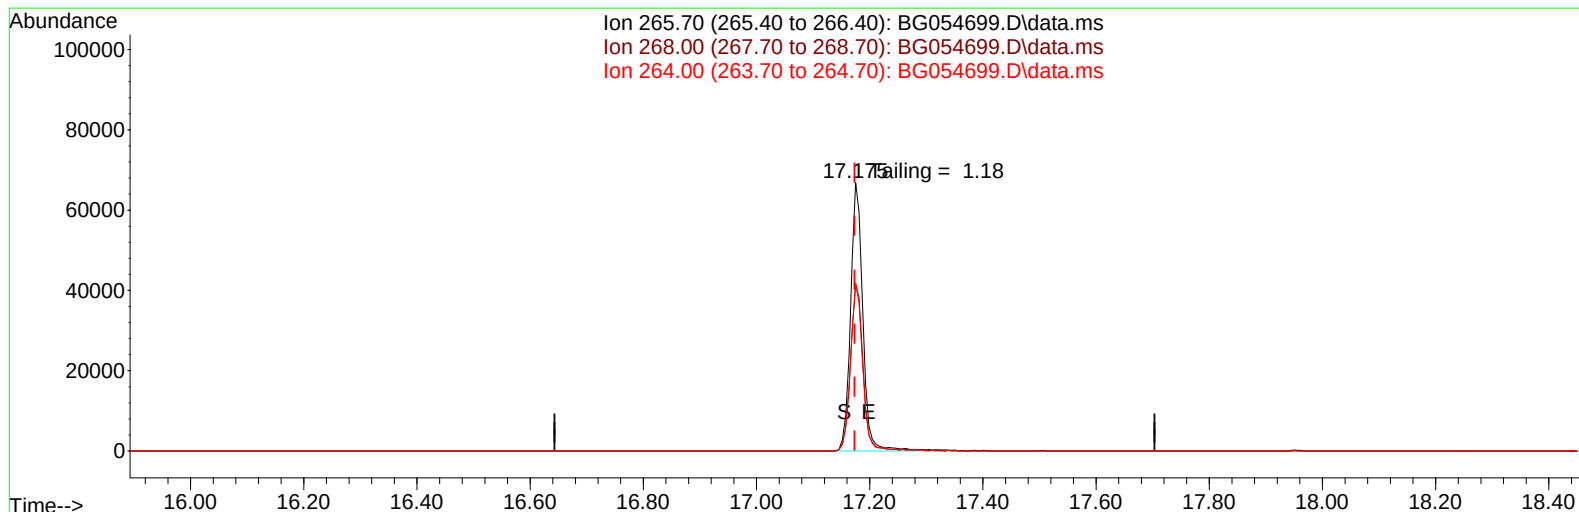

TIC: BG054699.D\data.ms

(70) Pentachlorophenol (C)

17.175min (+ 0.002) 245573.68 ng




response 100085

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.12
264.00	61.70	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082322\
Data File : BG054699.D
Acq On : 23 Aug 2022 9:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 03:56:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

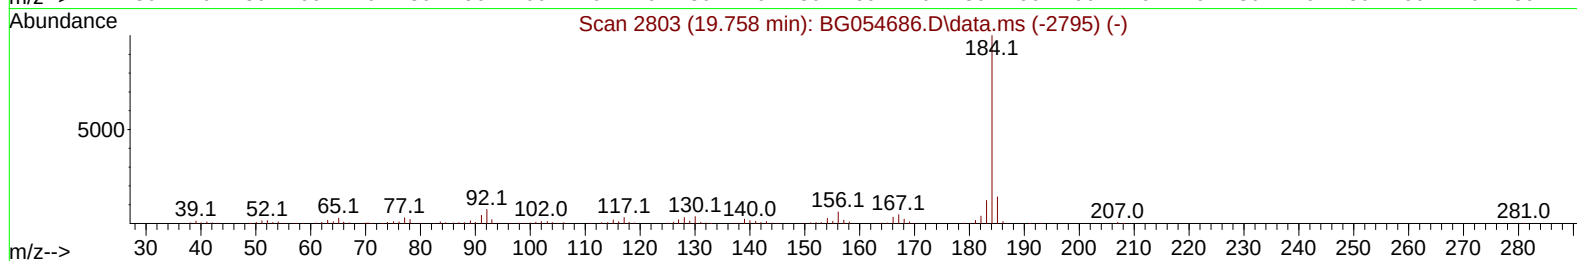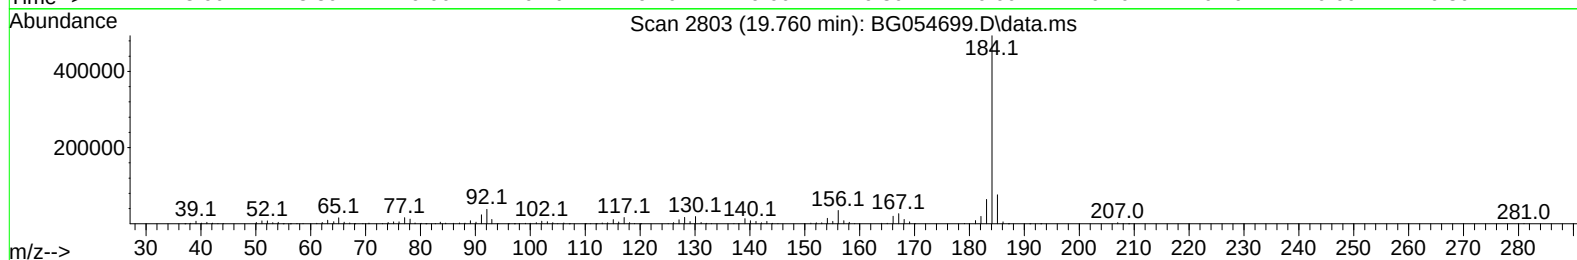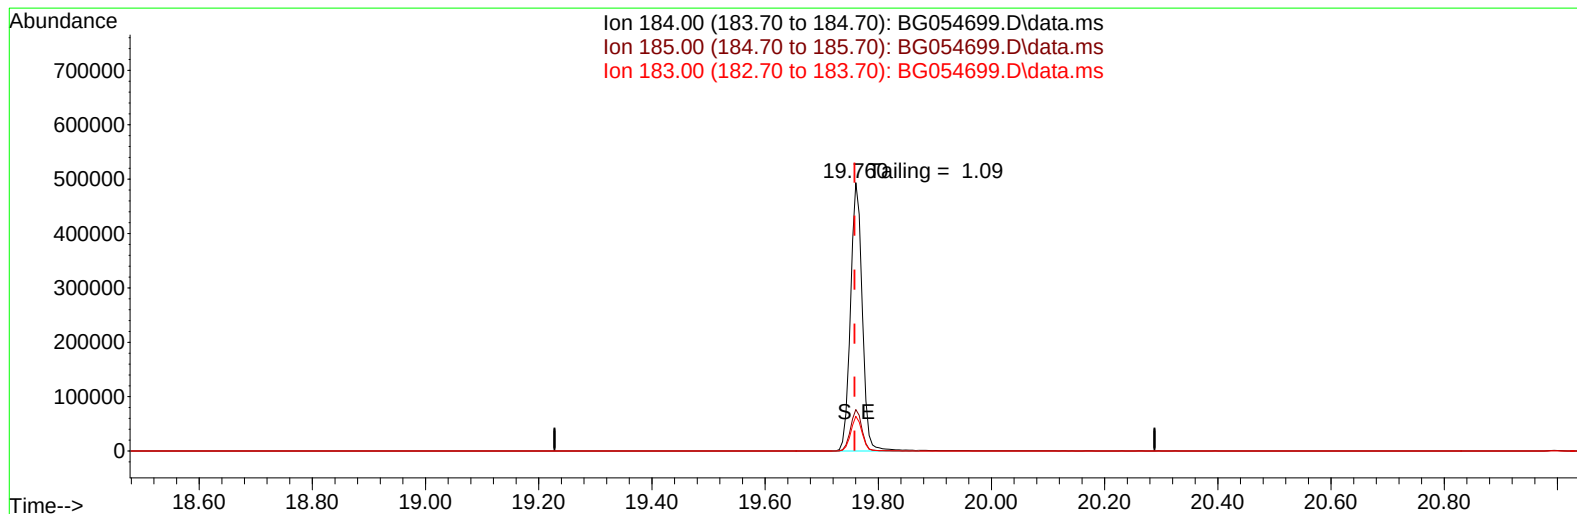

TIC: BG054699.D\data.ms

(77) Benzidine

19.760min (+ 0.003) 64583.56 ng

response 713748

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.43
183.00	12.30	12.97
0.00	0.00	0.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2022	BNA_G	<u>BG054699.D</u>
Compound Name	Response	Retention Time
DDT	266558	20.994
DDD	7595	20.548
DDE	2284	20.042
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9879	276437	3.57