
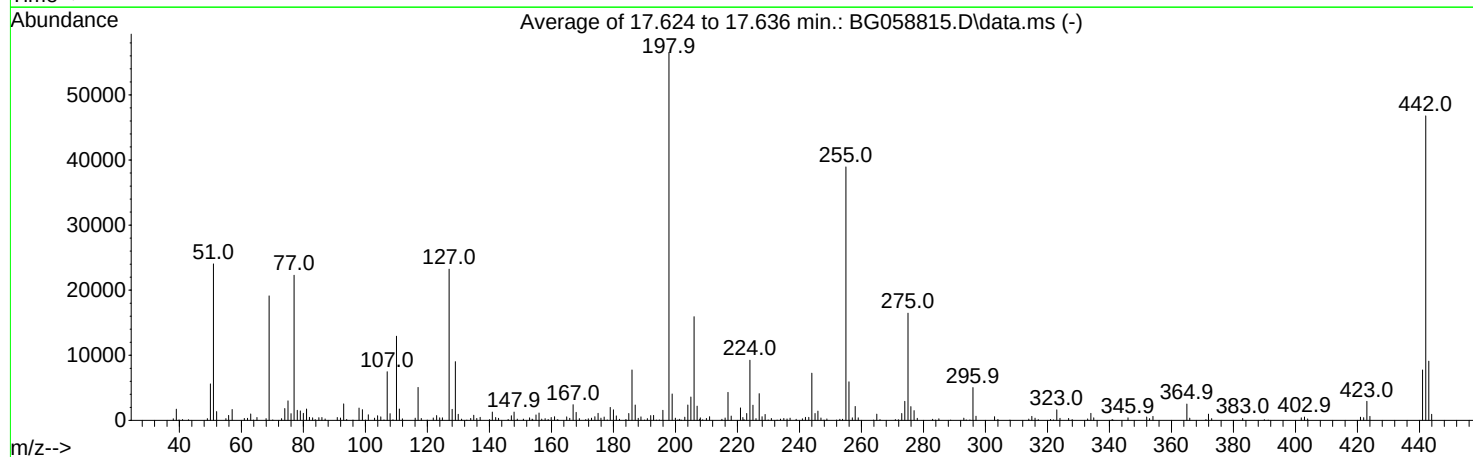


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082323\
Data File : BG058815.D
Acq On : 23 Aug 2023 9:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 21 01:40:57 2023

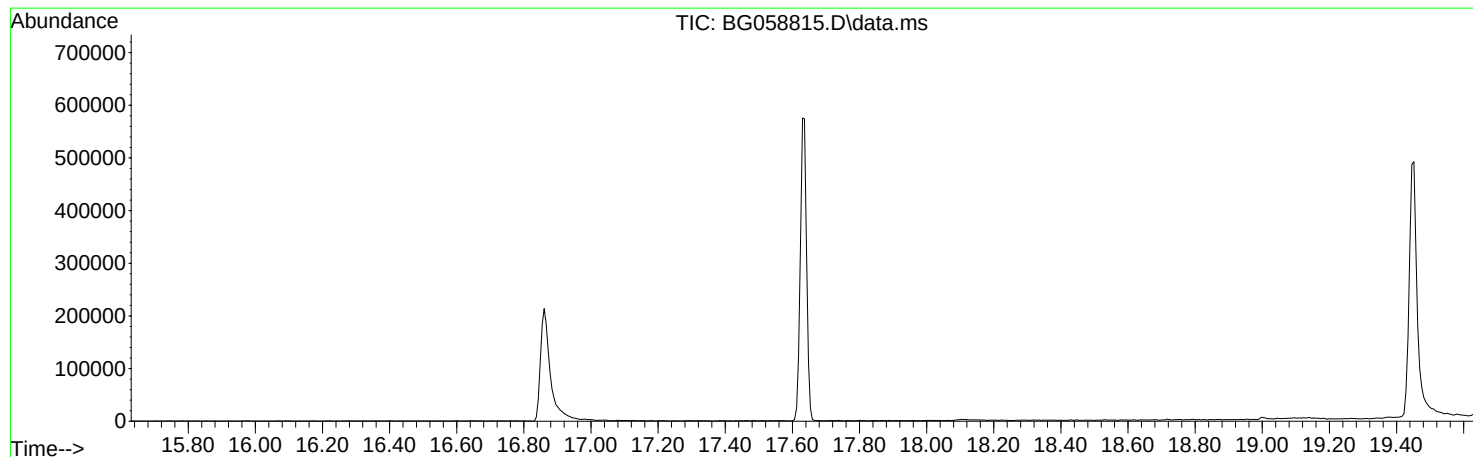




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	24051	PASS
68	69	0.00	2	1.5	280	PASS
69	198	0.00	100	33.8	19124	PASS
70	69	0.00	2	0.4	73	PASS
127	198	10	80	41.1	23227	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56515	PASS
199	198	5	9	7.2	4062	PASS
275	198	10	60	29.2	16477	PASS
365	198	1	100	4.4	2514	PASS
441	198	0.01	100	13.7	7753	PASS
442	442	50	100	100.0	46773	PASS
443	442	15	24	19.5	9109	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082323\
Data File : BG058815.D
Acq On : 23 Aug 2023 9:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 23 11:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

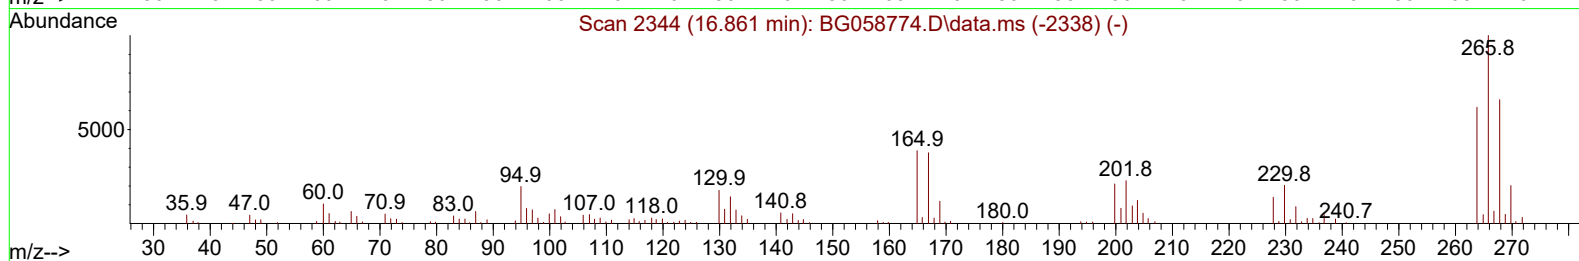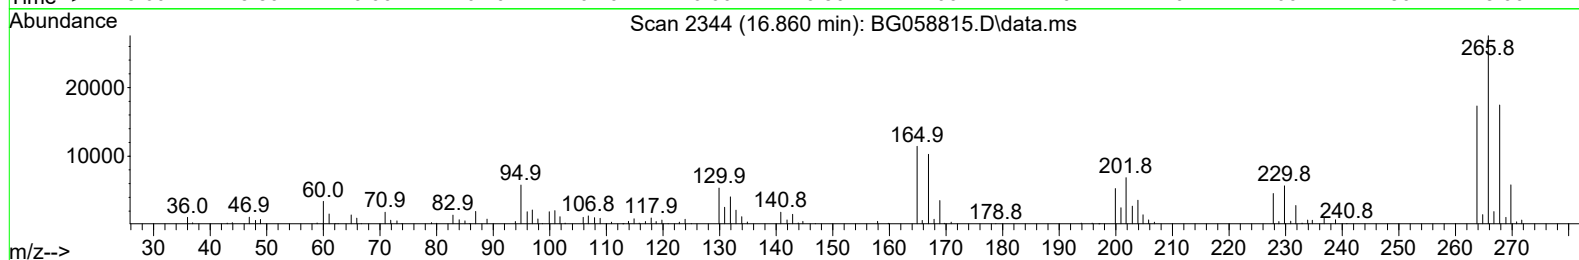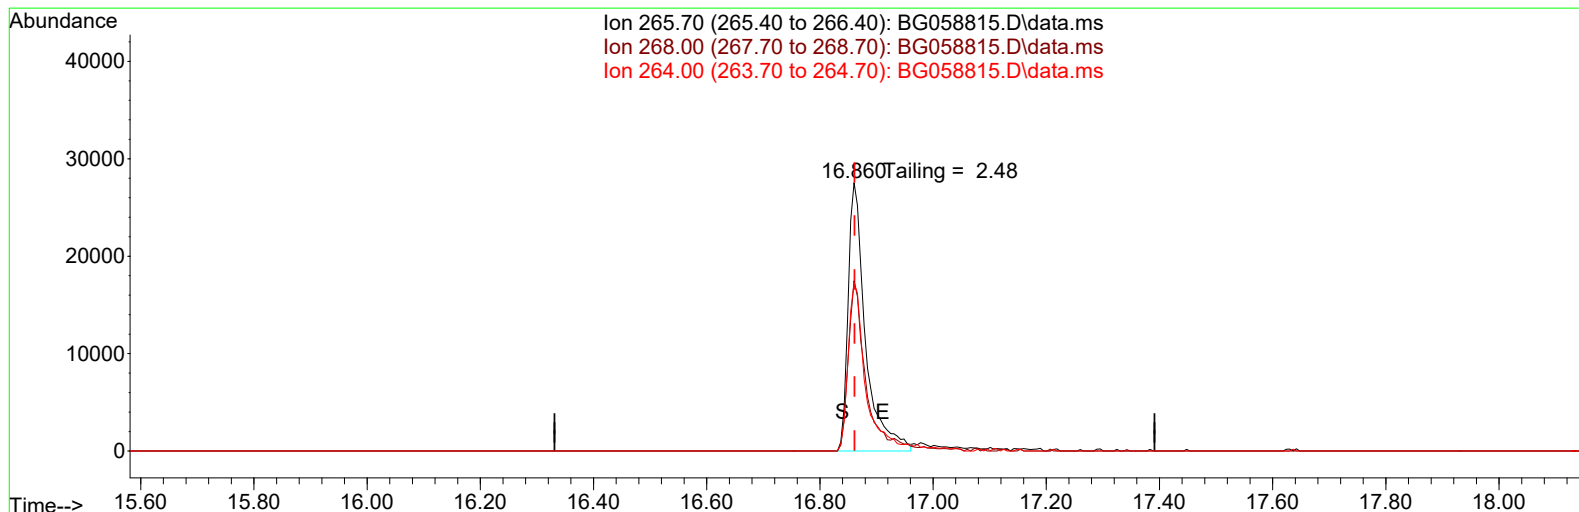

TIC: BG058815.D\data.ms

(70) Pentachlorophenol (C)

16.860min (-0.001) 23566.65 ng




response 58817

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	63.39
264.00	61.90	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082323\
Data File : BG058815.D
Acq On : 23 Aug 2023 9:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 23 11:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

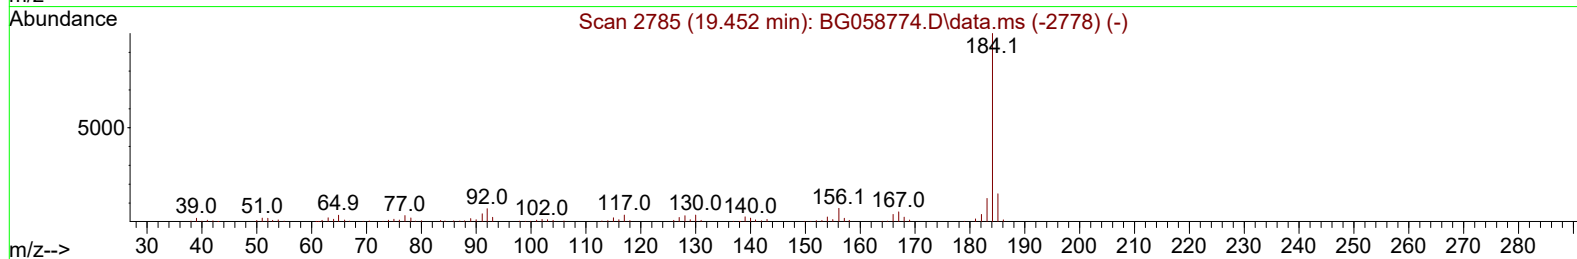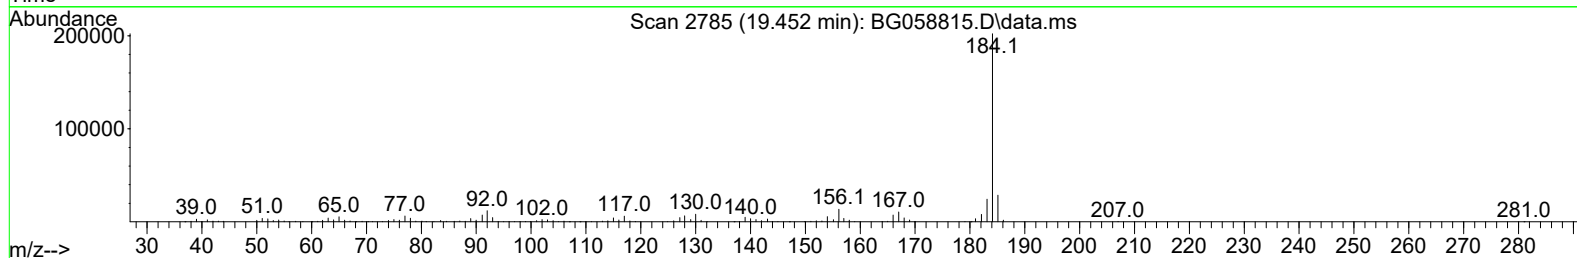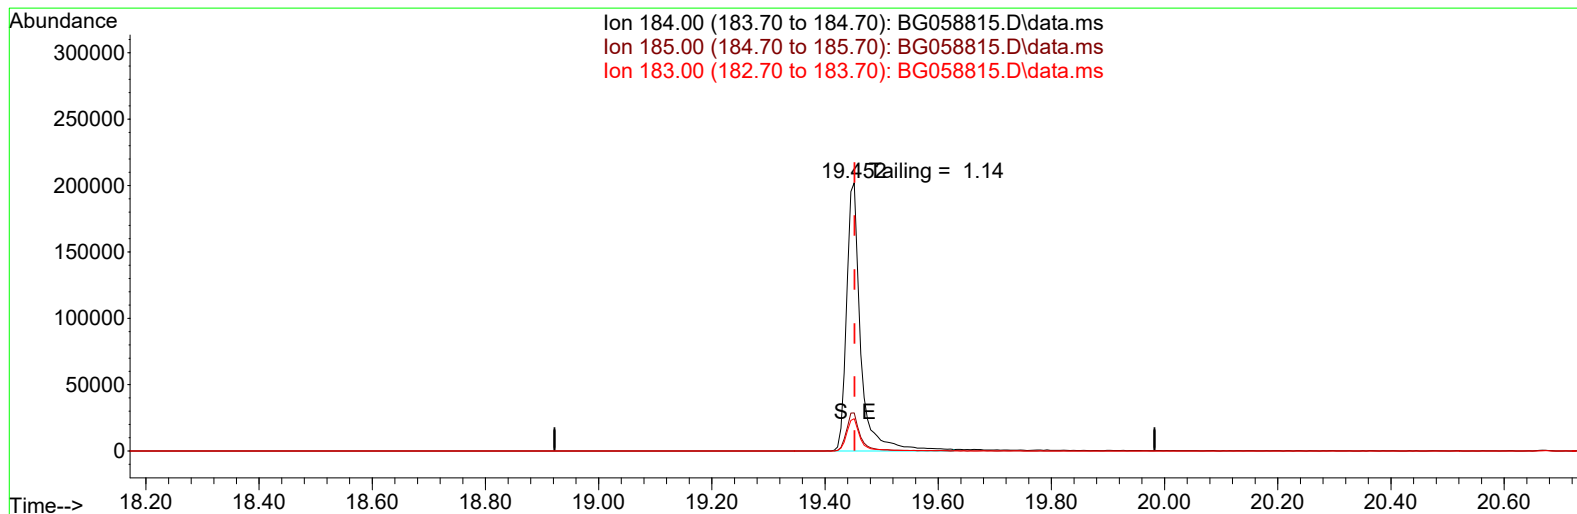

TIC: BG058815.D\data.ms

(77) Benzidine

19.452min (-0.000) 0.00 ng

response 354769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.23
183.00	12.50	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2023	BNA_G	<u>BG058815.D</u>
Compound Name	Response	Retention Time
DDT	171611	20.668
DDD	10945	20.233
DDE	822	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11767	183378	6.42

Instrument :
BNA_G
ClientSampleId :
DFTPP