
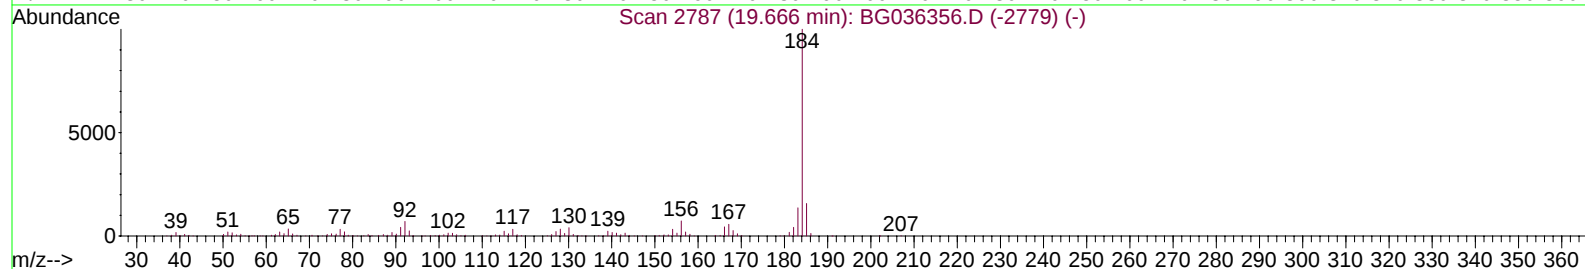
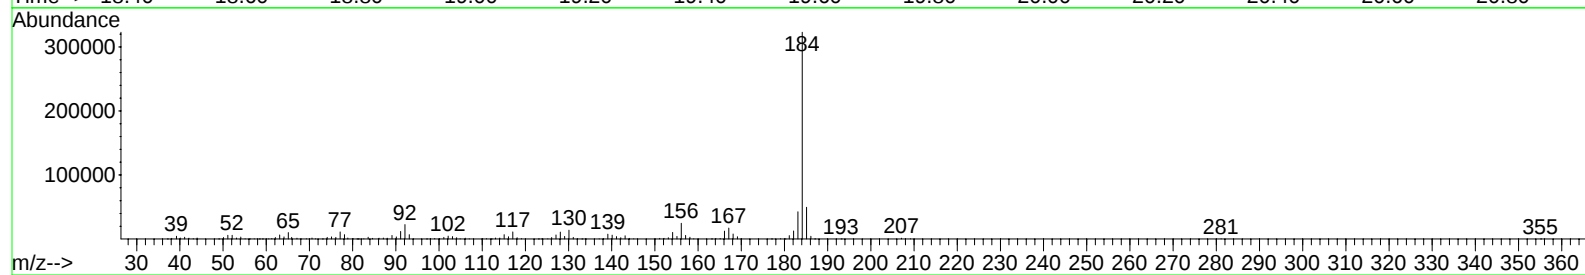


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082418\
Data File : BG036378.D
Acq On : 23 Aug 2018 14:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 17:40:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

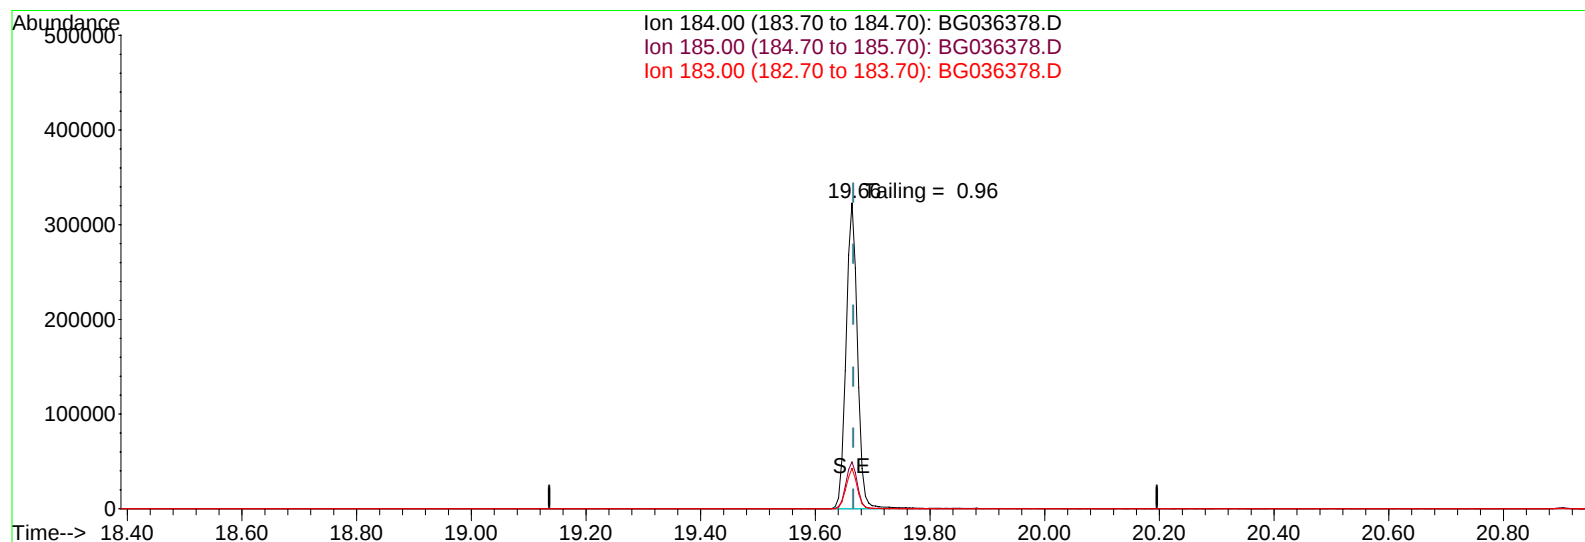

TIC: BG036378.D

(76) Benzidine




19.664min (-0.002) 0.00ng

response 447532

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.35
183.00	13.60	13.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082418\
Data File : BG036378.D
Acq On : 23 Aug 2018 14:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 17:40:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

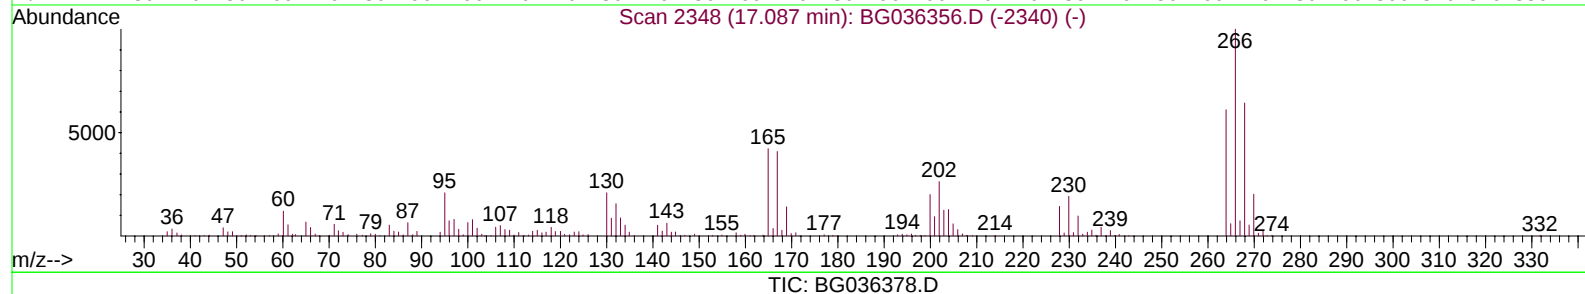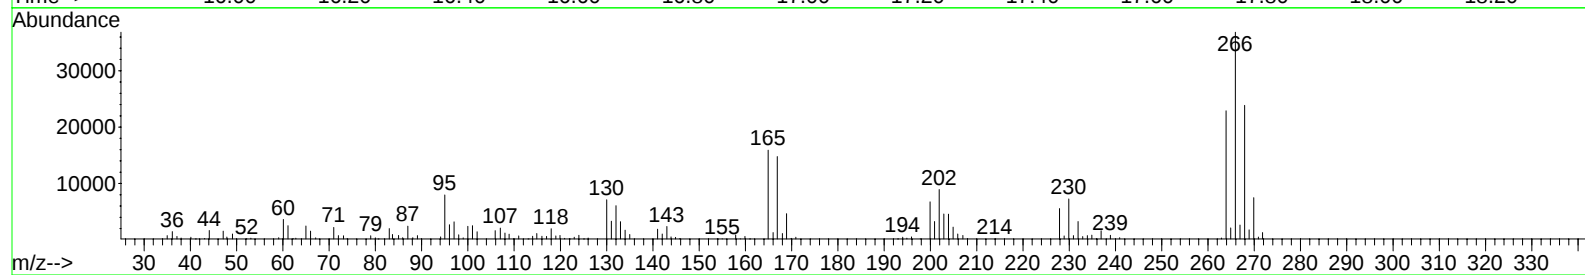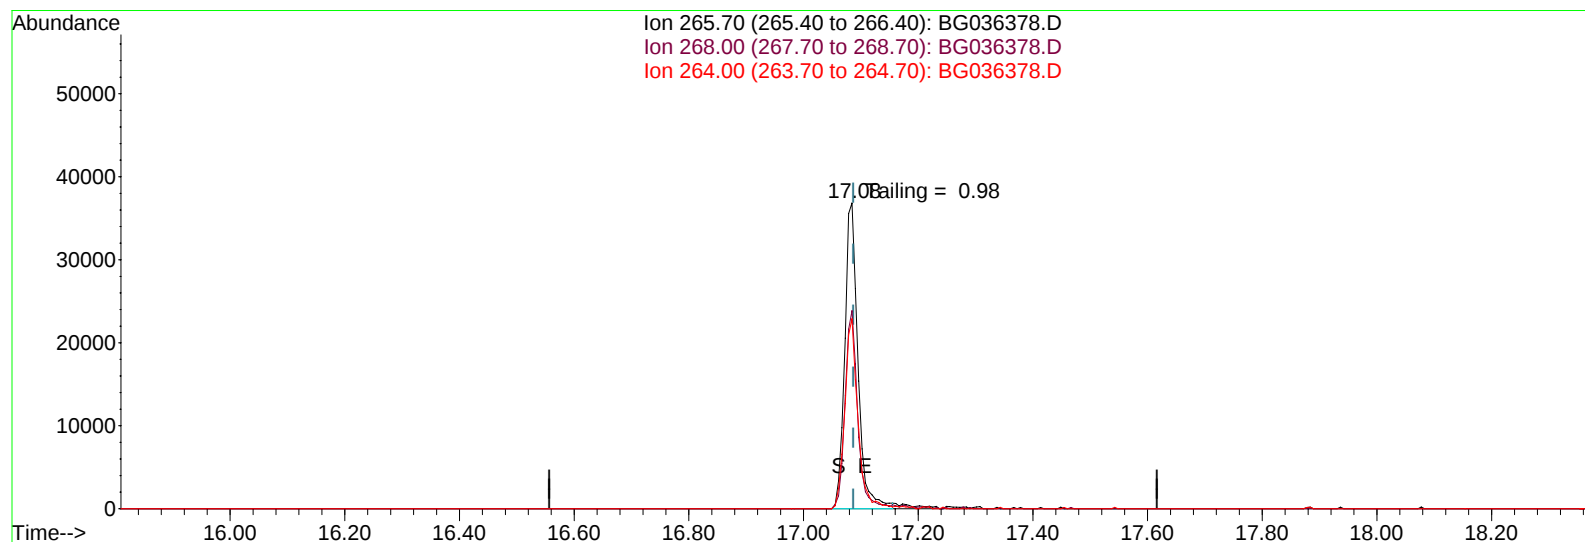

(69) Pentachlorophenol (C)

17.085min (-0.002) 25185.86ng

response 59428

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	64.78
264.00	61.10	62.17
0.00	0.00	0.00