
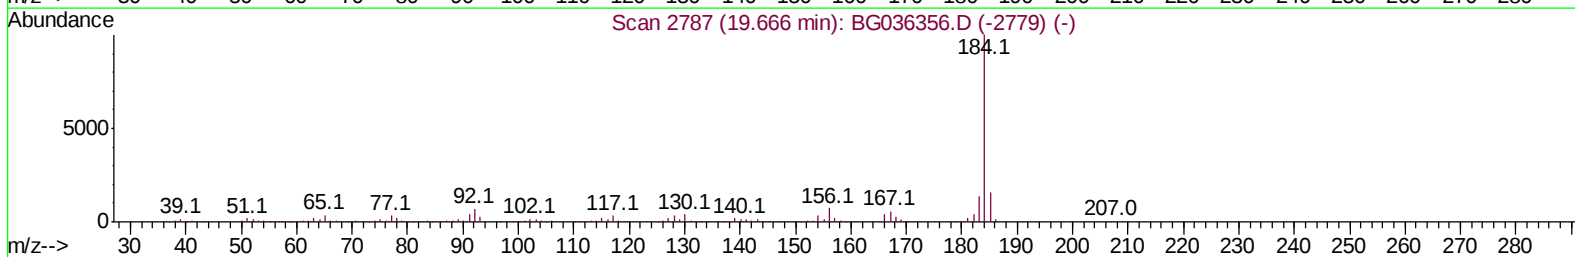
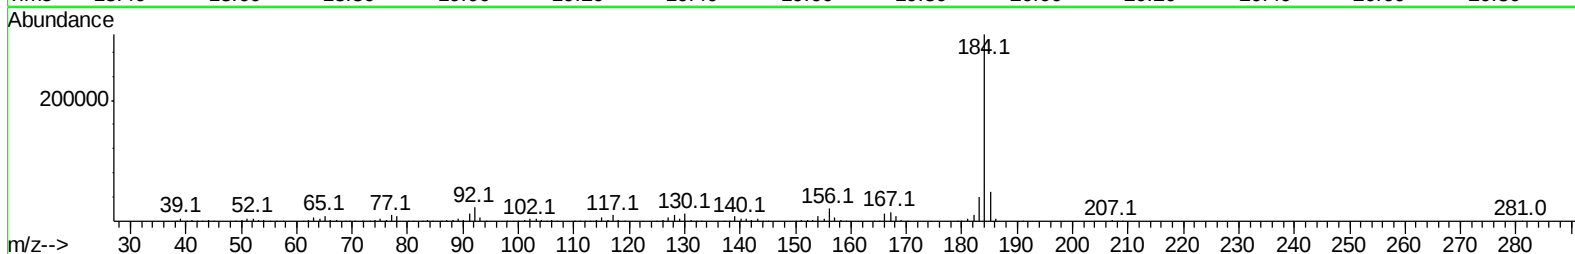


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082418\
 Data File : BG036396.D
 Acq On : 24 Aug 2018 3:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 07:36:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 12:07:02 2018
 Response via : Initial Calibration

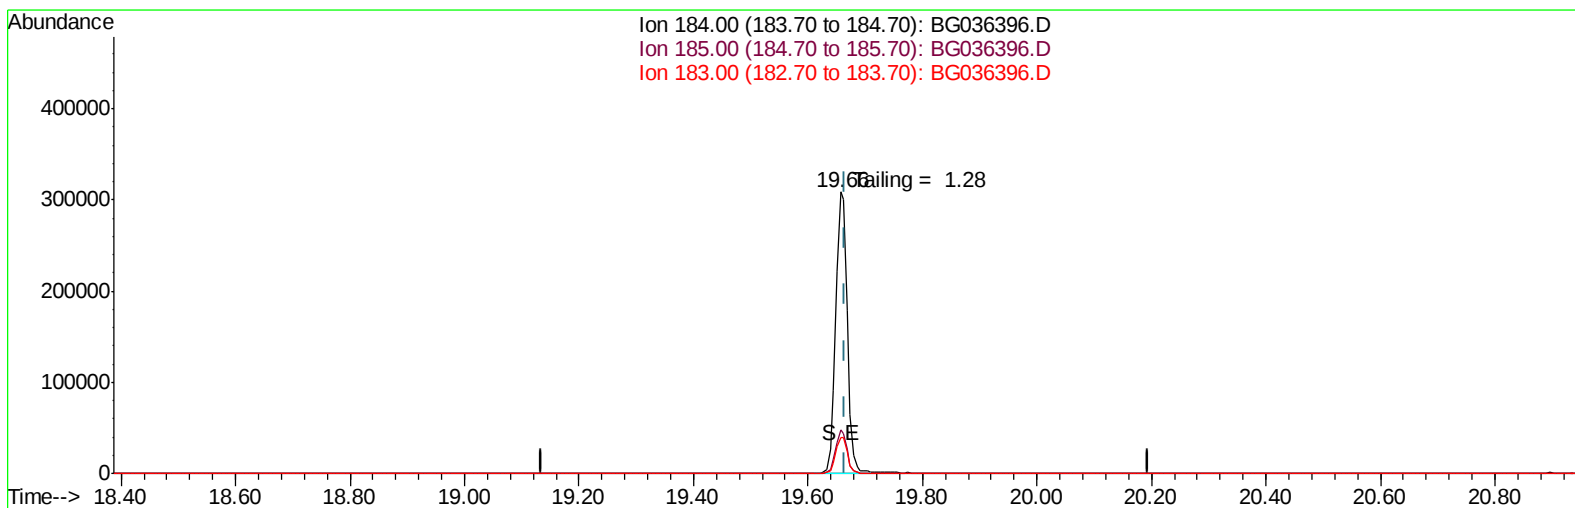

TIC: BG036396.D

(76) Benzidine

19.656min (-0.010) 0.00ng

response 438584

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.52
183.00	13.60	12.96
0.00	0.00	0.00

