

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082418\
 Data File : BG036406.D
 Acq On : 24 Aug 2018 9:52
 Operator : JU/SJ
 Sample : J4568-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 081718-SIDI-E-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.629	391	398	408	rVB	372029	598640	13.50%	3.292%
2	7.216	660	668	676	rBV	255657	422688	9.53%	2.325%
3	7.598	725	733	741	rBV	619189	1049853	23.67%	5.774%
4	8.068	803	813	820	rBV	183206	311269	7.02%	1.712%
5	8.391	859	868	877	rBV	826575	1401916	31.61%	7.710%
6	9.225	1002	1010	1022	rBV	704176	1223169	27.58%	6.727%
7	10.870	1283	1290	1299	rBV	243858	440428	9.93%	2.422%
8	13.320	1699	1707	1714	rBV	1858848	2961537	66.77%	16.288%
9	14.137	1841	1846	1852	rBV	49081	69621	1.57%	0.383%
10	14.689	1933	1940	1952	rVB2	417958	655955	14.79%	3.608%
11	15.988	2156	2161	2167	rVB	57937	75264	1.70%	0.414%
12	16.176	2185	2193	2205	rBV	1006181	1555243	35.06%	8.553%
13	17.433	2400	2407	2416	rBV2	567123	854817	19.27%	4.701%
14	18.320	2554	2558	2566	rBV5	33149	54264	1.22%	0.298%
15	20.042	2845	2851	2857	rBV	3410232	4435667	100.00%	24.395%
16	21.699	3126	3133	3140	rBV	647312	1063195	23.97%	5.847%
17	24.919	3670	3681	3692	rBV2	356748	1009271	22.75%	5.551%


Sum of corrected areas: 18182797

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082418\
Data File : BG036406.D
Acq On : 24 Aug 2018 9:52
Operator : JU/SJ
Sample : J4568-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
081718-SIDI-E-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

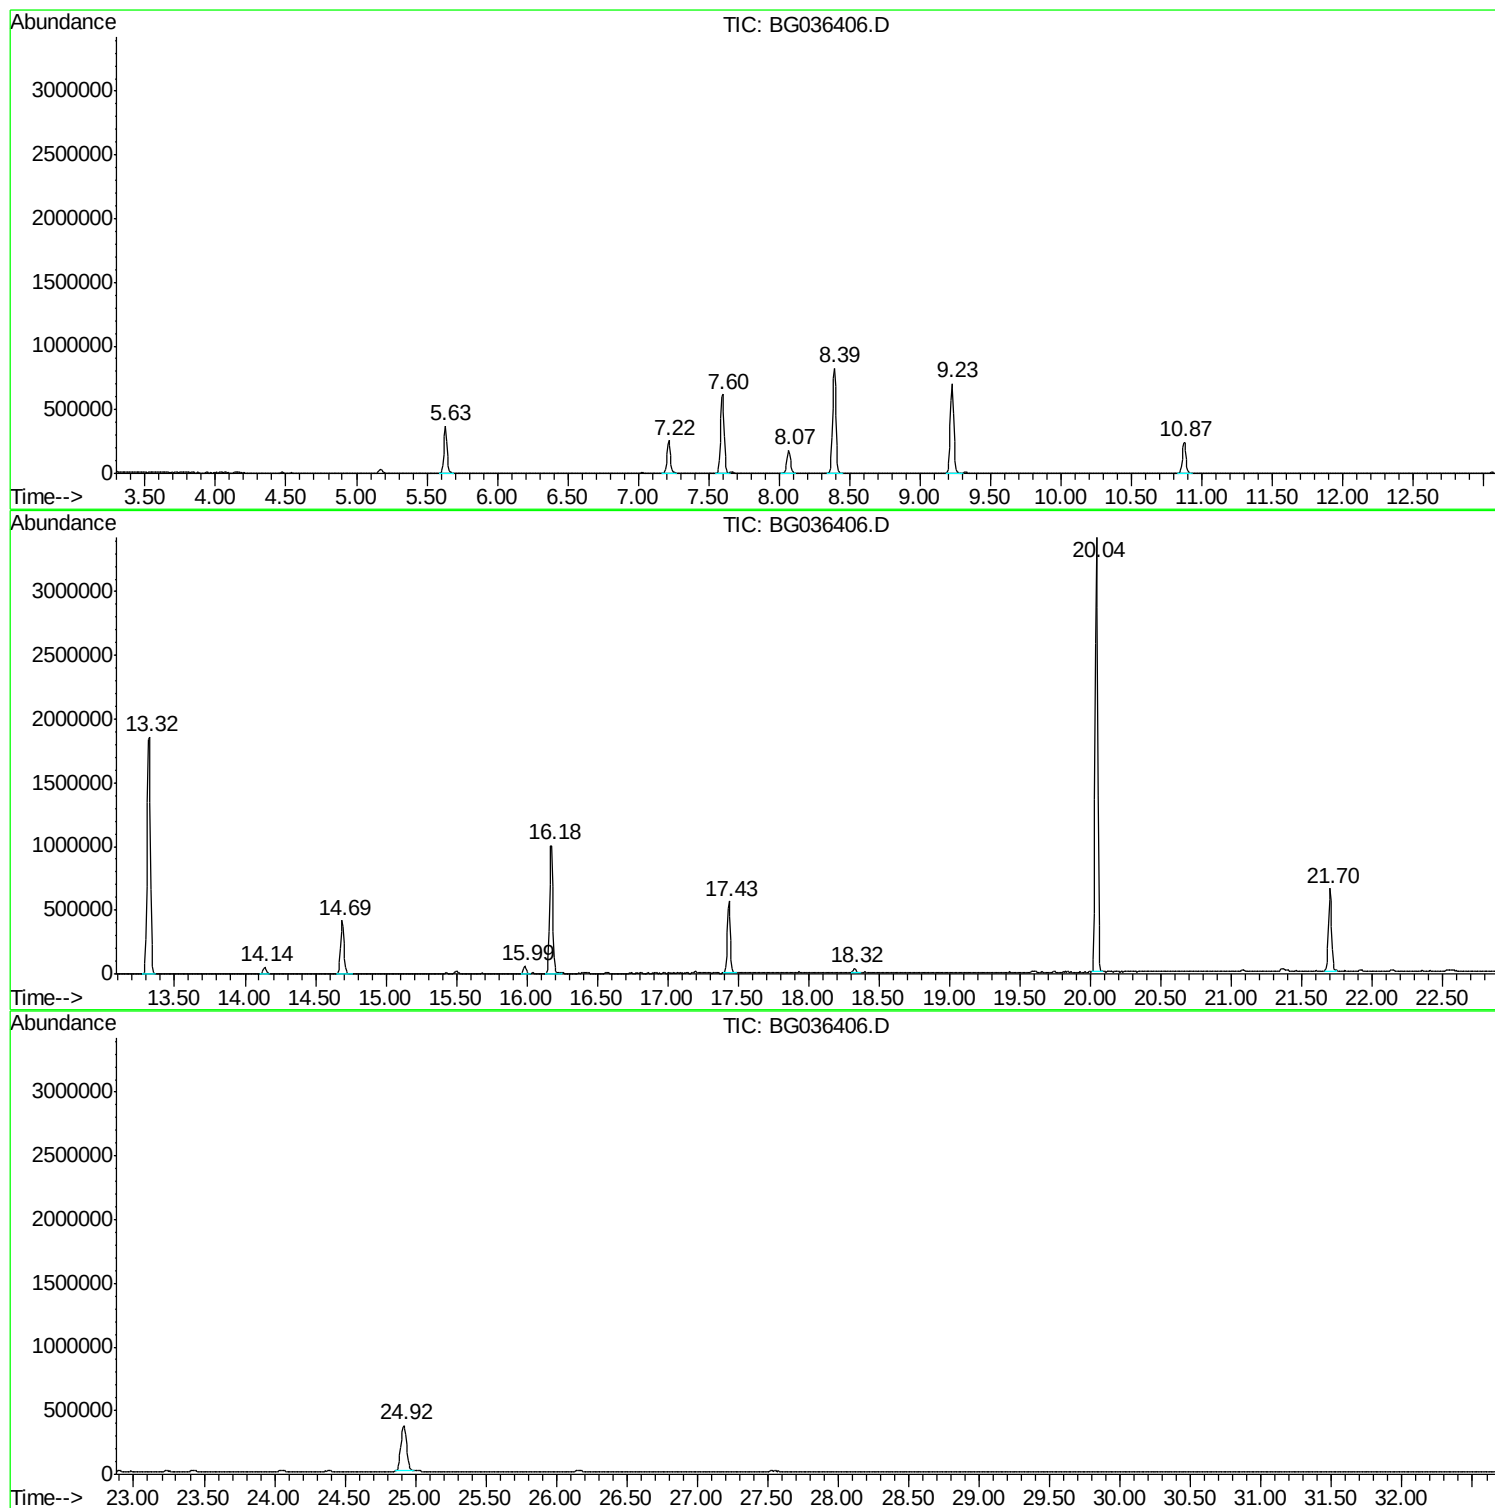

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082418\
Data File : BG036406.D
Acq On : 24 Aug 2018 9:52
Operator : JU/SJ
Sample : J4568-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
081718-SIDI-E-U-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.60 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	67.46 ng	1049850	1,4-Dichlorobenzene-d4	8.07

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
4		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5		Xenon	132	Xe	007440-63-3	9

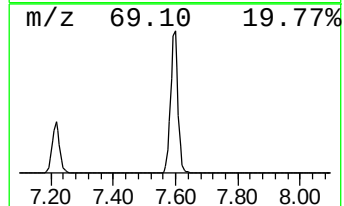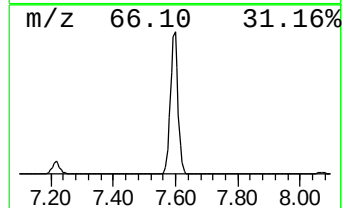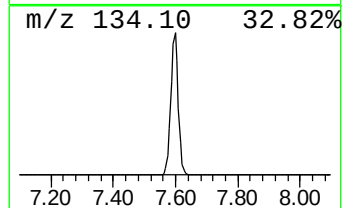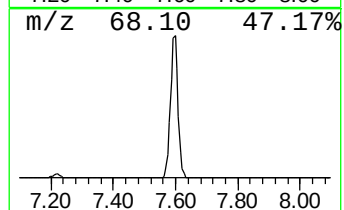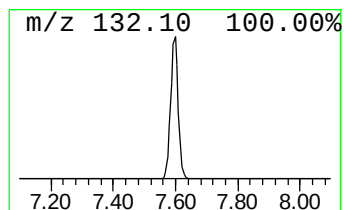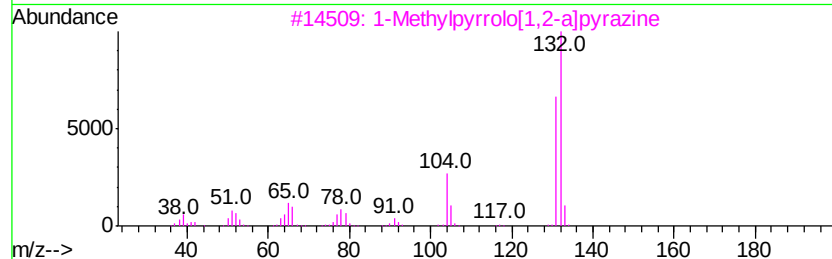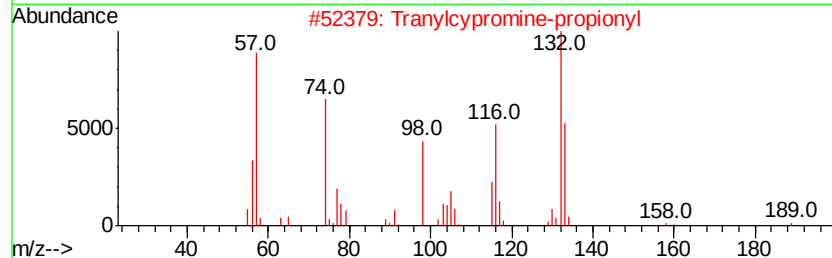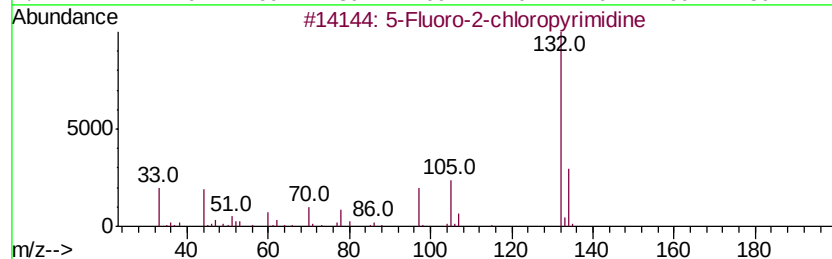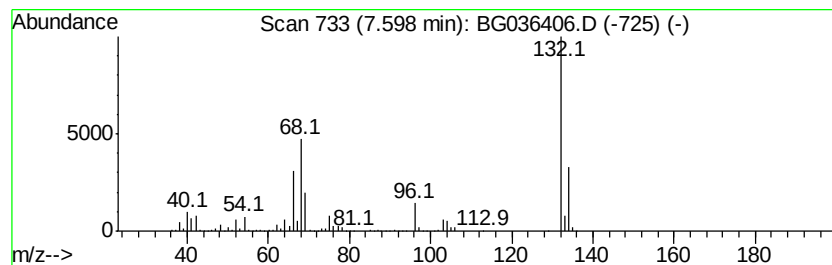

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082418\
Data File : BG036406.D
Acq On : 24 Aug 2018 9:52
Operator : JU/SJ
Sample : J4568-03
Misc :
ALS Vial : 27 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
081718-SIDI-E-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triethyl citrate Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.99	2.29 ng	75264	Acenaphthene-d10	14.69
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		Triethyl citrate	276 C12H20O7	000077-93-0 90
2		0-Acetylcitric acid triethyl ester	318 C14H22O8	000077-89-4 78
3		3-Chloro2-fluorobenzoic acid, 6-...	384 C22H34ClF02	1000338-65-3 50
4		3-Chloro2-fluorobenzoic acid, 3-...	370 C21H32ClF02	1000338-64-6 50
5		3-Chloro2-fluorobenzoic acid, 6-...	370 C21H32ClF02	1000338-64-9 42

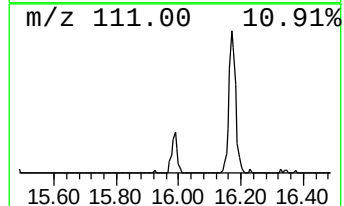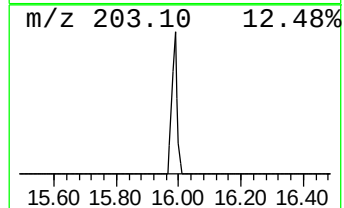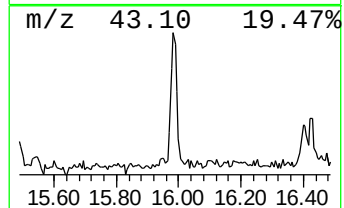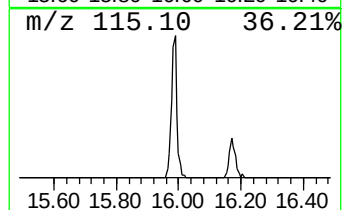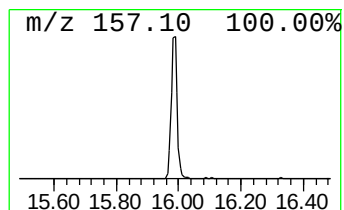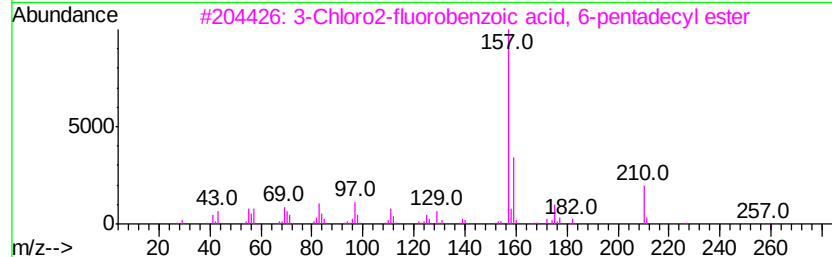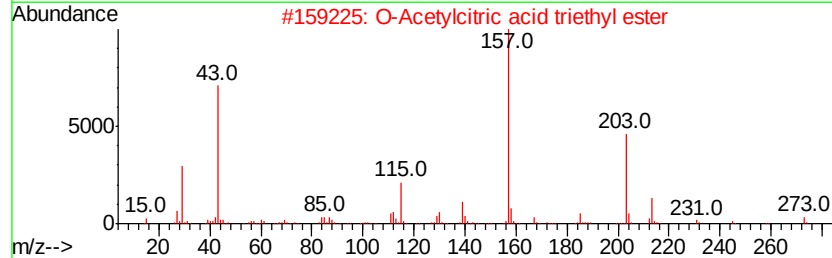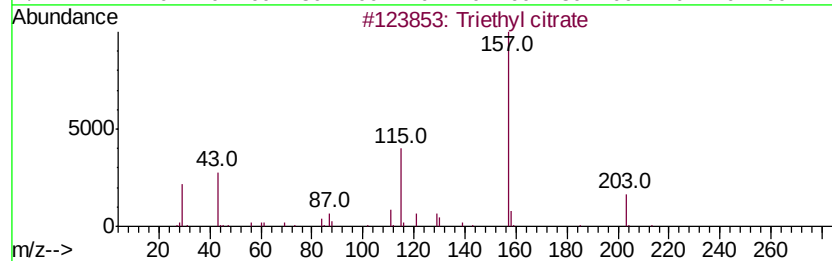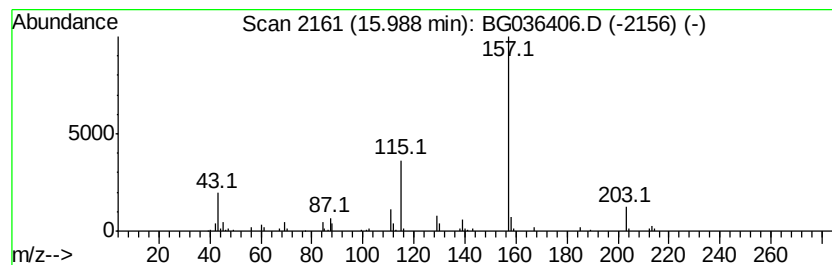

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082418\
Data File : BG036406.D
Acq On : 24 Aug 2018 9:52
Operator : JU/SJ
Sample : J4568-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
081718-SIDI-E-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.60	7.60	67.5	ng	1049850	1	8.07	311269	20.0
Triethyl citrate	15.99	2.3	ng	75264	3	14.69	655955	20.0