


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082418\
 Data File : BG036396.D
 Acq On : 24 Aug 2018 3:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

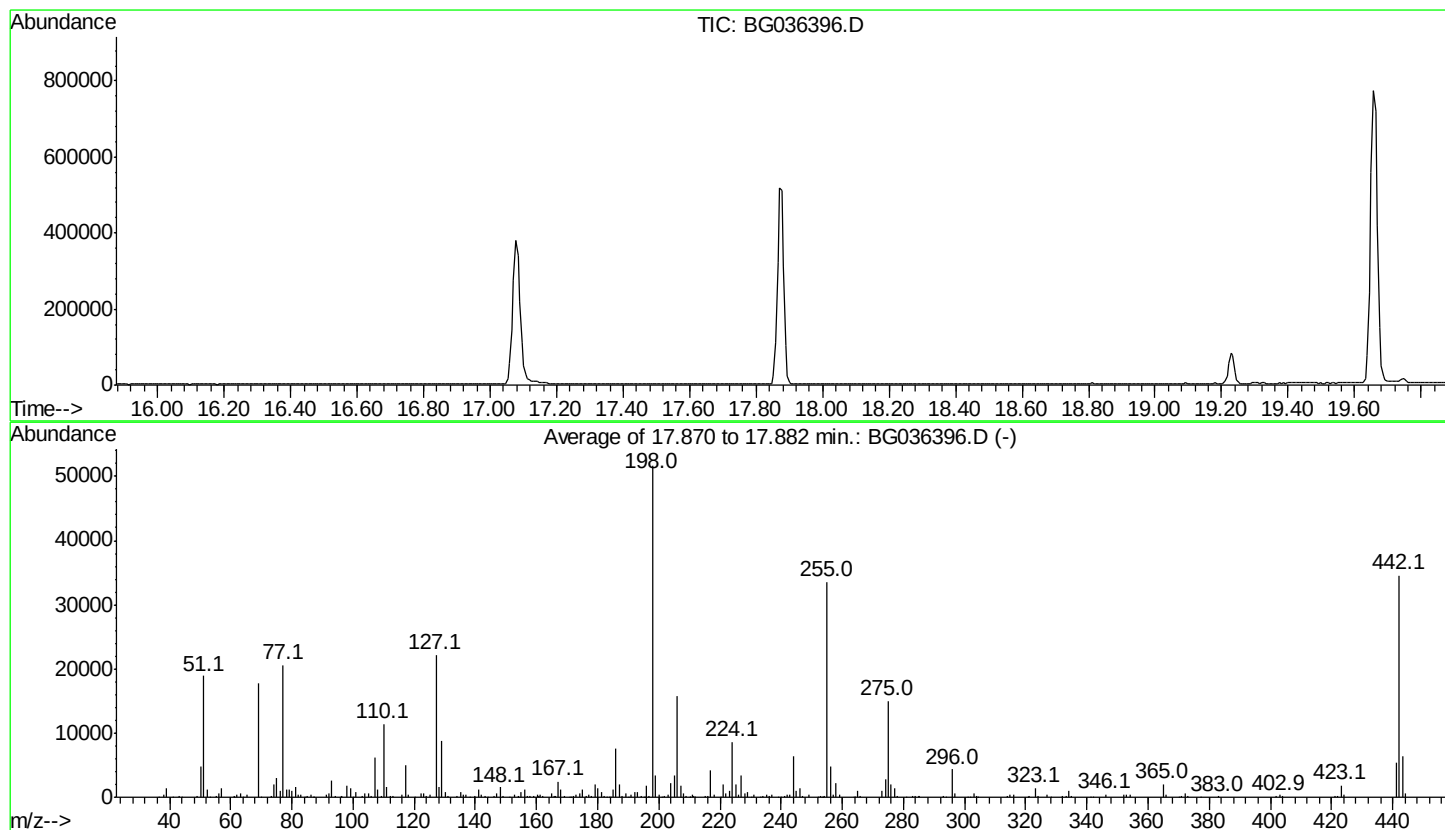

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	18947	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.3	17727	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	43.0	22203	PASS
197	198	0.00	2	0.3	161	PASS
198	198	100	100	100.0	51677	PASS
199	198	5	9	6.5	3384	PASS
275	198	10	60	29.0	14970	PASS
365	198	1	100	3.9	2029	PASS
441	198	0.01	100	10.6	5468	PASS
442	198	50	100	66.9	34573	PASS
443	442	15	24	18.6	6429	PASS