
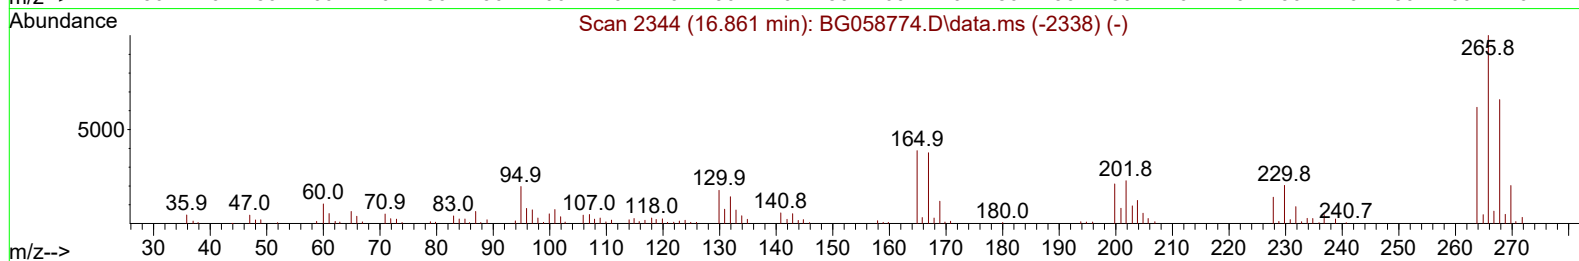
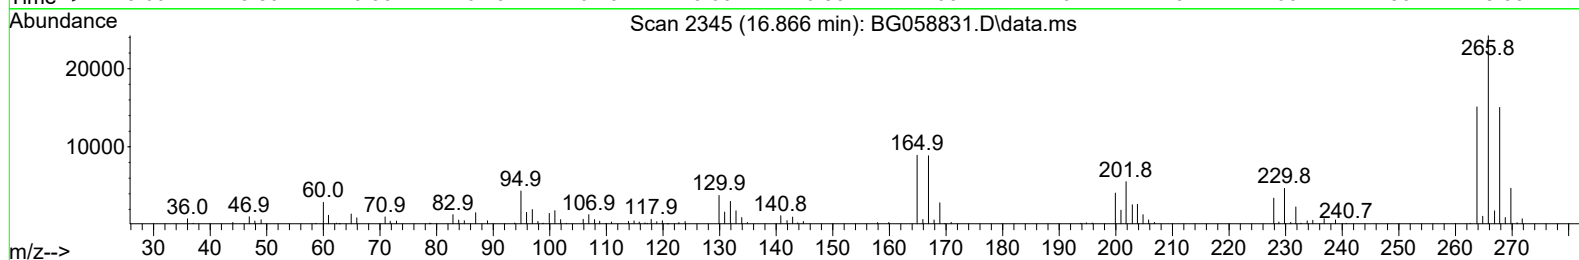


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082423\
Data File : BG058831.D
Acq On : 24 Aug 2023 9:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 10:54:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

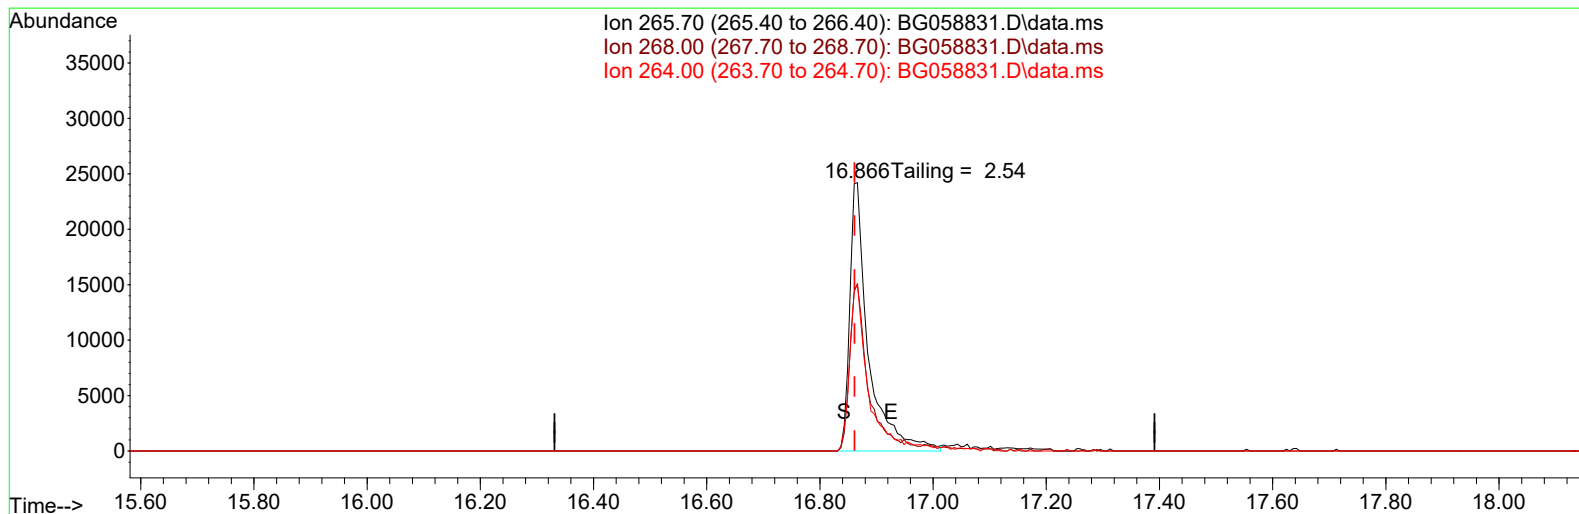

TIC: BG058831.D\data.ms

(70) Pentachlorophenol (C)




16.866min (+ 0.005) 21002.82 ng

response 55670

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.12
264.00	61.90	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082423\
Data File : BG058831.D
Acq On : 24 Aug 2023 9:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 10:54:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

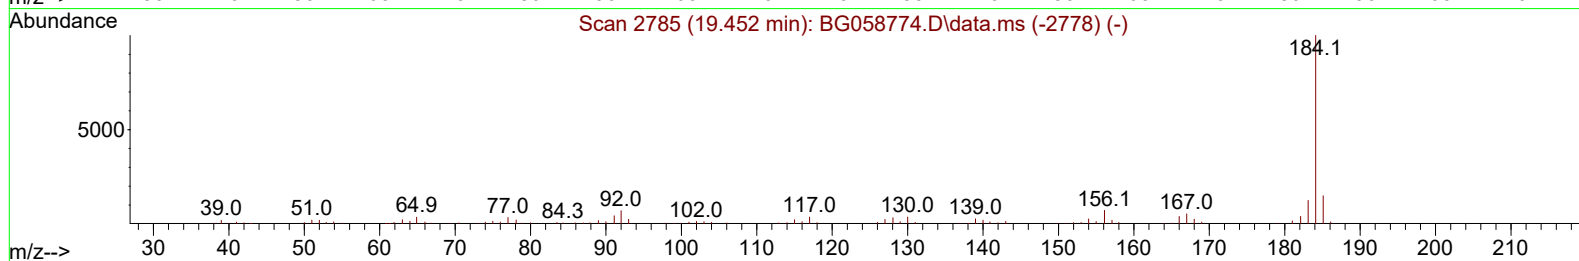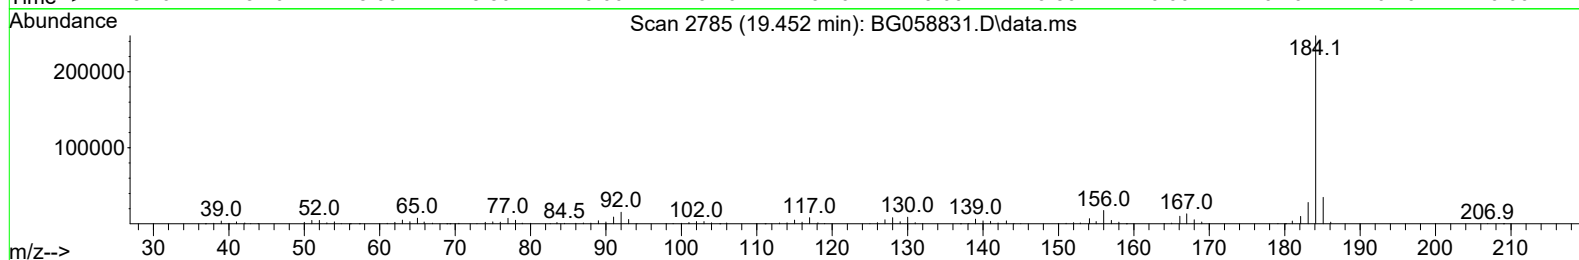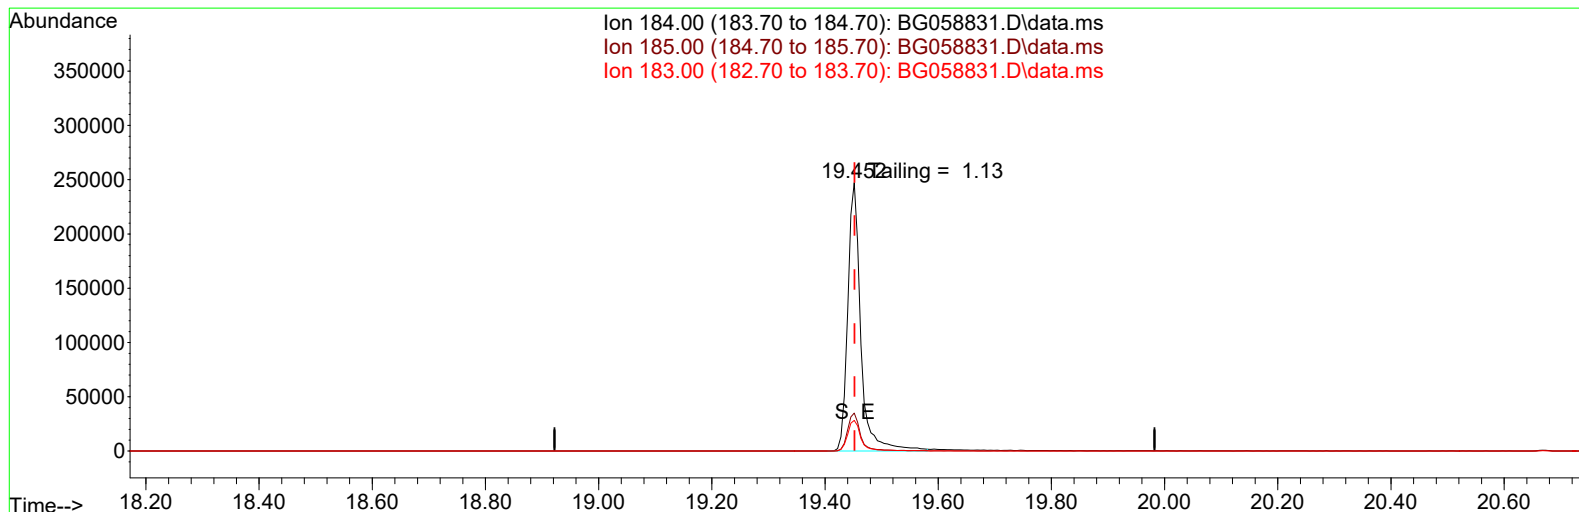

TIC: BG058831.D\data.ms

(77) Benzidine

19.452min (-0.000) 0.00 ng

response 396528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.12
183.00	12.50	11.41
0.00	0.00	0.00