


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082423\
Data File : BG058831.D
Acq On : 24 Aug 2023 9:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 21 01:40:57 2023

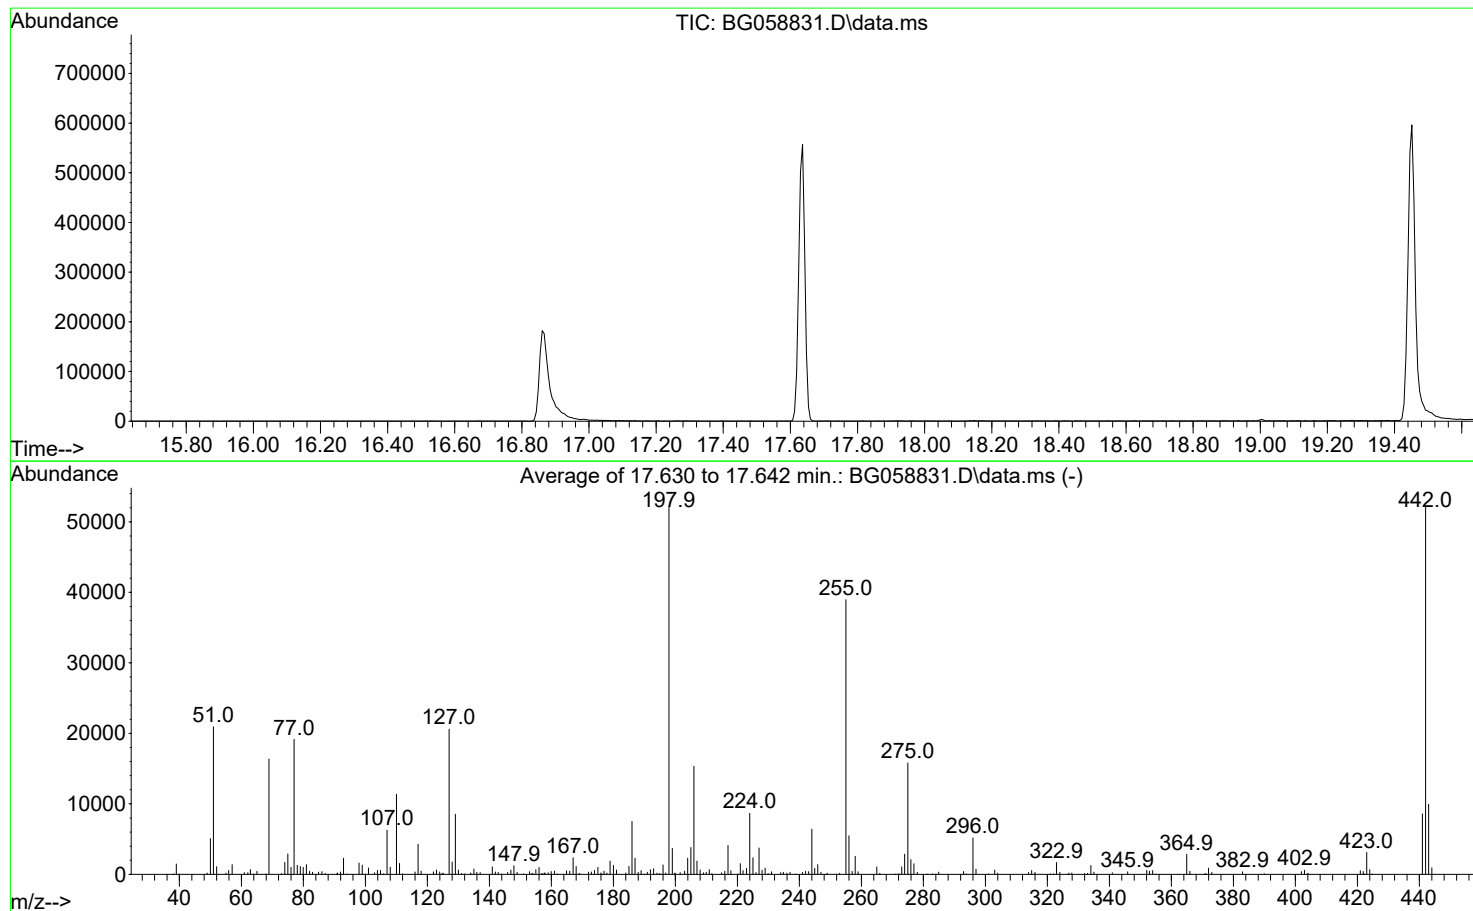




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	20916	PASS
68	69	0.00	2	0.5	79	PASS
69	198	0.00	100	31.4	16373	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.4	20580	PASS
197	198	0.00	2	0.4	199	PASS
198	198	100	100	100.0	52173	PASS
199	198	5	9	7.1	3685	PASS
275	198	10	60	30.3	15794	PASS
365	198	1	100	5.4	2835	PASS
441	198	0.01	100	16.5	8589	PASS
442	442	50	100	100.0	52085	PASS
443	442	15	24	19.1	9944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082423\
Data File : BG058831.D
Acq On : 24 Aug 2023 9:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 10:54:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

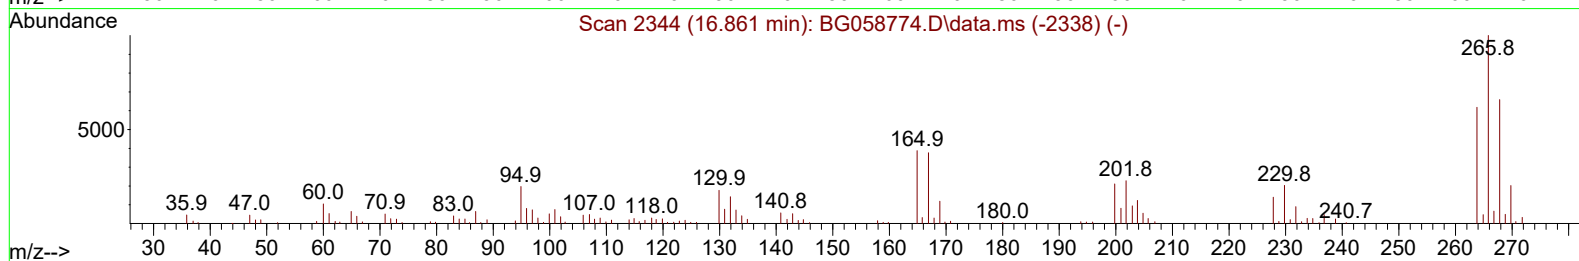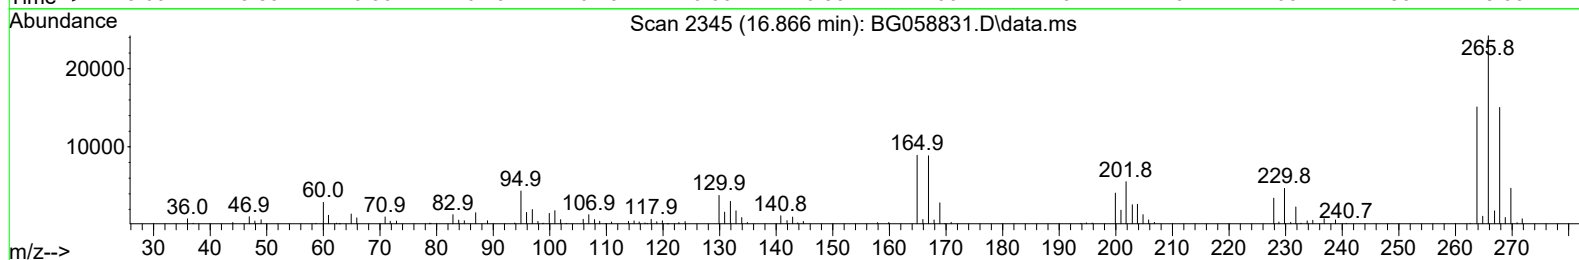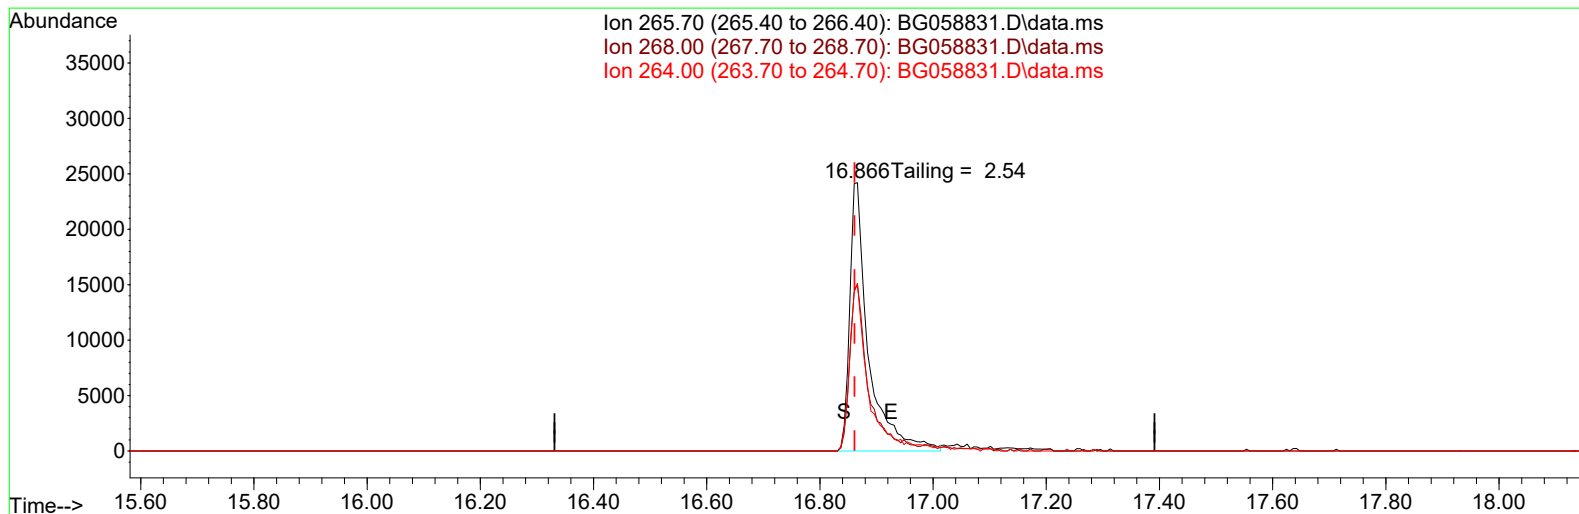

TIC: BG058831.D\data.ms

(70) Pentachlorophenol (C)

16.866min (+ 0.005) 21002.82 ng




response 55670

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.12
264.00	61.90	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082423\
Data File : BG058831.D
Acq On : 24 Aug 2023 9:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 10:54:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

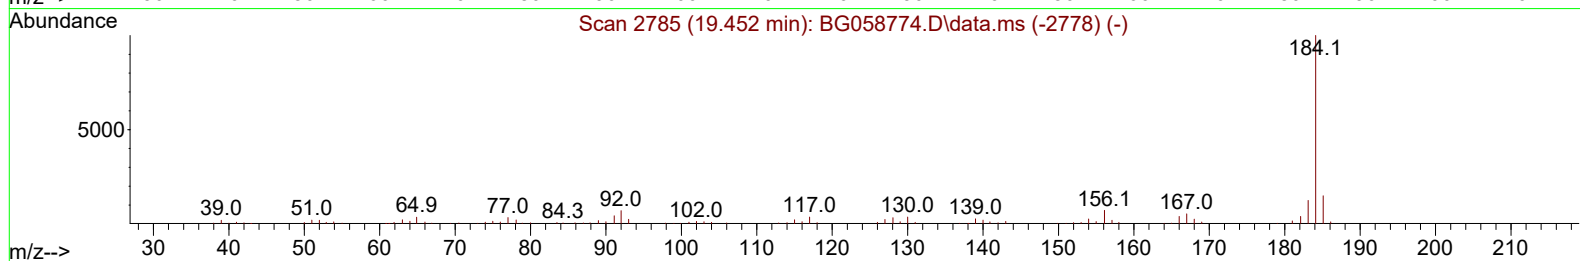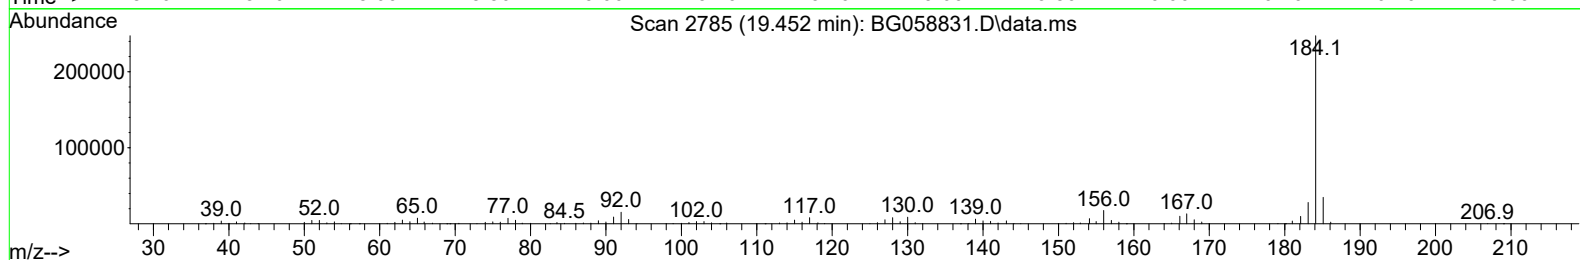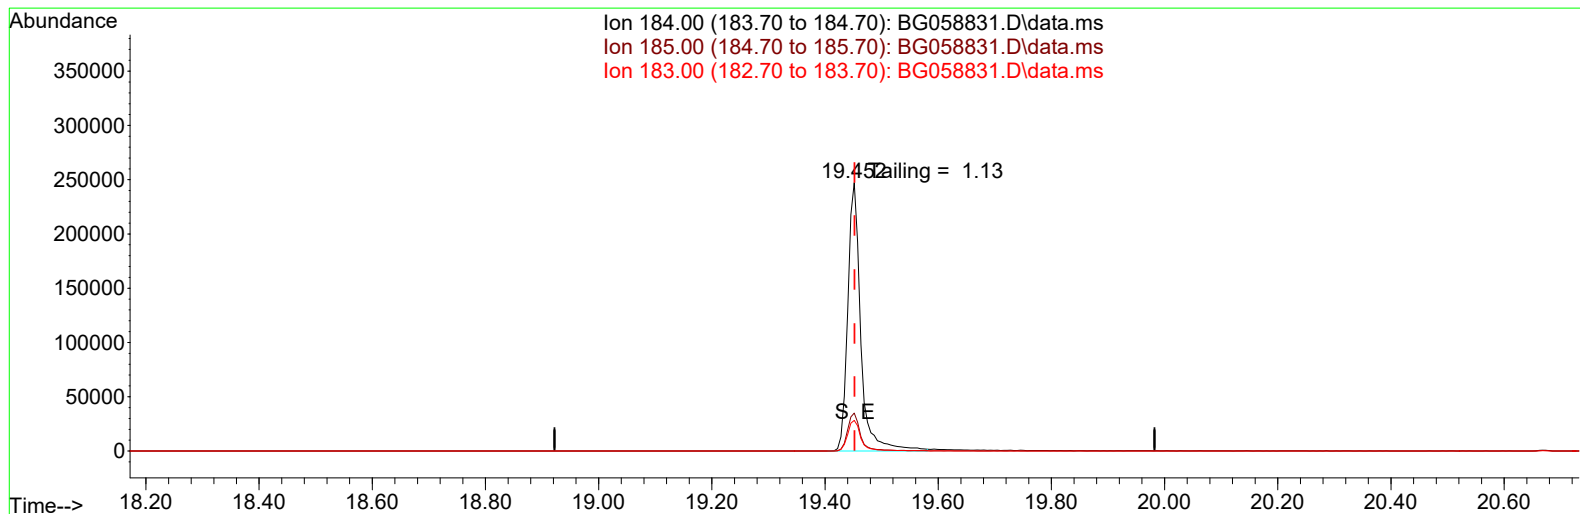

TIC: BG058831.D\data.ms

(77) Benzidine

19.452min (-0.000) 0.00 ng

response 396528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.12
183.00	12.50	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2023	BNA_G	<u>BG058831.D</u>
Compound Name	Response	Retention Time
DDT	197396	20.668
DDD	4421	20.239
DDE	367	19.722
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4788	202184	2.37

Instrument :
BNA_G
ClientSampleId :
DFTPP