
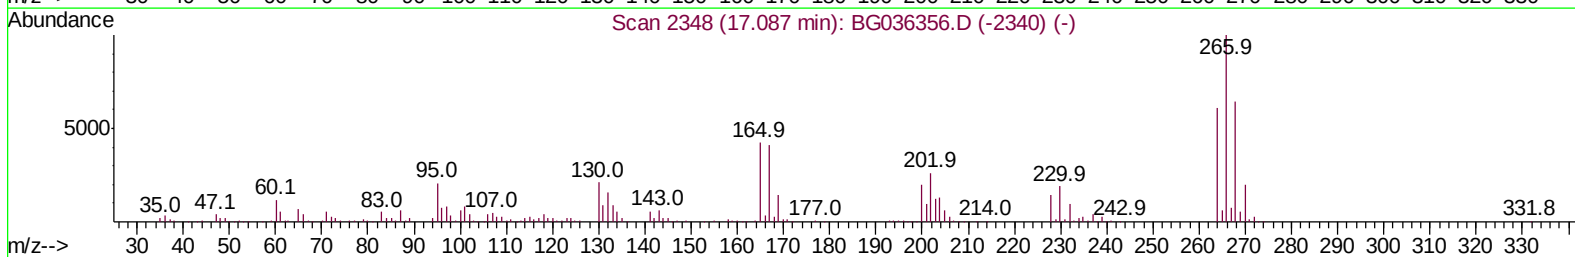
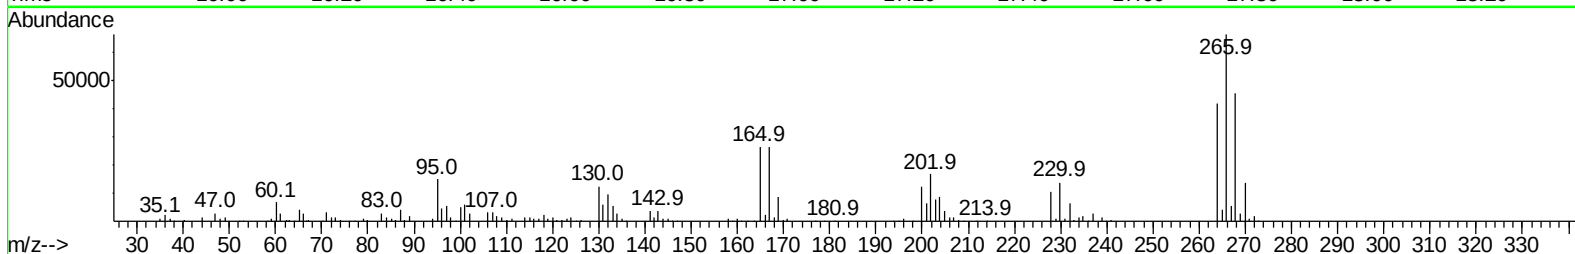


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082518\
Data File : BG036415.D
Acq On : 24 Aug 2018 16:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 03:16:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

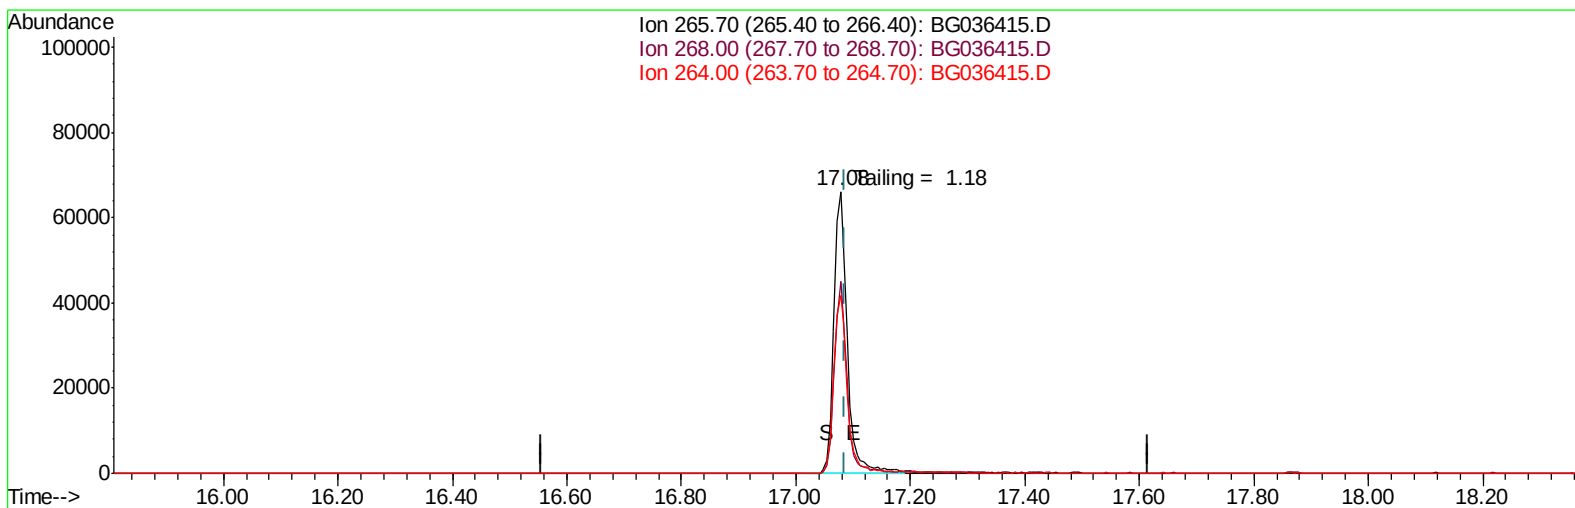

TIC: BG036415.D

(69) Pentachlorophenol (C)




17.078min (-0.009) 32836.89ng

response 107405

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	68.27
264.00	61.10	63.14
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082518\
 Data File : BG036415.D
 Acq On : 24 Aug 2018 16:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 03:16:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 12:07:02 2018
 Response via : Initial Calibration

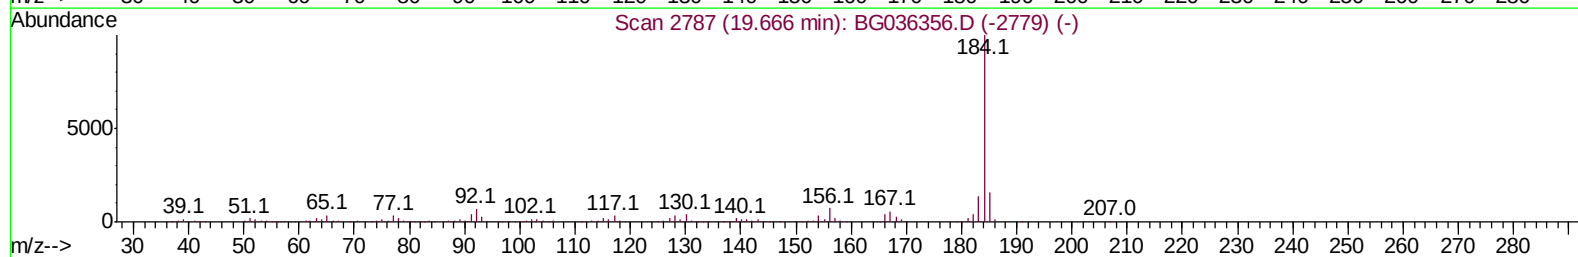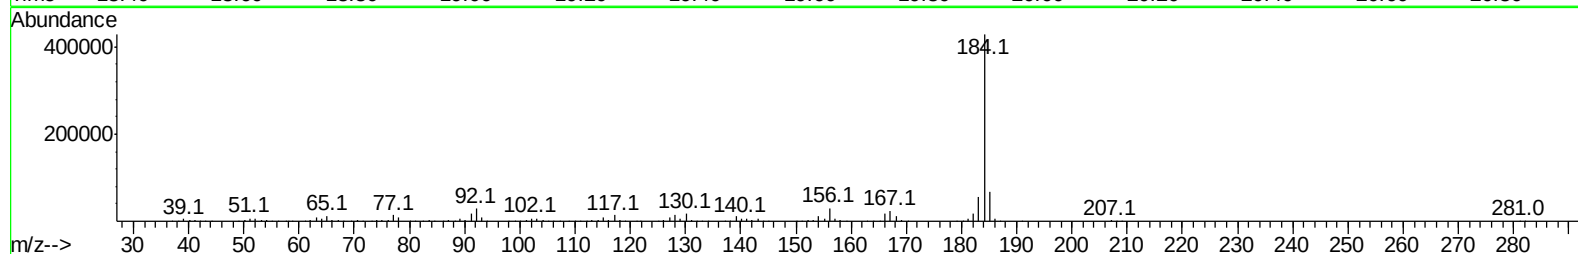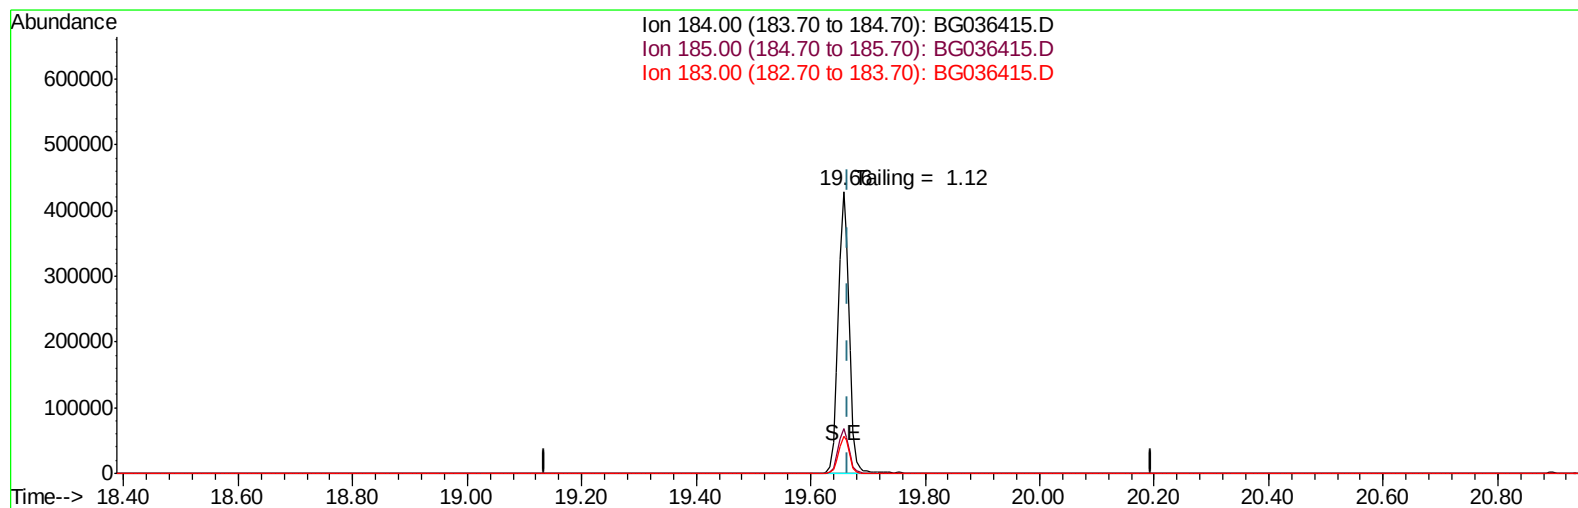

TIC: BG036415.D

(76) Benzidine

19.657min (-0.009) 0.00ng

response 574151

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.95
183.00	13.60	13.17
0.00	0.00	0.00