


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082518\
 Data File : BG036415.D
 Acq On : 24 Aug 2018 16:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

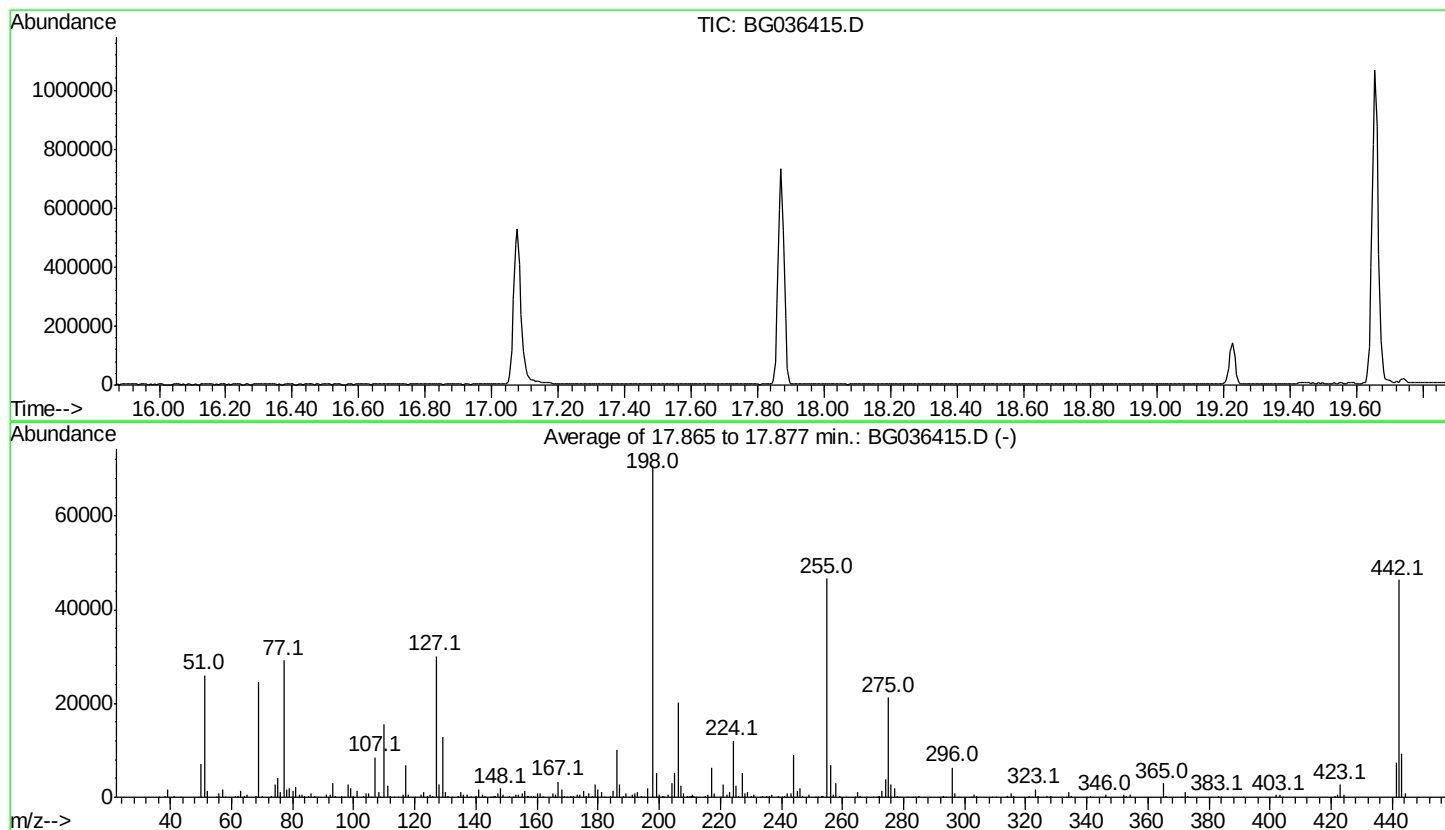

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	26045	PASS
68	69	0.00	2	1.6	391	PASS
69	198	0.00	100	34.8	24642	PASS
70	69	0.00	2	0.7	165	PASS
127	198	10	80	42.5	30064	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70725	PASS
199	198	5	9	7.2	5097	PASS
275	198	10	60	30.1	21285	PASS
365	198	1	100	4.2	2969	PASS
441	198	0.01	100	10.5	7444	PASS
442	198	50	100	65.6	46402	PASS
443	442	15	24	20.2	9355	PASS