


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082518\
 Data File : BG036420.D
 Acq On : 25 Aug 2018 10:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

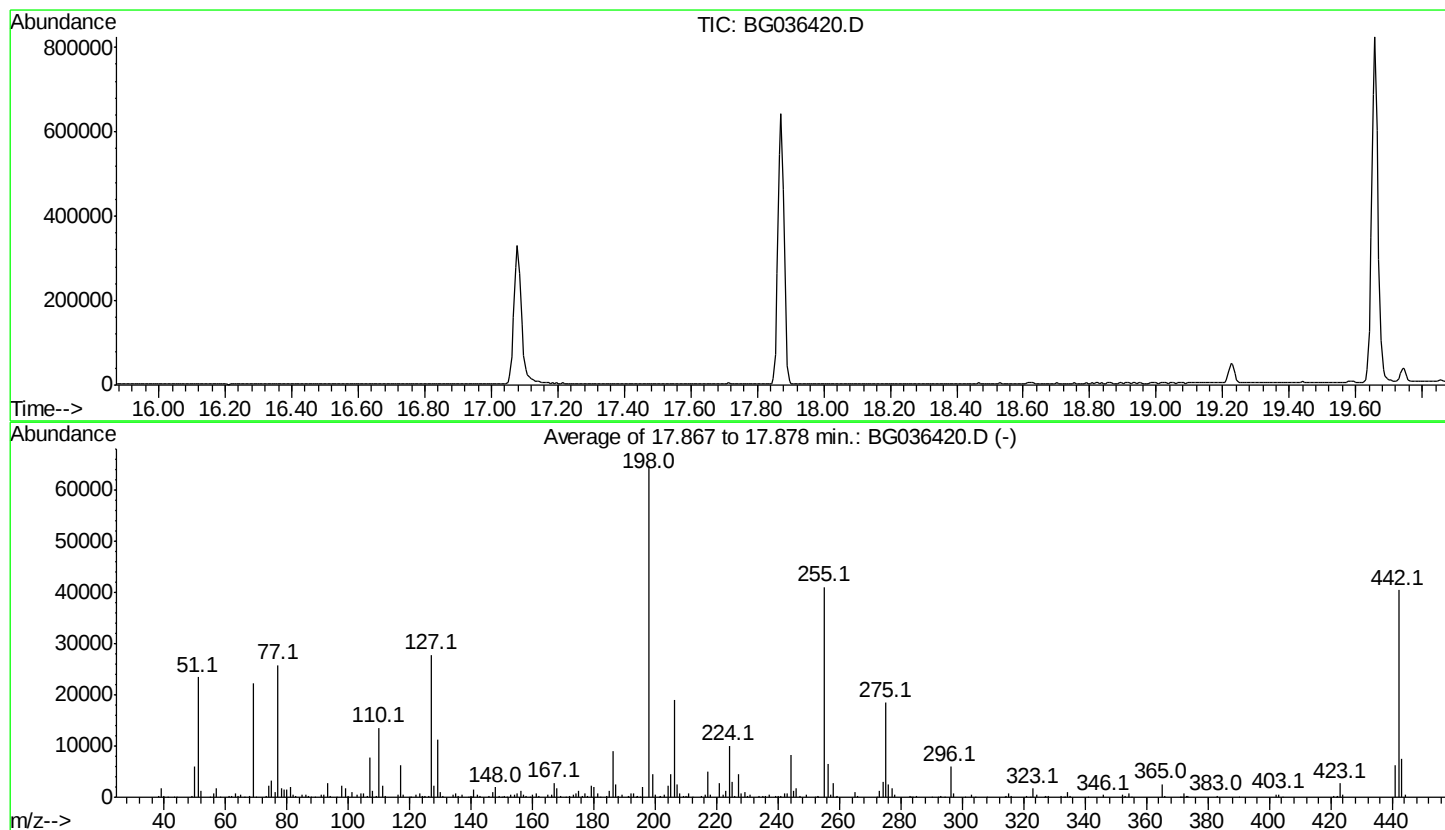

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	23450	PASS
68	69	0.00	2	1.3	286	PASS
69	198	0.00	100	34.5	22373	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	43.0	27925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64874	PASS
199	198	5	9	6.9	4493	PASS
275	198	10	60	28.4	18426	PASS
365	198	1	100	4.0	2577	PASS
441	198	0.01	100	9.8	6345	PASS
442	198	50	100	62.4	40466	PASS
443	442	15	24	18.8	7590	PASS