
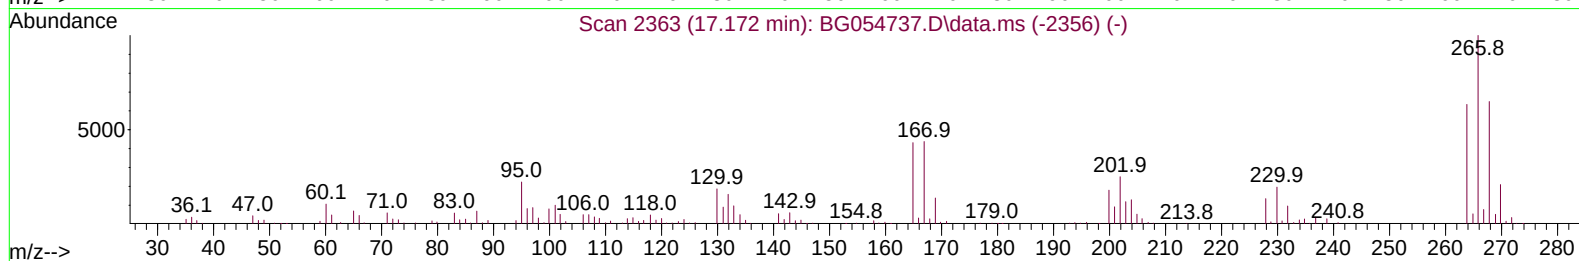
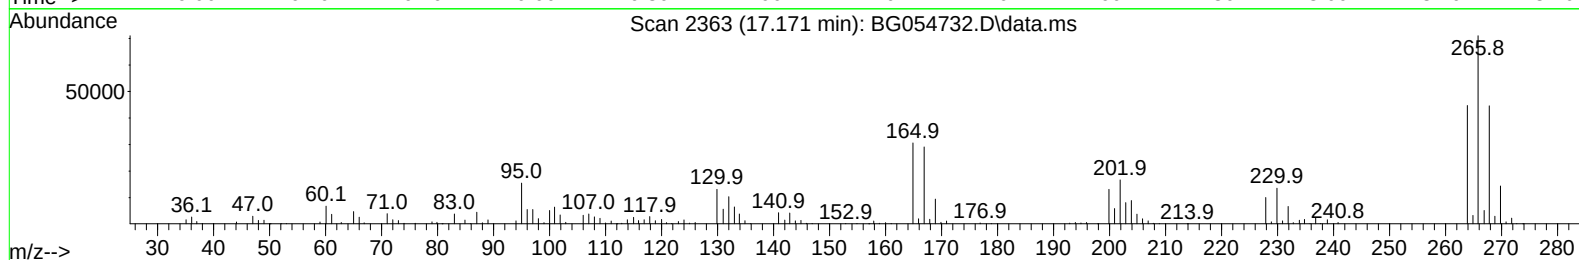


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
Data File : BG054732.D
Acq On : 25 Aug 2022 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 17:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 16:00:11 2022
Response via : Initial Calibration

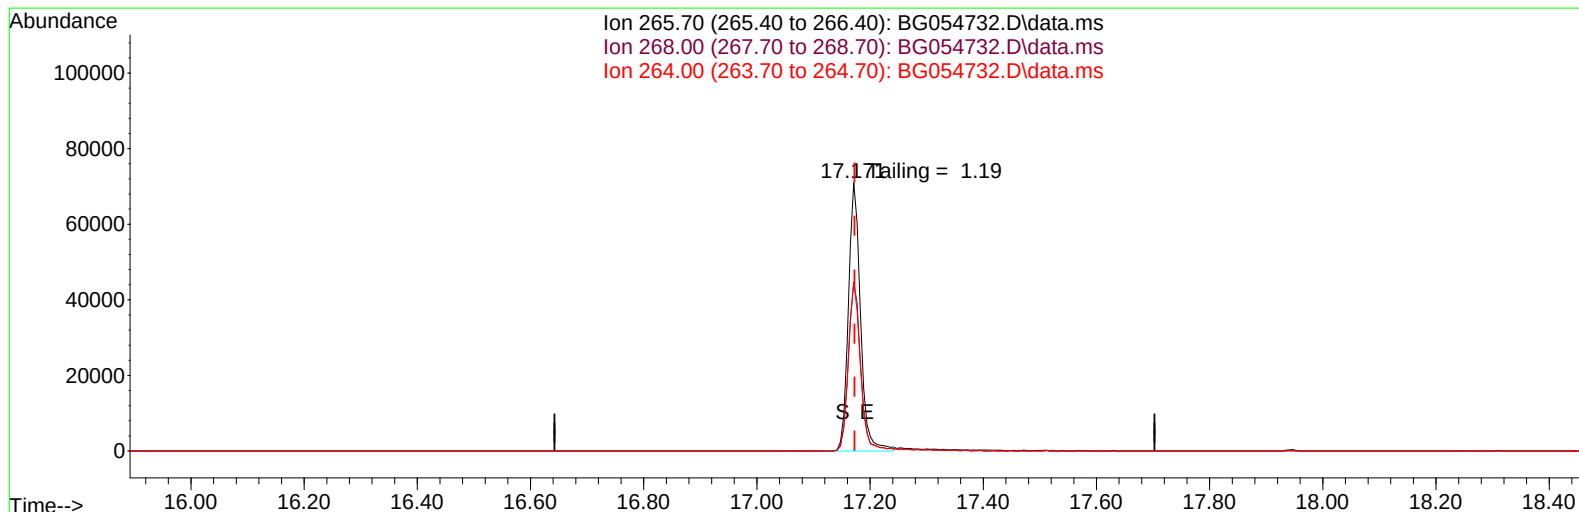

TIC: BG054732.D\data.ms

(70) Pentachlorophenol (C)




17.171min (-0.001) 79777.43 ng

response 107871

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.82
264.00	61.70	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
Data File : BG054732.D
Acq On : 25 Aug 2022 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 17:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 16:00:11 2022
Response via : Initial Calibration

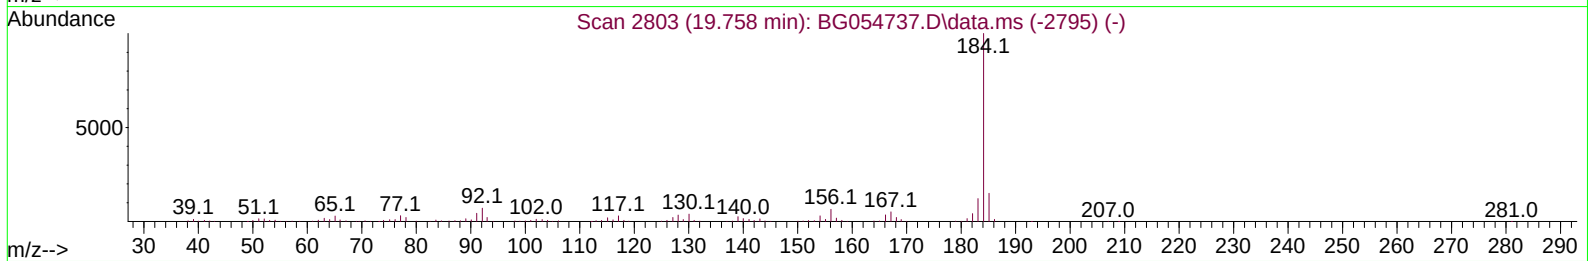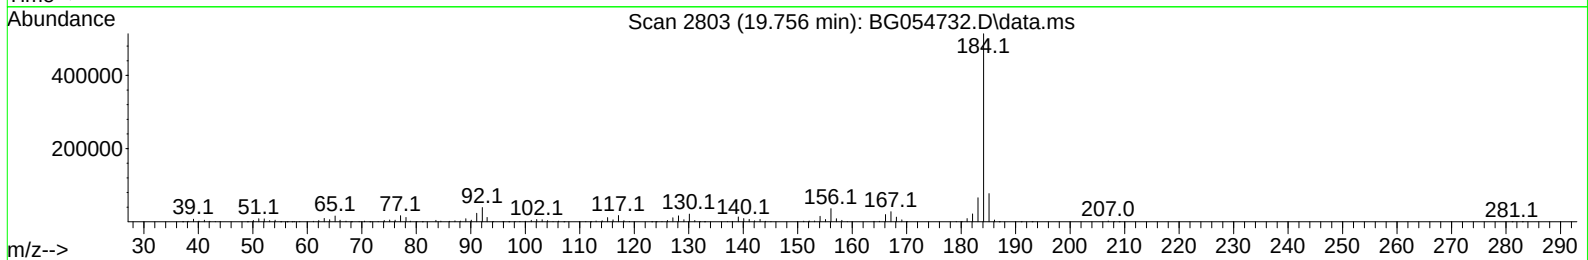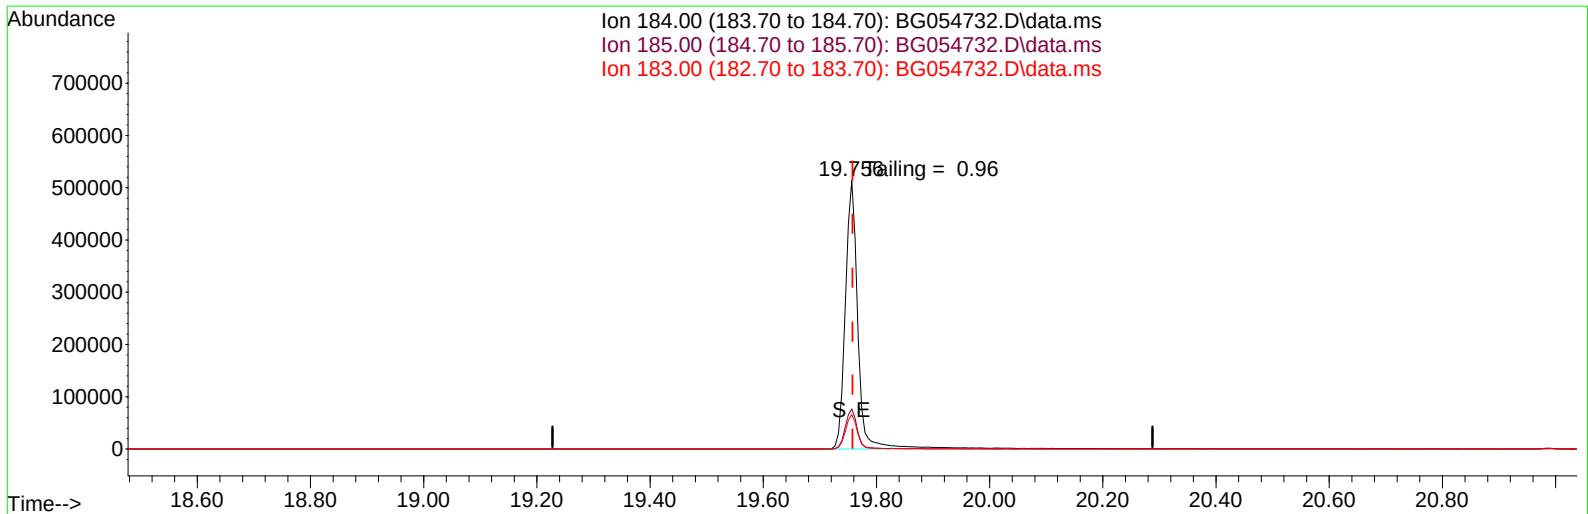

TIC: BG054732.D\data.ms

(77) Benzidine

19.756min (-0.001) 615084.70 ng

response 787938

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.99
183.00	12.30	12.83
0.00	0.00	0.00