

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
 Data File : BG054742.D
 Acq On : 25 Aug 2022 19:06
 Operator : CG/JU
 Sample : PB147245BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB147245BL

Quant Time: Aug 26 05:17:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 17:50:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.148	152	50122	20.000	ng	0.00
21) Naphthalene-d8	10.974	136	199766	20.000	ng	0.00
39) Acenaphthene-d10	14.781	164	132264	20.000	ng	0.00
64) Phenanthrene-d10	17.525	188	319709	20.000	ng	0.00
76) Chrysene-d12	21.820	240	328244	20.000	ng	0.00
86) Perylene-d12	25.181	264	334840	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.686	112	393292	136.639	ng	0.00
7) Phenol-d6	7.296	99	519591	131.998	ng	0.00
23) Nitrobenzene-d5	9.323	82	317869	83.533	ng	0.00
42) 2,4,6-Tribromophenol	16.268	330	216235	130.835	ng	0.00
45) 2-Fluorobiphenyl	13.412	172	743274	84.464	ng	0.00
79) Terphenyl-d14	20.128	244	1423554	85.930	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
Data File : BG054742.D
Acq On : 25 Aug 2022 19:06
Operator : CG/JU
Sample : PB147245BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB147245BL

Quant Time: Aug 26 05:17:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration




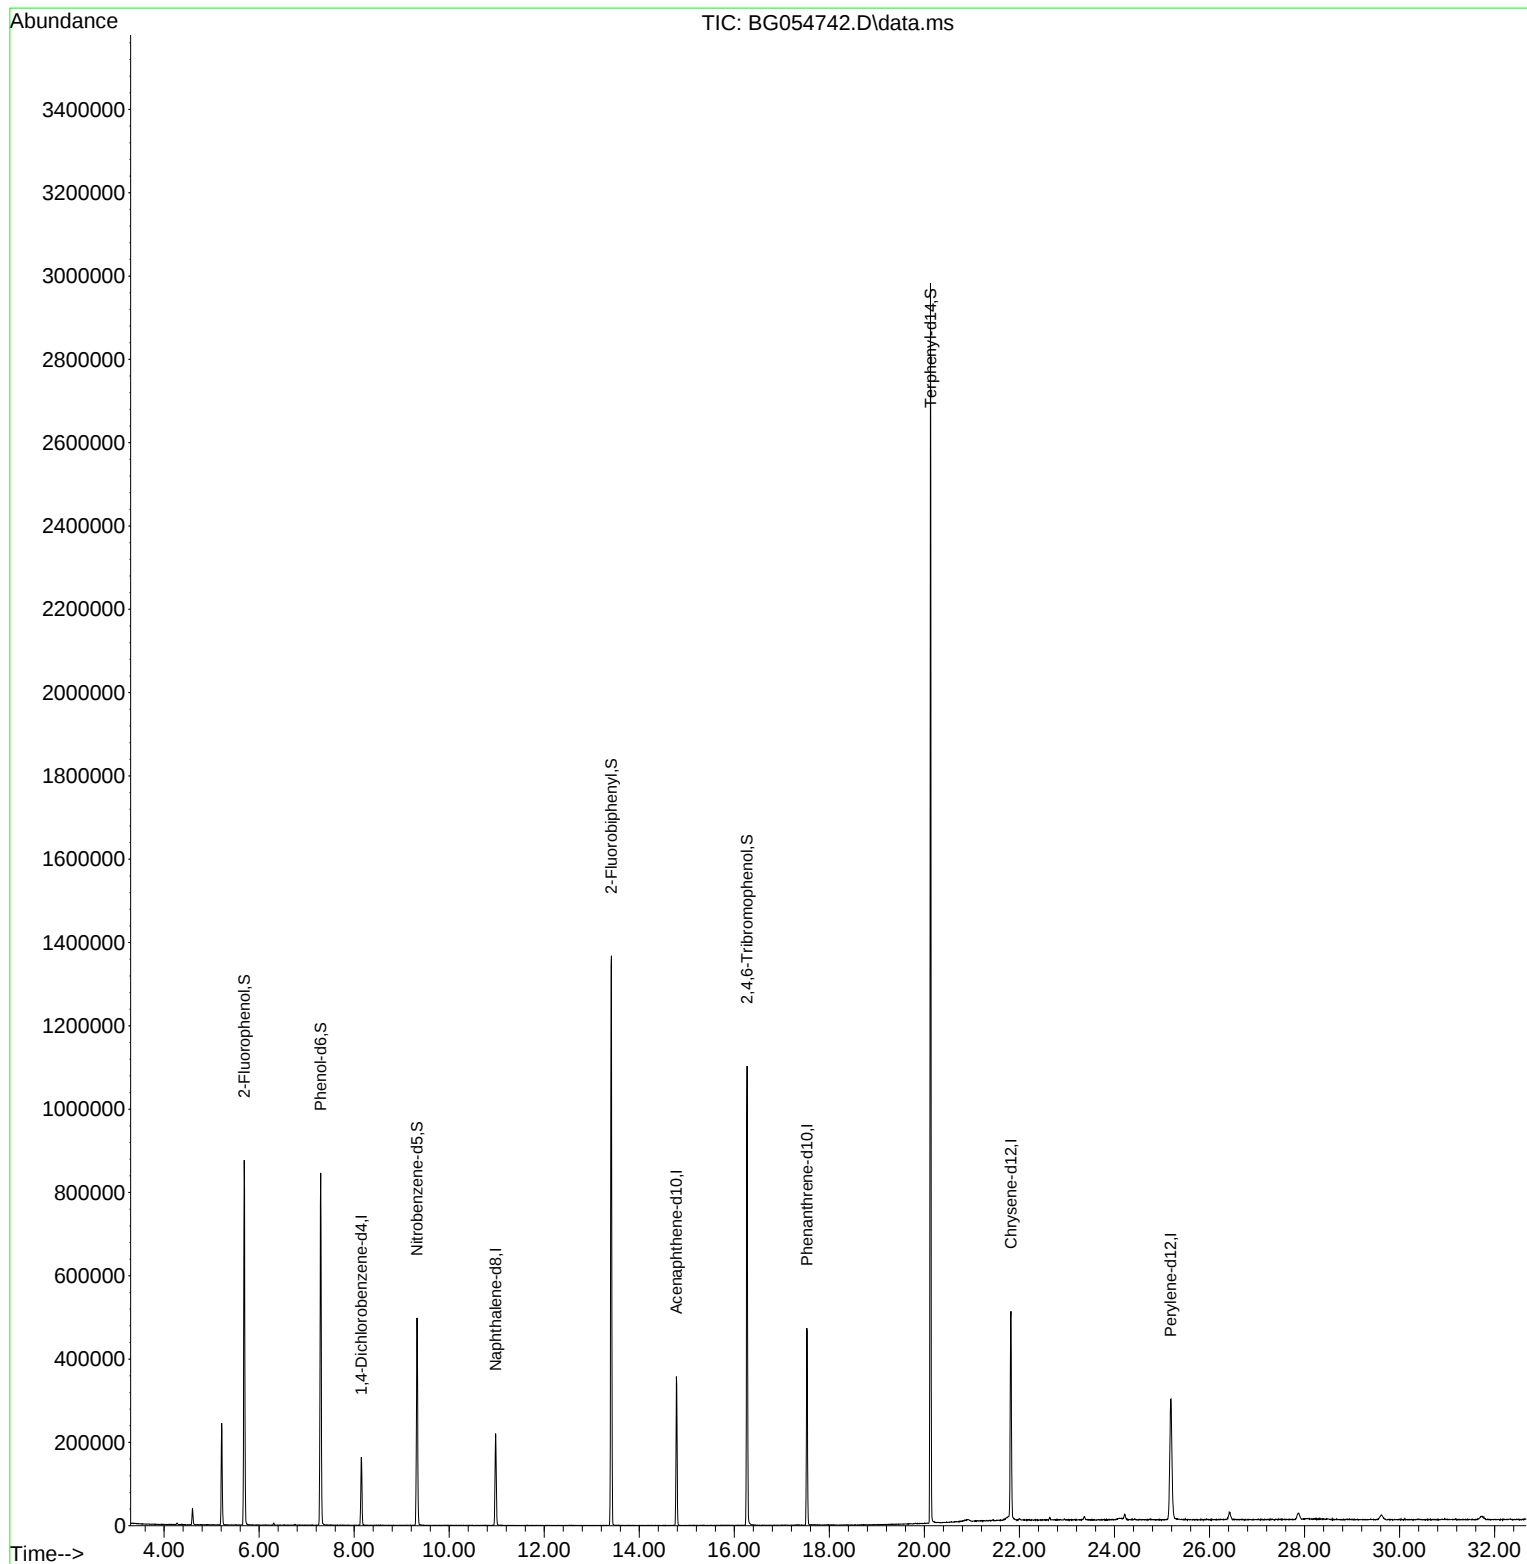




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.148 min Scan# 81
Delta R.T. -0.005 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06




Instrument :
BNA_G
ClientSampleId :
PB147245BL

Tgt Ion:152 Resp: 50122
Ion Ratio Lower Upper
152 100
150 157.7 125.2 187.8
115 55.3 47.9 71.9

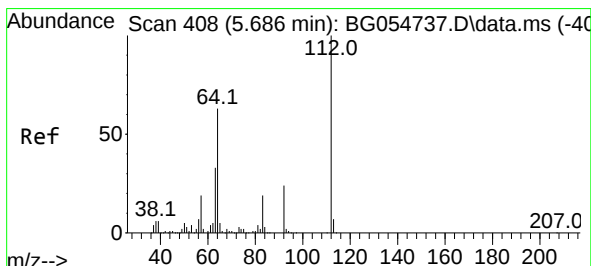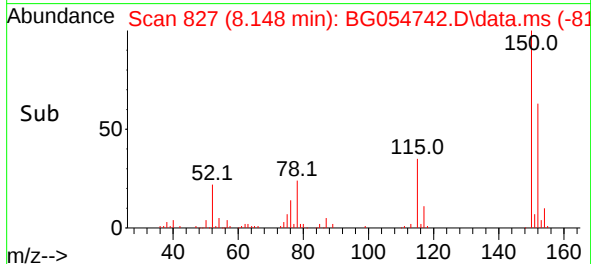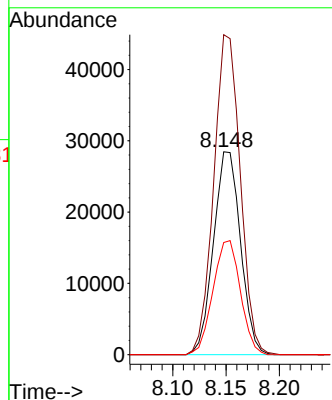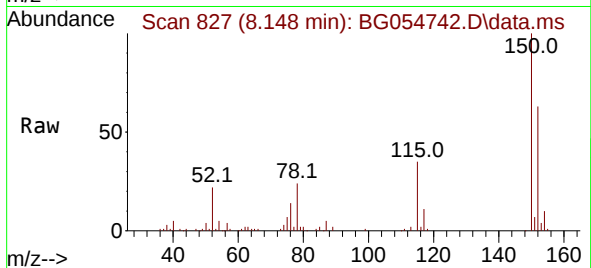

#5
2-Fluorophenol
Concen: 136.639 ng
RT: 5.686 min Scan# 408
Delta R.T. 0.000 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06

Tgt Ion:112 Resp: 393292
Ion Ratio Lower Upper
112 100
64 64.0 49.3 73.9
63 33.4 26.3 39.5


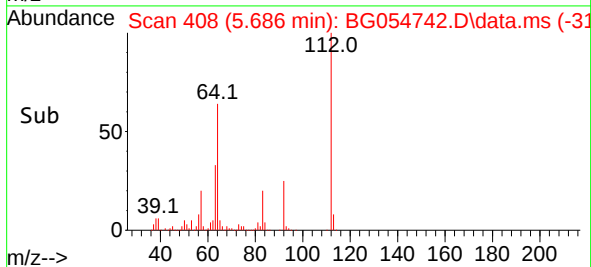
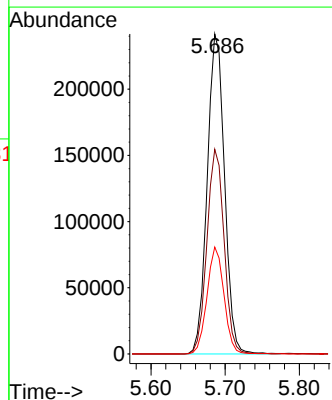
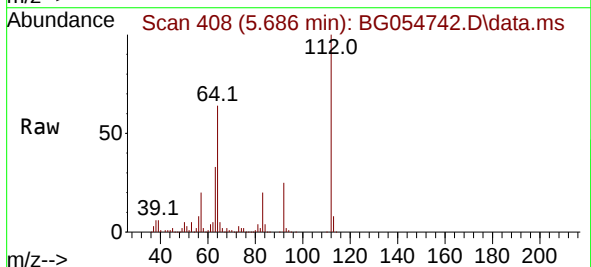




#7
Phenol-d6
Concen: 131.998 ng
RT: 7.296 min Scan# 61
Delta R.T. 0.000 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06




Instrument :
BNA_G
ClientSampleId :
PB147245BL


Tgt Ion: 99 Resp: 519591
Ion Ratio Lower Upper
99 100
42 17.9 14.6 22.0
71 31.4 24.6 37.0

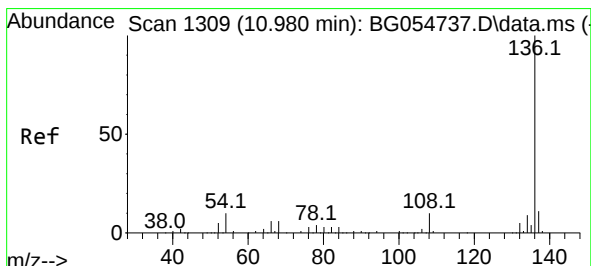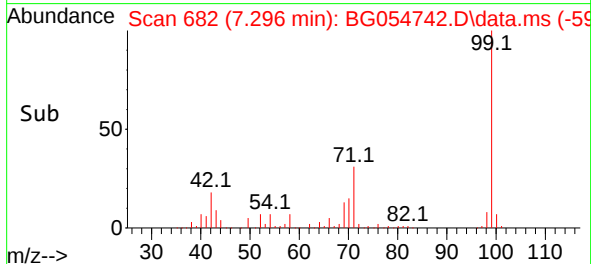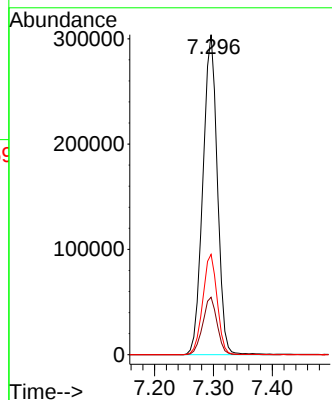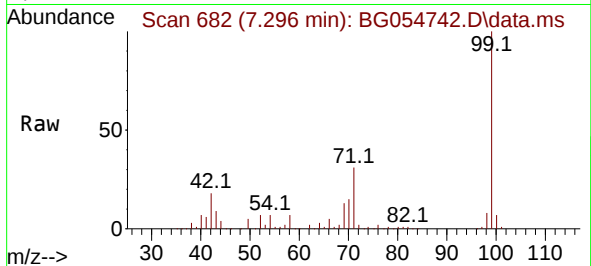

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.974 min Scan# 1308
Delta R.T. -0.006 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06

Tgt Ion: 136 Resp: 199766
Ion Ratio Lower Upper
136 100
137 11.2 9.2 13.8
54 9.0 7.7 11.5
68 6.2 5.6 8.4

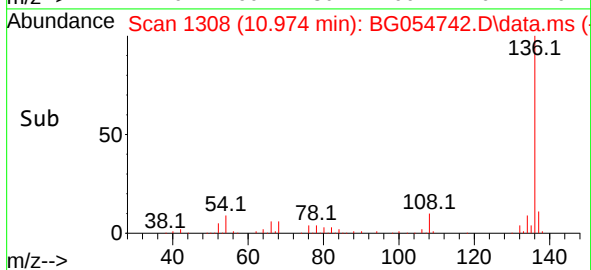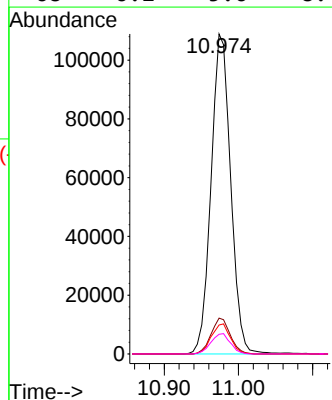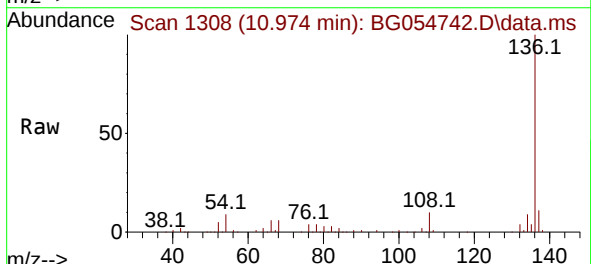

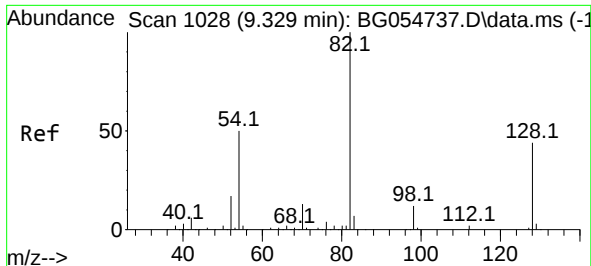

#23
Nitrobenzene-d5
Concen: 83.533 ng
RT: 9.323 min Scan# 1027
Delta R.T. -0.006 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06





Instrument :

BNA_G

ClientSampleId :




PB147245BL


Tgt Ion: 82 Resp: 317869
Ion Ratio Lower Upper
82 100
128 42.8 32.2 48.2
54 50.3 41.4 62.0

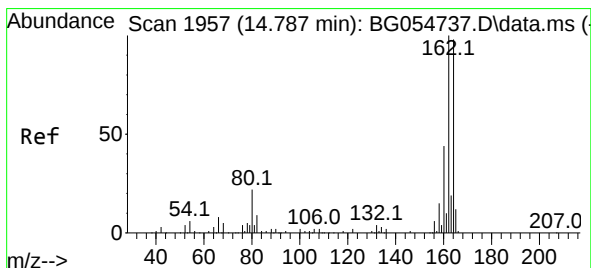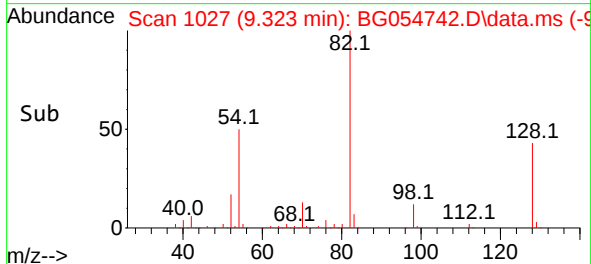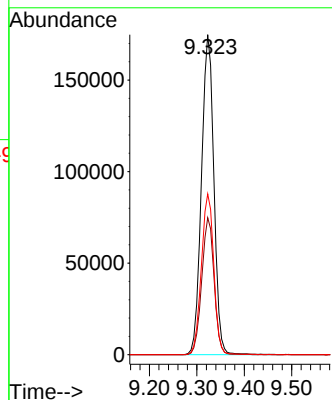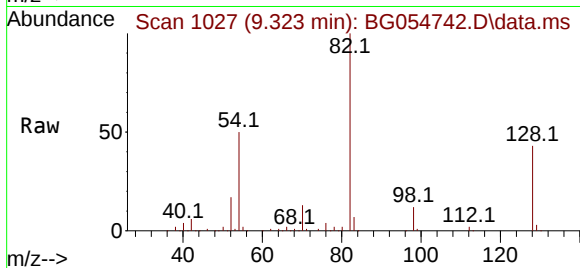

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.781 min Scan# 1956
Delta R.T. -0.006 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06


Tgt Ion:164 Resp: 132264
Ion Ratio Lower Upper
164 100
162 101.4 83.0 124.4
160 47.4 38.0 57.0

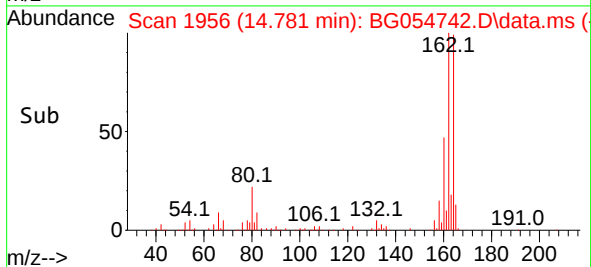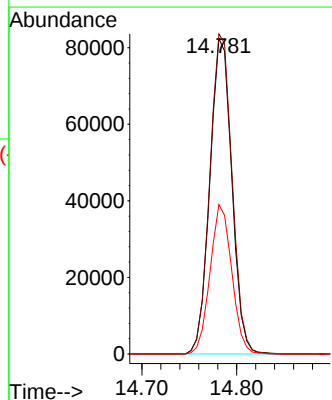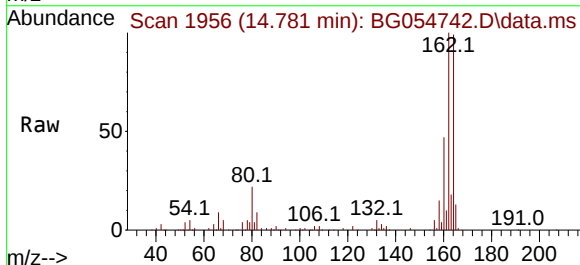



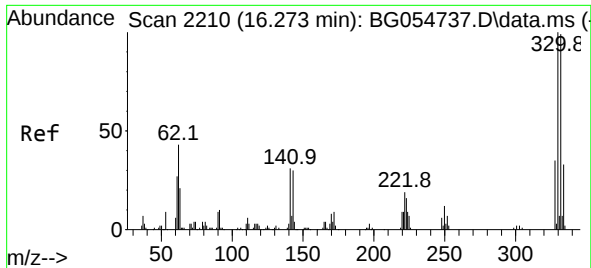


#42
2,4,6-Tribromophenol
Concen: 130.835 ng
RT: 16.268 min Scan# 21
Delta R.T. -0.006 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06

Instrument :
BNA_G
ClientSampleId :
PB147245BL



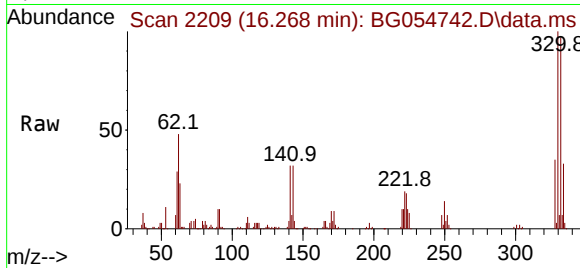



Tgt Ion:330 Resp: 216235
Ion Ratio Lower Upper
330 100
332 97.5 79.8 119.6
141 32.9 26.8 40.2

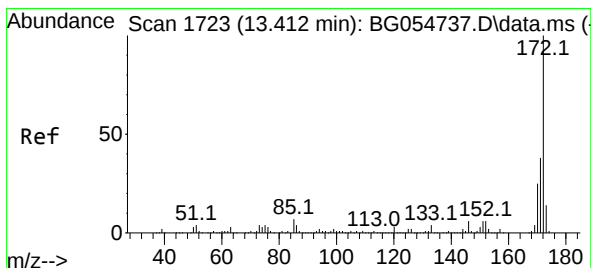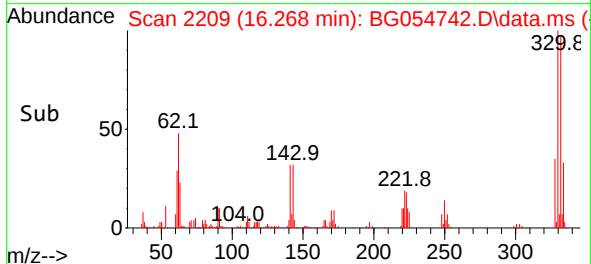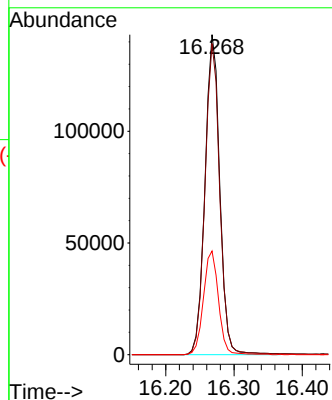

#45
2-Fluorobiphenyl
Concen: 84.464 ng
RT: 13.412 min Scan# 1723
Delta R.T. 0.000 min
Lab File: BG054742.D
Acq: 25 Aug 2022 19:06

Tgt Ion:172 Resp: 743274
Ion Ratio Lower Upper
172 100
171 37.9 31.2 46.8
170 24.7 20.6 30.8

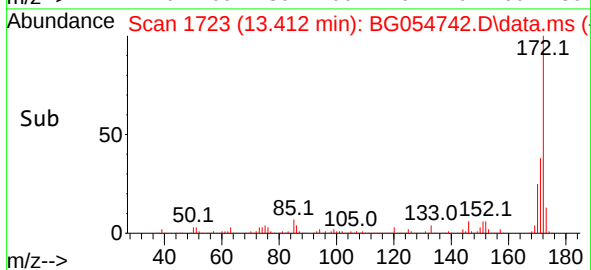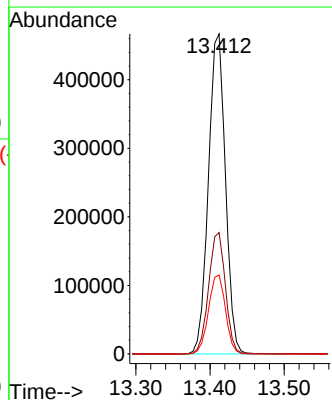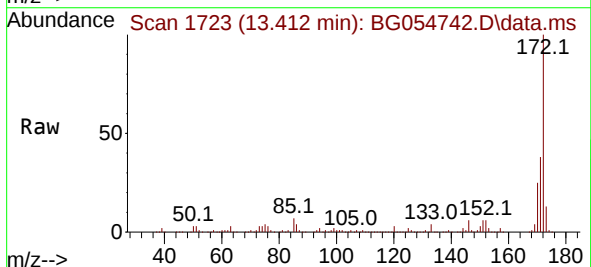

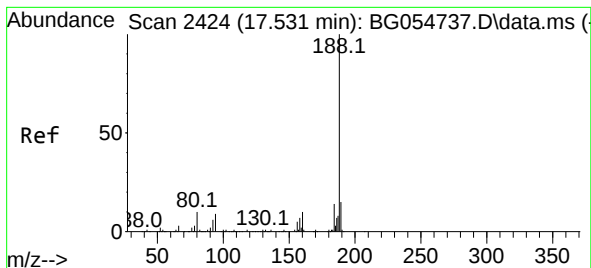

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.525 min Scan# 24

Delta R.T. -0.006 min

Lab File: BG054742.D

Acq: 25 Aug 2022 19:06

Instrument :

BNA_G

ClientSampleId :

PB147245BL





Tgt Ion:188 Resp: 319709

Ion Ratio Lower Upper

188 100

94 9.3 7.0 10.4

80 9.9 7.9 11.9

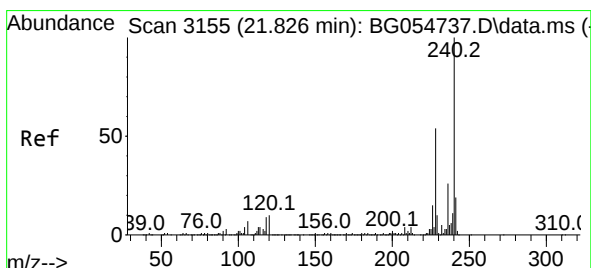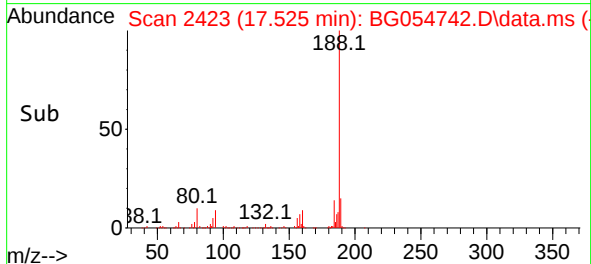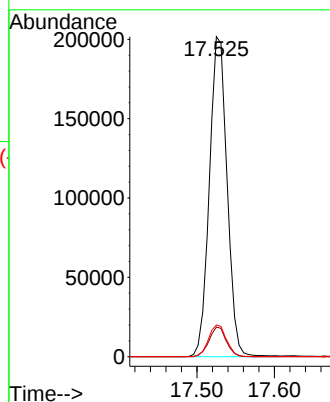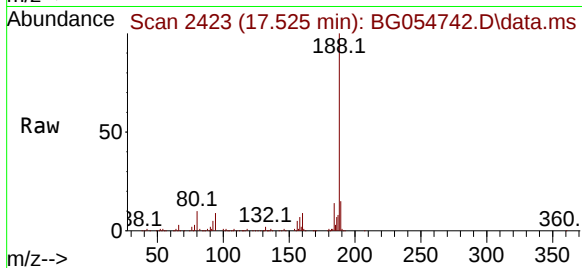

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.820 min Scan# 3154

Delta R.T. -0.006 min

Lab File: BG054742.D

Acq: 25 Aug 2022 19:06




Tgt Ion:240 Resp: 328244


Ion Ratio Lower Upper

240 100

120 10.1 8.2 12.4


236 27.6 21.2 31.8

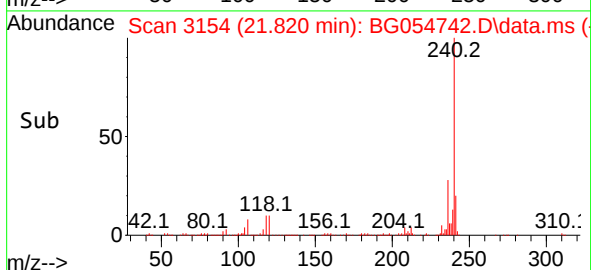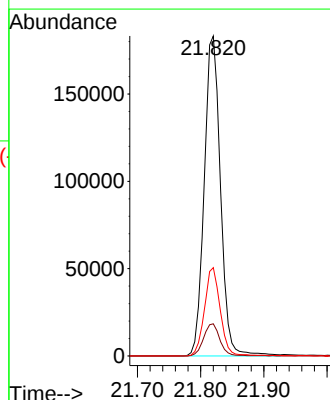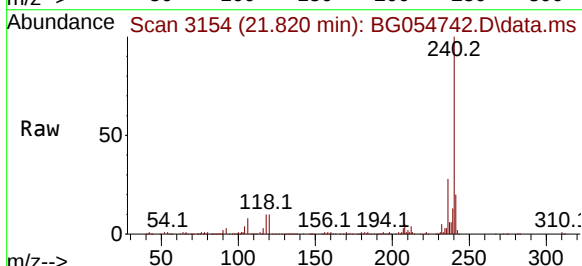



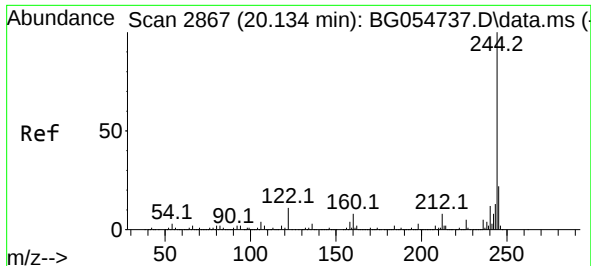


#79
 Terphenyl-d14
 Concen: 85.930 ng
 RT: 20.128 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BG054742.D
 Acq: 25 Aug 2022 19:06

Instrument :
 BNA_G
 ClientSampleId :
 PB147245BL

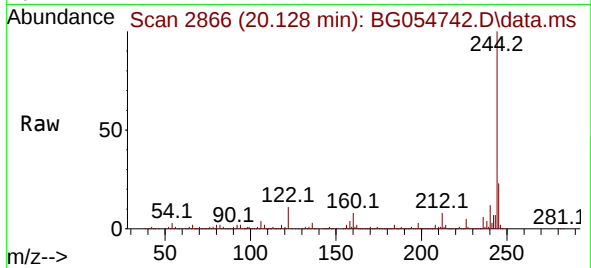

Tgt Ion:244 Resp: 1423554
 Ion Ratio Lower Upper
 244 100
 212 8.2 6.2 9.2
 122 11.0 9.0 13.6

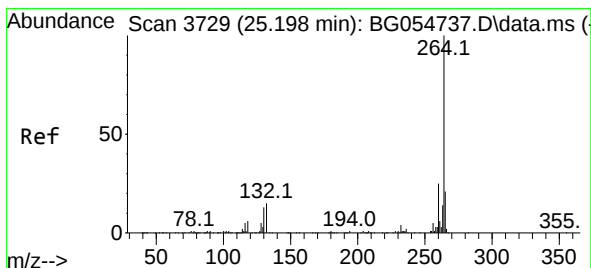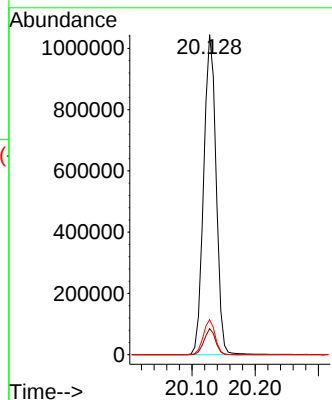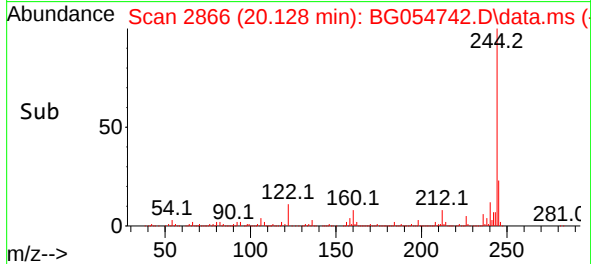

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.181 min Scan# 3726
 Delta R.T. -0.017 min
 Lab File: BG054742.D
 Acq: 25 Aug 2022 19:06

Tgt Ion:264 Resp: 334840
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.9 29.9
 265 21.3 16.9 25.3

