
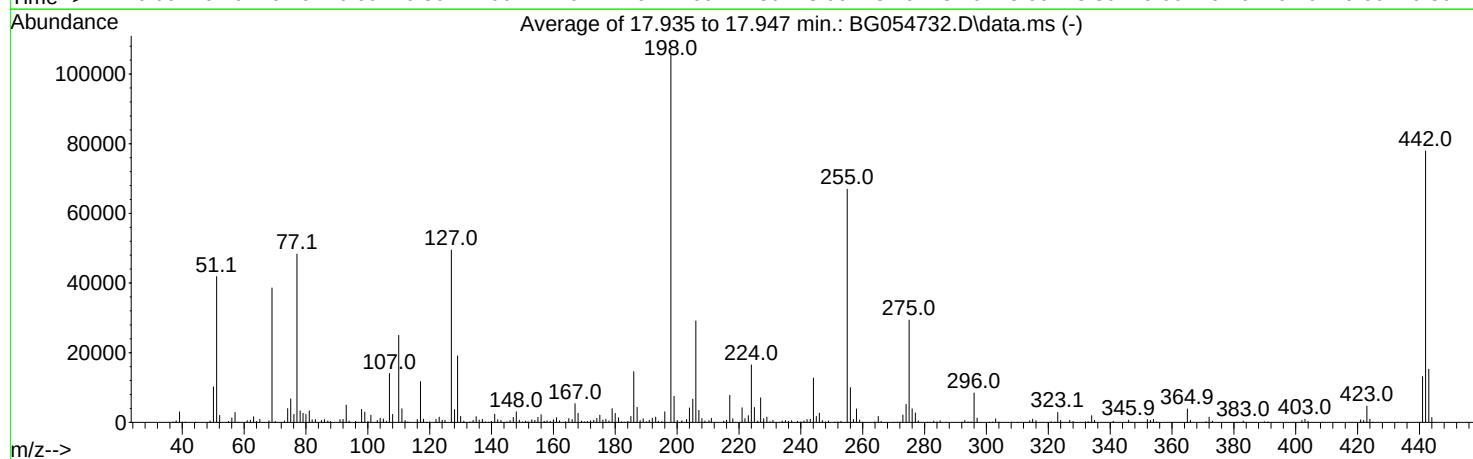


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
 Data File : BG054732.D
 Acq On : 25 Aug 2022 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

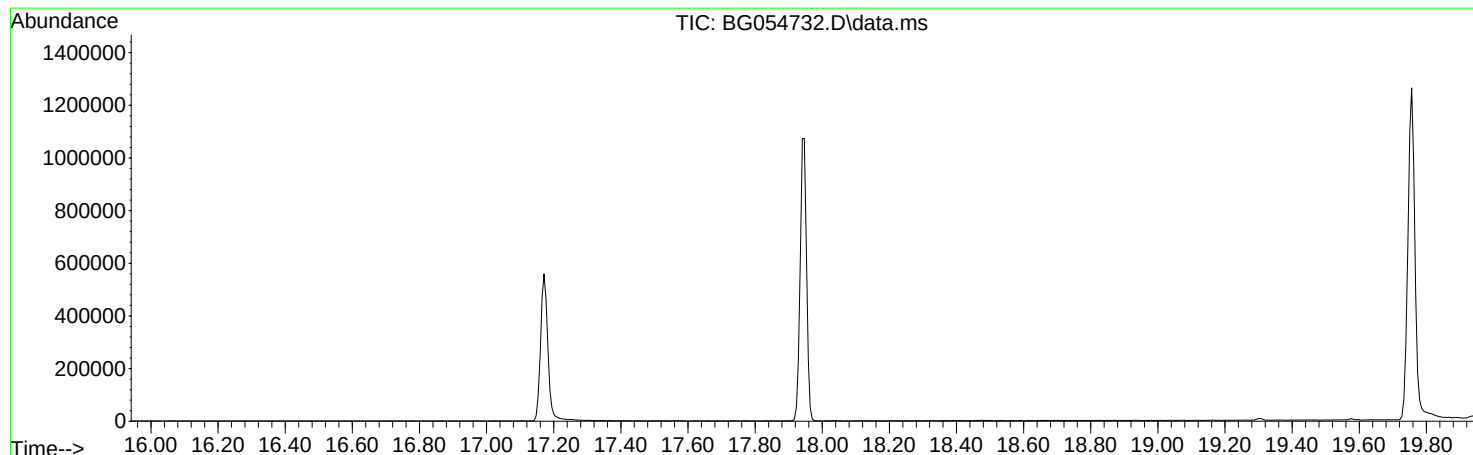

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	41848	PASS
68	69	0.00	2	1.2	448	PASS
69	198	0.00	100	36.6	38608	PASS
70	69	0.00	2	0.7	272	PASS
127	198	10	80	46.8	49469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105619	PASS
199	198	5	9	7.1	7508	PASS
275	198	10	60	27.8	29349	PASS
365	198	1	100	3.7	3876	PASS
441	198	0.01	100	12.4	13125	PASS
442	442	50	100	100.0	77925	PASS
443	442	15	24	19.6	15242	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/25/2022	BNA_G	<u>BG054732.D</u>
Compound Name	Response	Retention Time
DDT	365536	20.99
DDD	10143	20.53
DDE	646	20.03
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10789	376325	2.87

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
Data File : BG054732.D
Acq On : 25 Aug 2022 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 25 17:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 16:00:11 2022
Response via : Initial Calibration

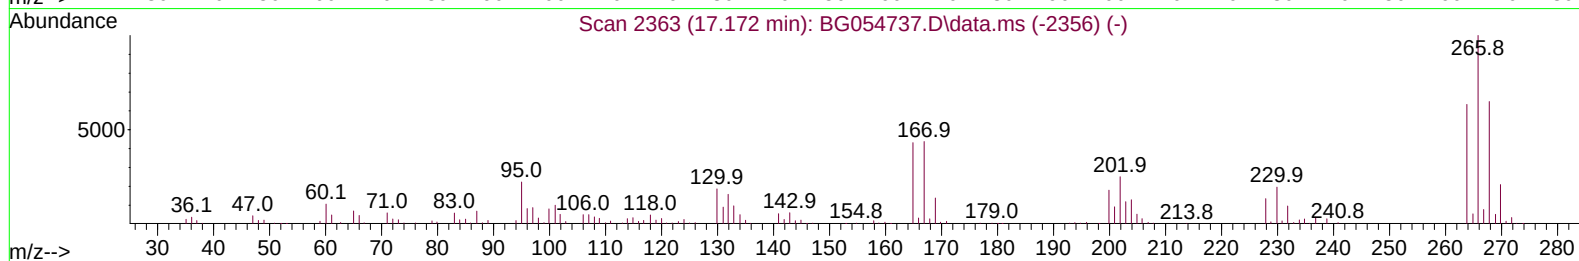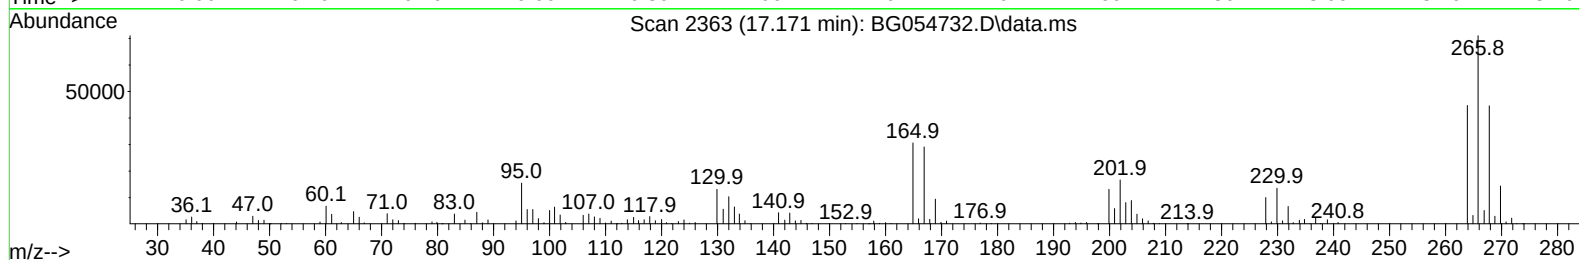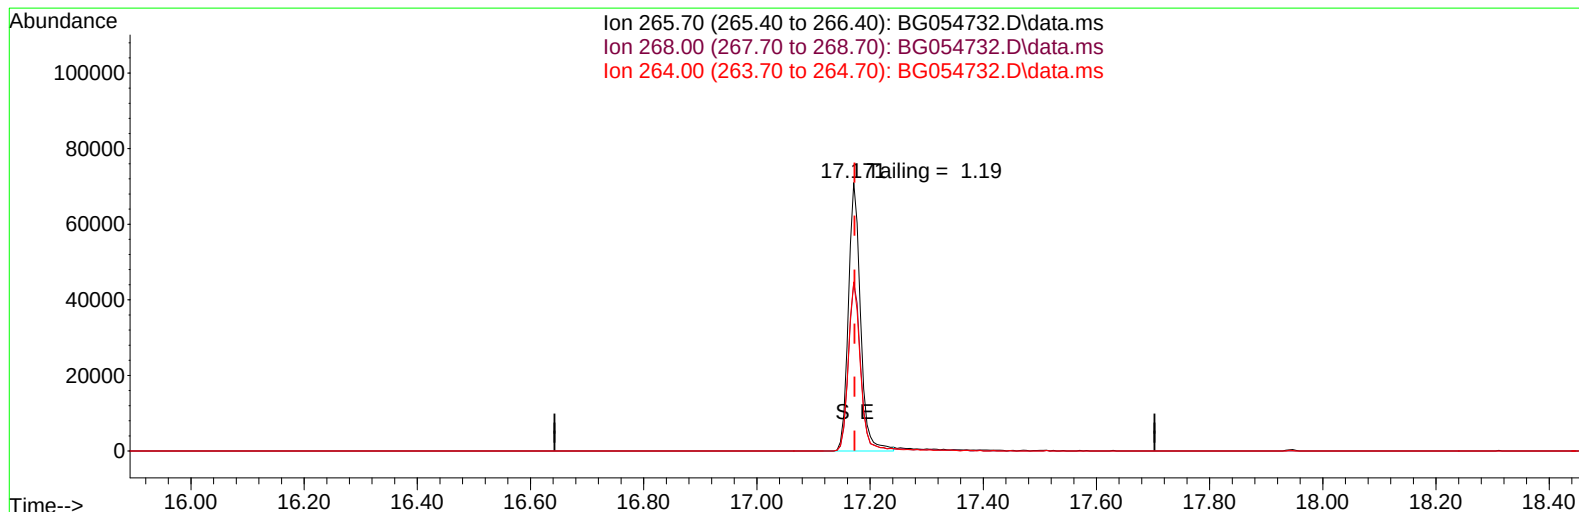

TIC: BG054732.D\data.ms

(70) Pentachlorophenol (C)

17.171min (-0.001) 79777.43 ng




response 107871

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.82
264.00	61.70	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082522\
Data File : BG054732.D
Acq On : 25 Aug 2022 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 25 17:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 16:00:11 2022
Response via : Initial Calibration

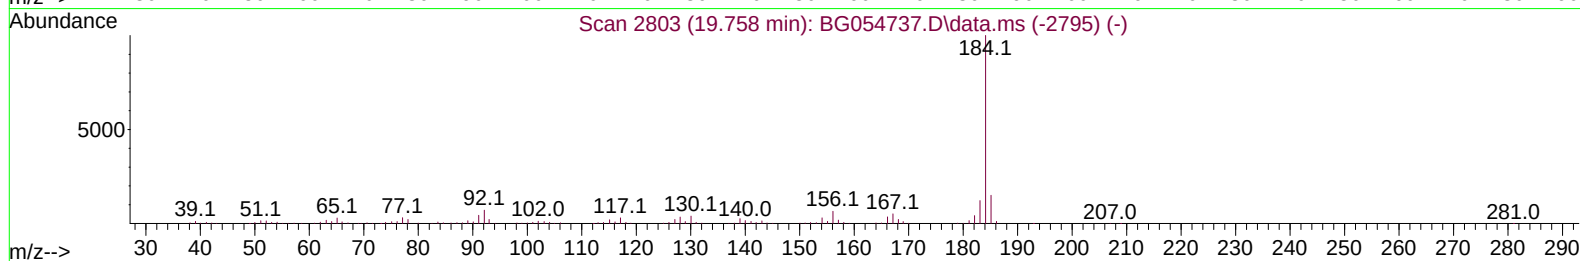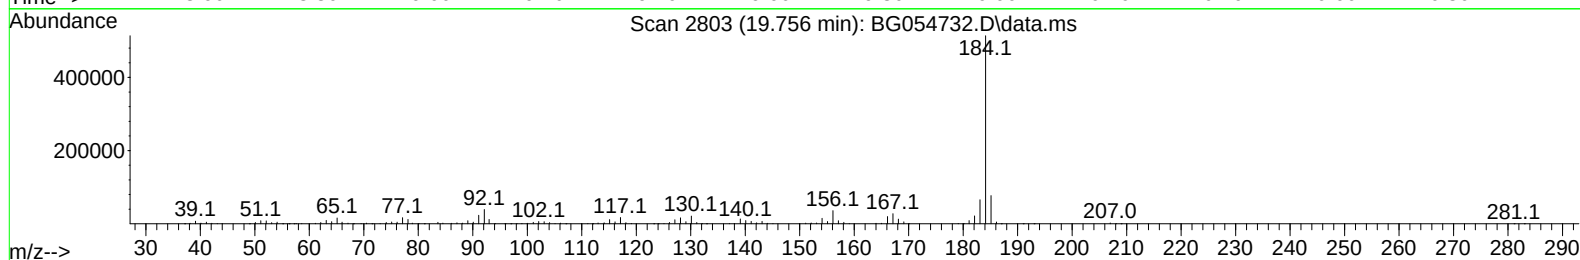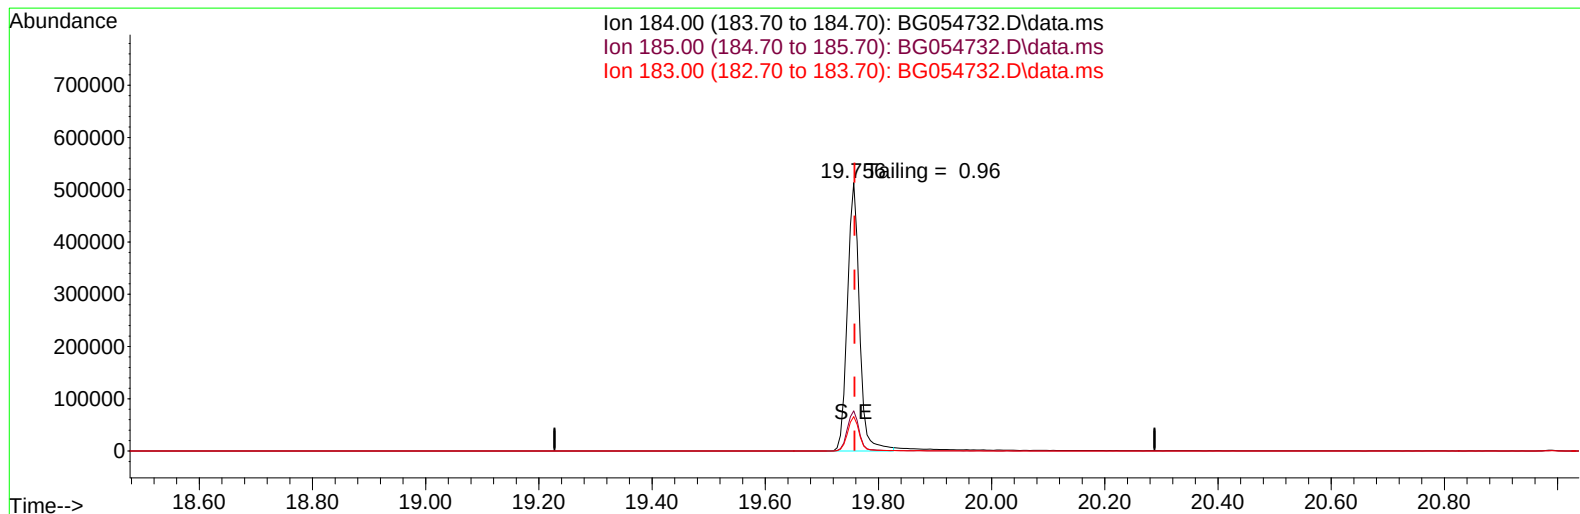

TIC: BG054732.D\data.ms

(77) Benzidine

19.756min (-0.001) 615084.70 ng

response 787938

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.99
183.00	12.30	12.83
0.00	0.00	0.00