


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082523\
Data File : BG058848.D
Acq On : 25 Aug 2023 13:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 27 03:38:58 2023

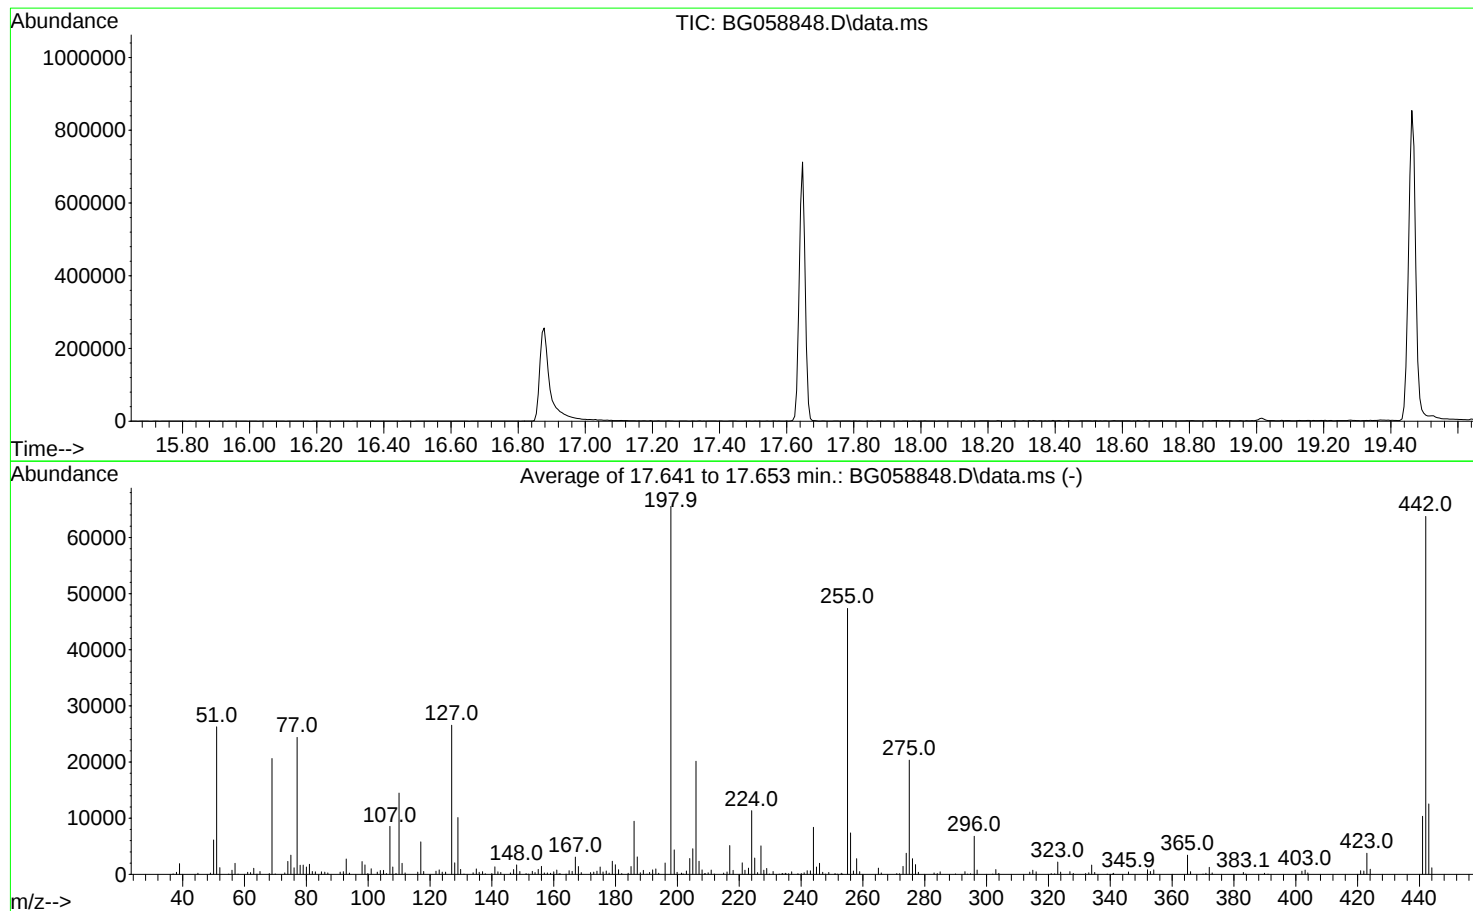




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	26267	PASS
68	69	0.00	2	0.7	152	PASS
69	198	0.00	100	31.5	20643	PASS
70	69	0.00	2	0.4	78	PASS
127	198	10	80	40.5	26557	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65520	PASS
199	198	5	9	6.7	4363	PASS
275	198	10	60	31.1	20355	PASS
365	198	1	100	5.2	3430	PASS
441	198	0.01	100	15.8	10363	PASS
442	442	50	100	100.0	63755	PASS
443	442	15	24	19.7	12539	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082523\
Data File : BG058848.D
Acq On : 25 Aug 2023 13:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 25 15:29:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

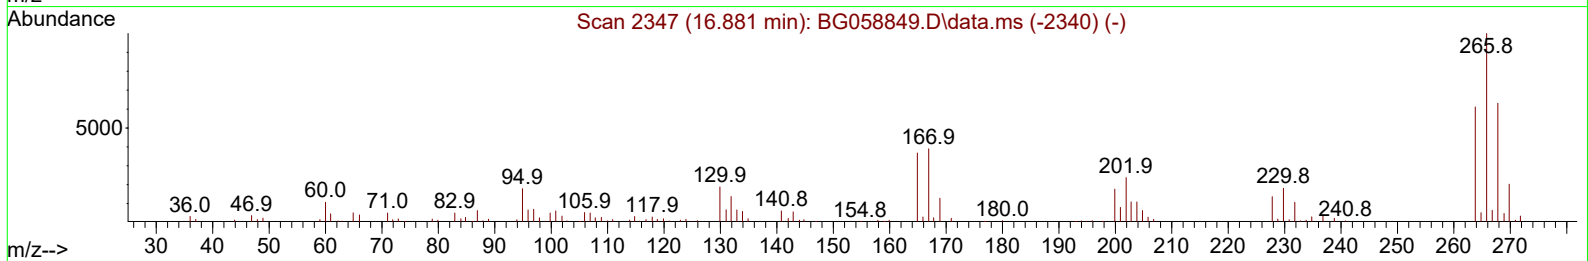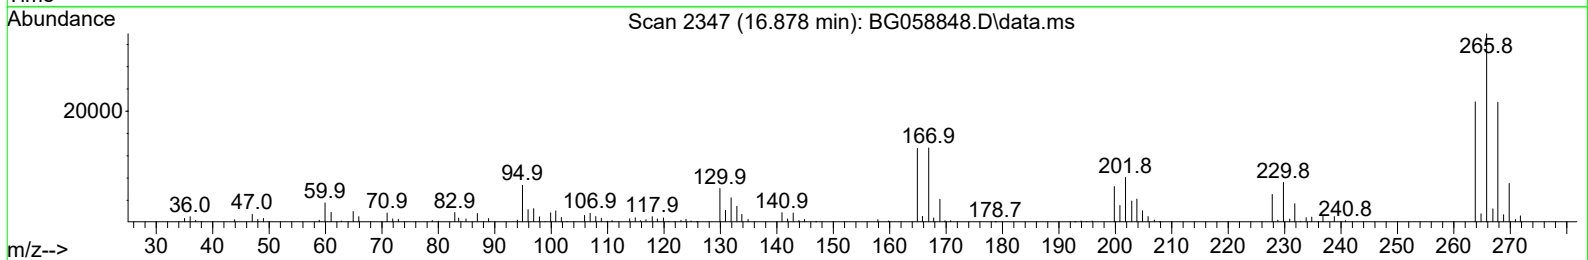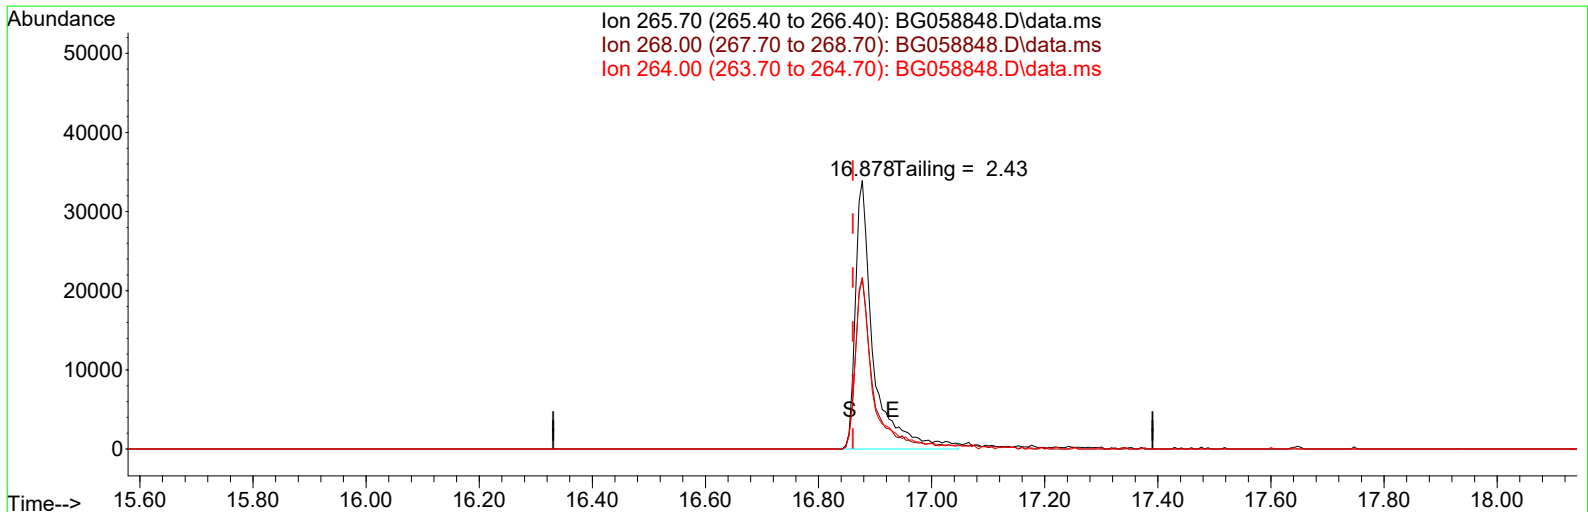

TIC: BG058848.D\data.ms

(70) Pentachlorophenol (C)

16.878min (+ 0.017) 40362.27 ng




response 73989

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	63.77
264.00	61.90	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082523\
Data File : BG058848.D
Acq On : 25 Aug 2023 13:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 25 15:29:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 01:40:57 2023
Response via : Initial Calibration

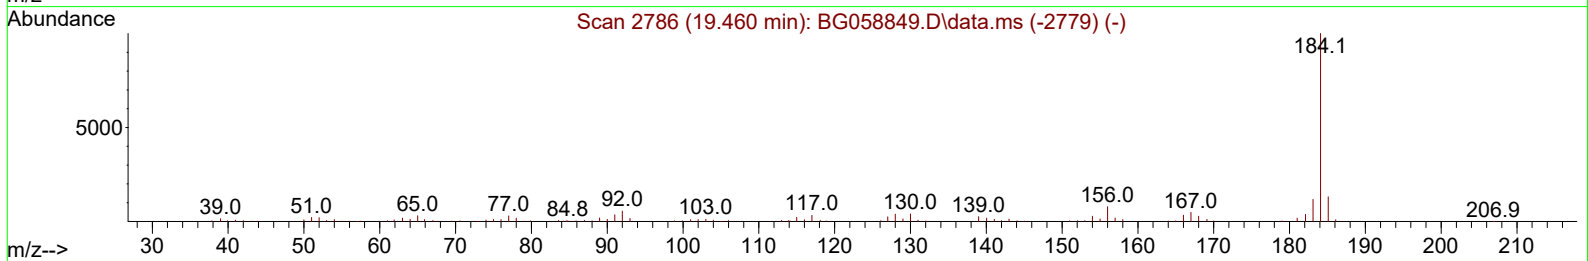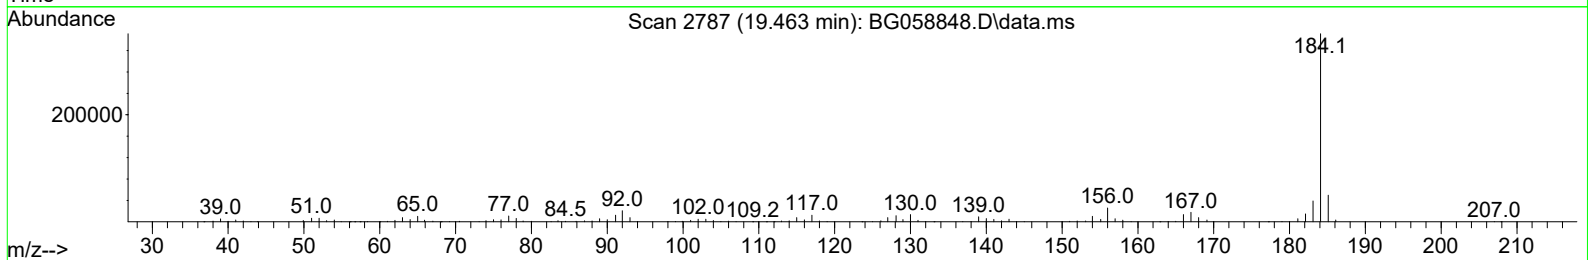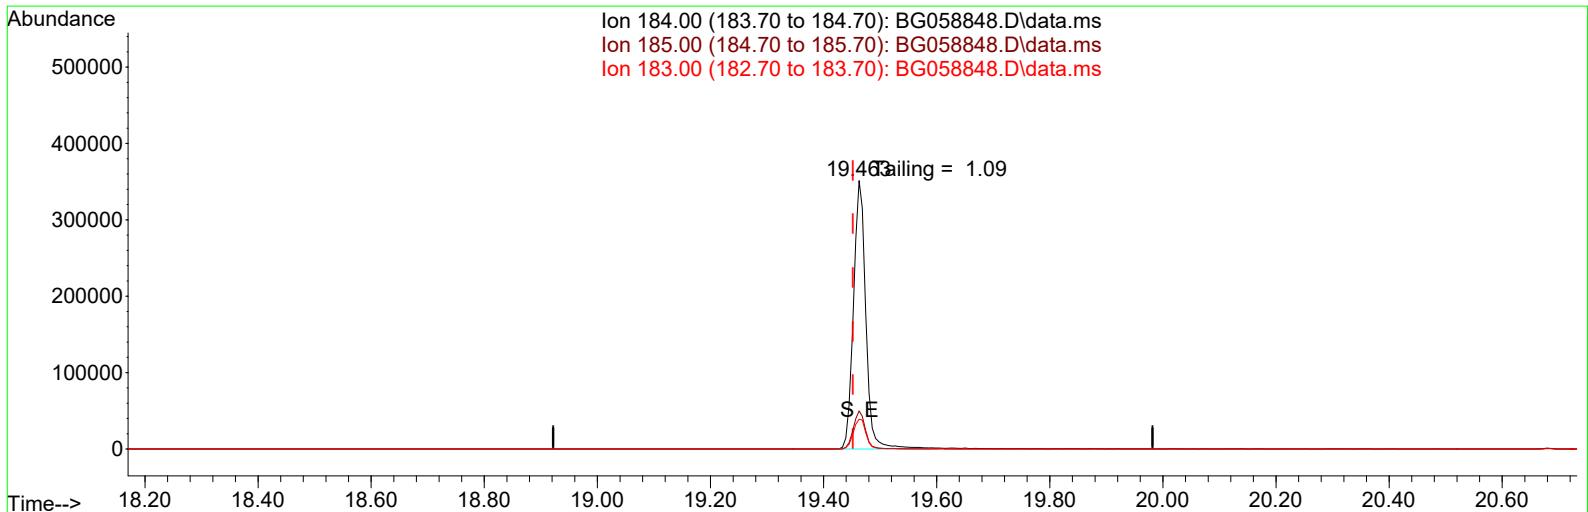

TIC: BG058848.D\data.ms

(77) Benzidine

19.463min (+ 0.011) 0.00 ng

response 536272

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.21
183.00	12.50	11.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_G	<u>BG058848.D</u>
Compound Name	Response	Retention Time
DDT	267290	20.685
DDD	4621	20.291
DDE	189	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4810	272100	1.77

Instrument :
BNA_G
ClientSampleId :
DFTPP