
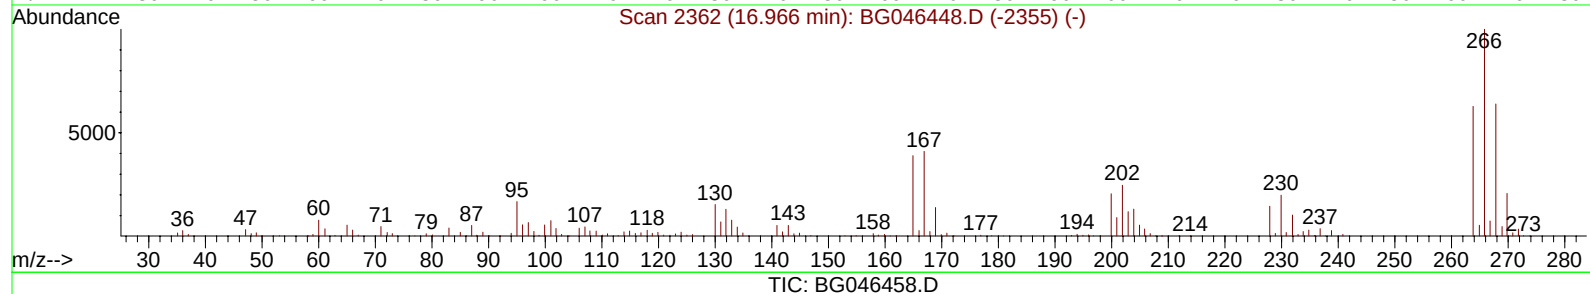
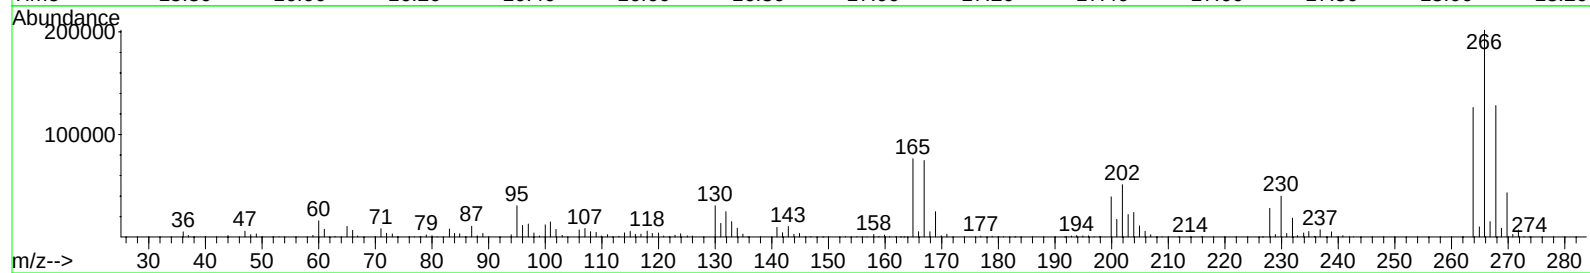


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082620\
Data File : BG046458.D
Acq On : 26 Aug 2020 17:50
Operator : CG/JU
Sample : PB131215BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 26 18:45:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 25 18:00:34 2020
Response via : Initial Calibration

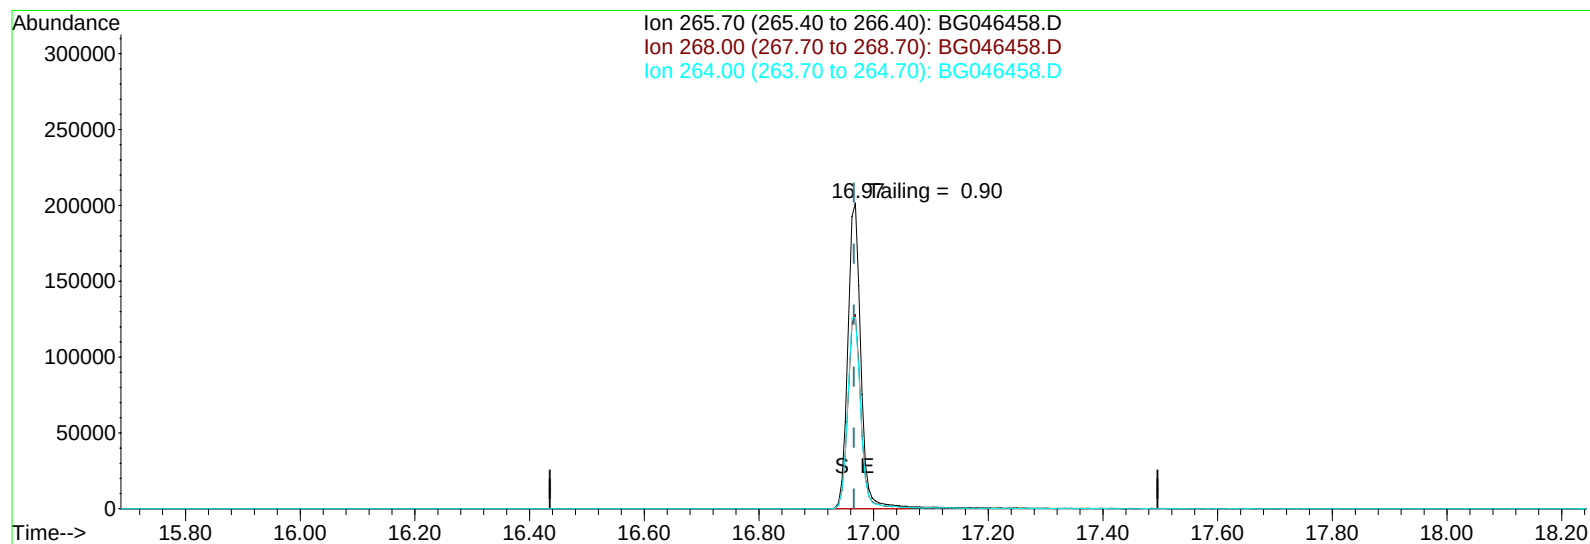

(70) Pentachlorophenol (C)




16.968min (+0.003) 94.12ng

response 319681

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.59
264.00	62.70	62.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082620\
 Data File : BG046458.D
 Acq On : 26 Aug 2020 17:50
 Operator : CG/JU
 Sample : PB131215BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 26 18:45:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 25 18:00:34 2020
 Response via : Initial Calibration

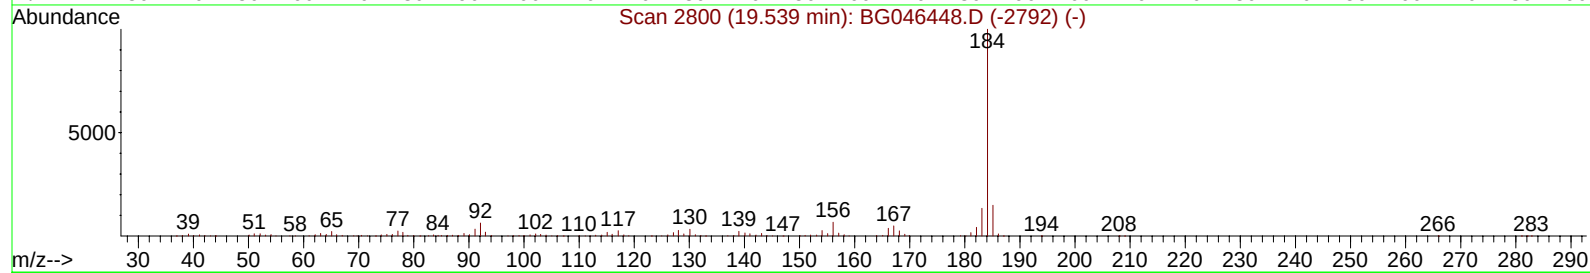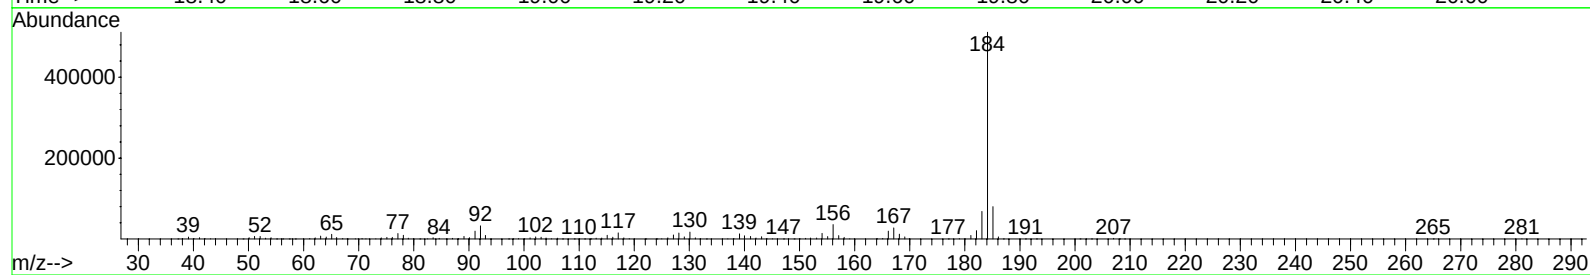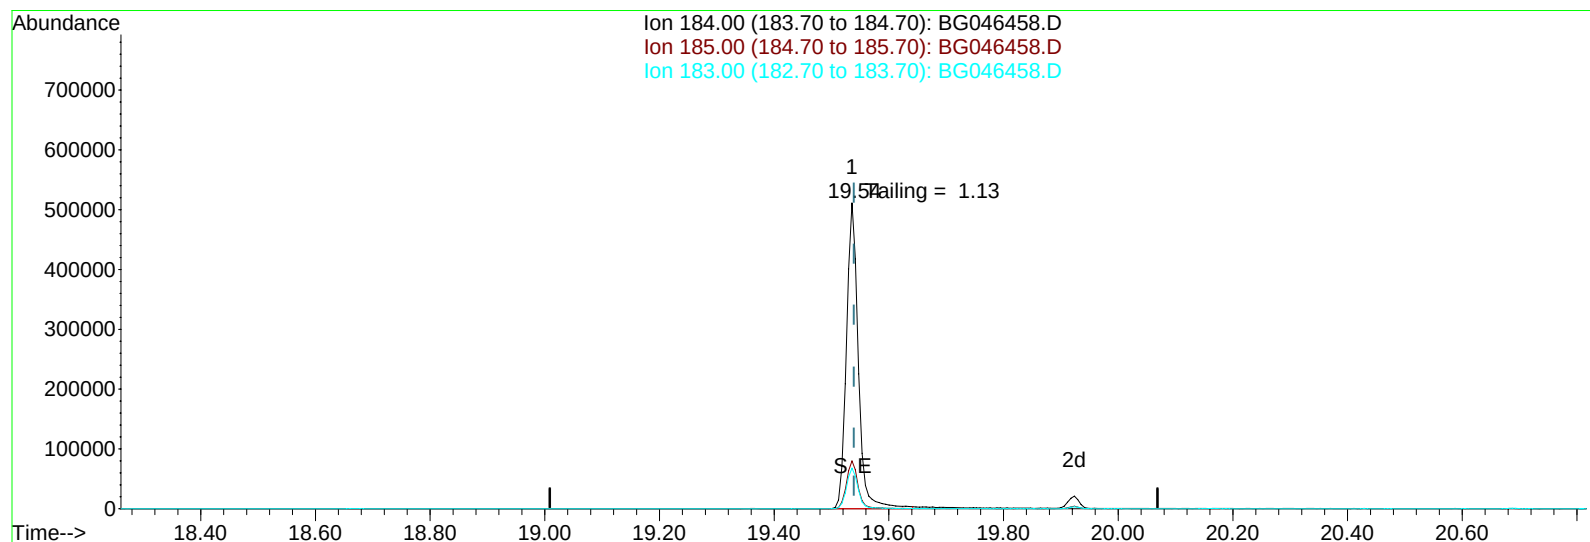

TIC: BG046458.D

(77) Benzidine

19.536min (-0.003) 60.49ng

response 745488

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.65
183.00	13.40	13.31
0.00	0.00	0.00