
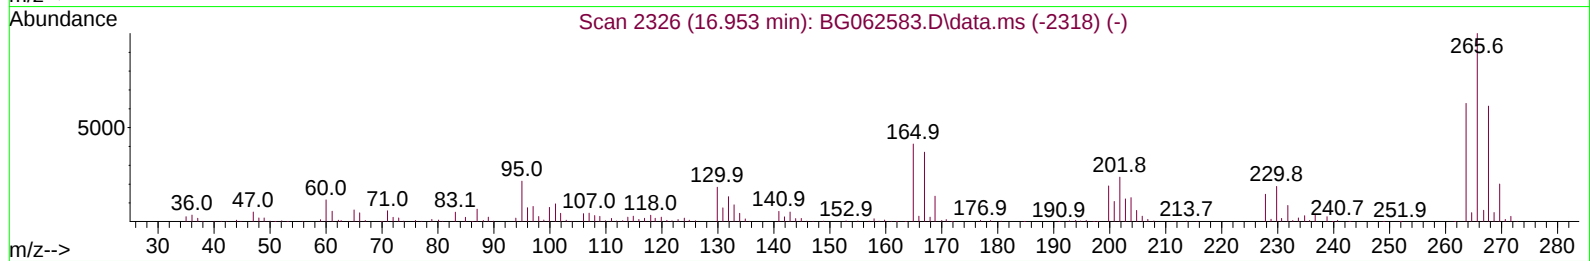
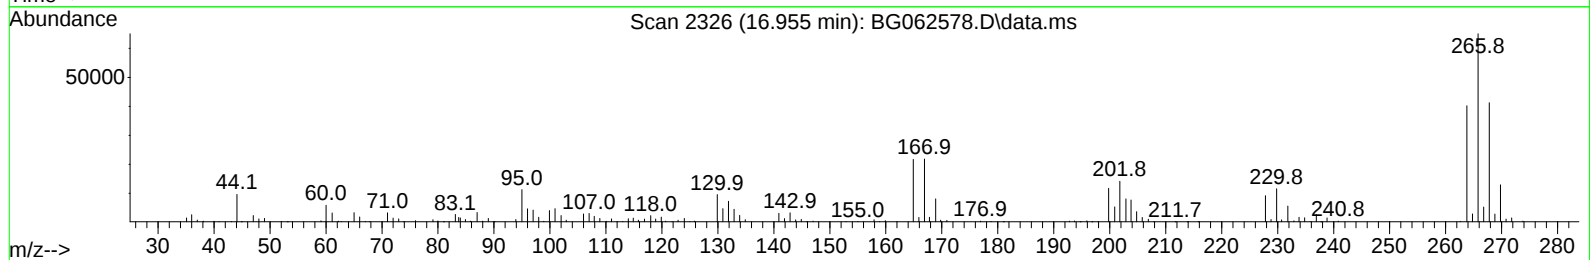


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082724\
Data File : BG062578.D
Acq On : 27 Aug 2024 14:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 01:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 00:59:59 2024
Response via : Initial Calibration

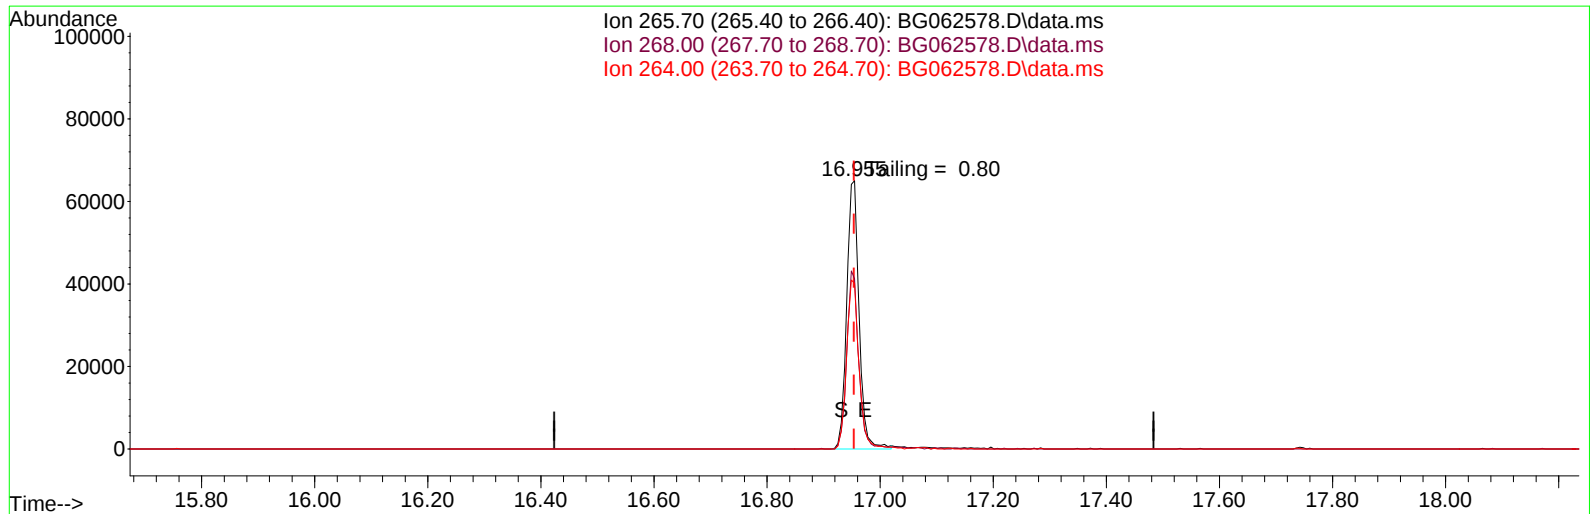

TIC: BG062578.D\data.ms

(70) Pentachlorophenol (C)




16.955min (+ 0.001) 69538.07 ng

response 99660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.40	63.42
264.00	67.80	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082724\
Data File : BG062578.D
Acq On : 27 Aug 2024 14:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 01:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 00:59:59 2024
Response via : Initial Calibration

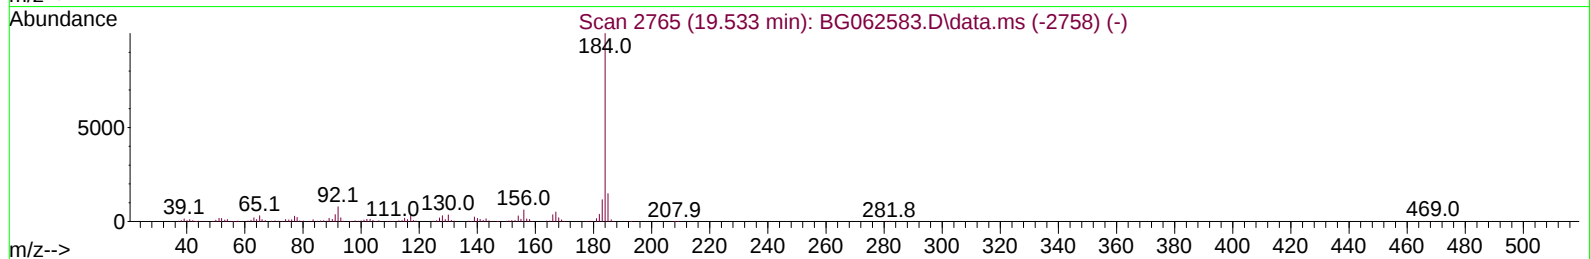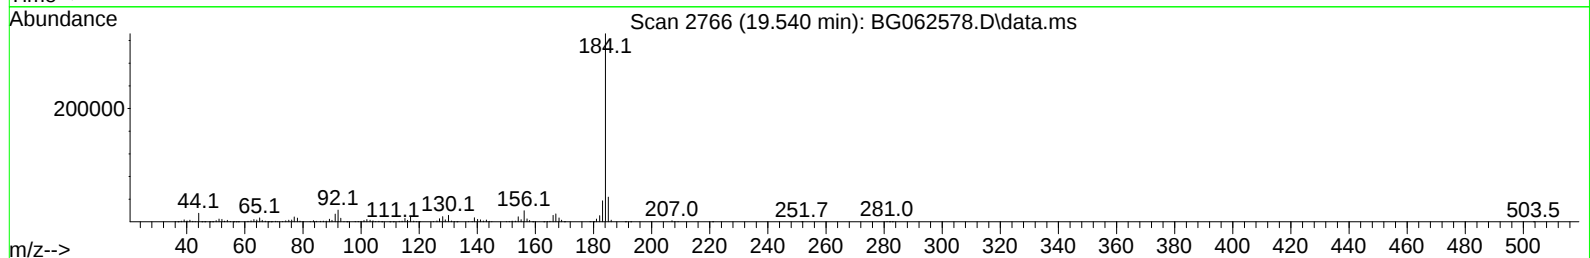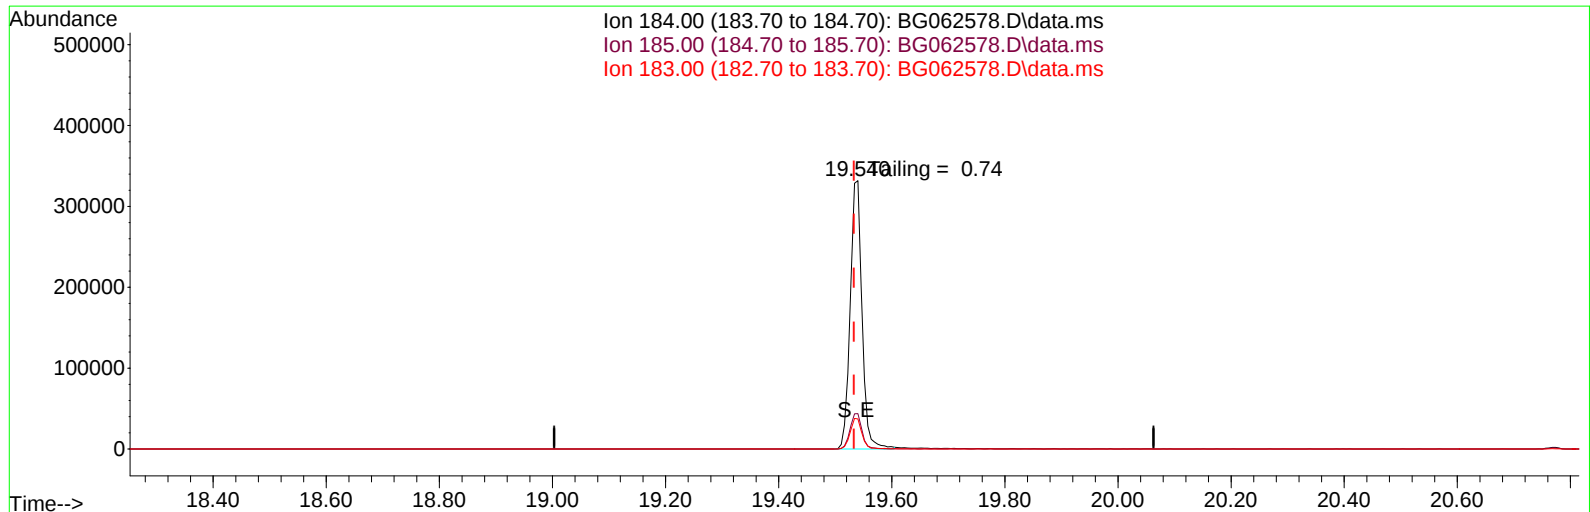

TIC: BG062578.D\data.ms

(77) Benzidine**19.540min (+ 0.007) 53666.69 ng****response 483627**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.18
183.00	11.60	11.21
0.00	0.00	0.00