
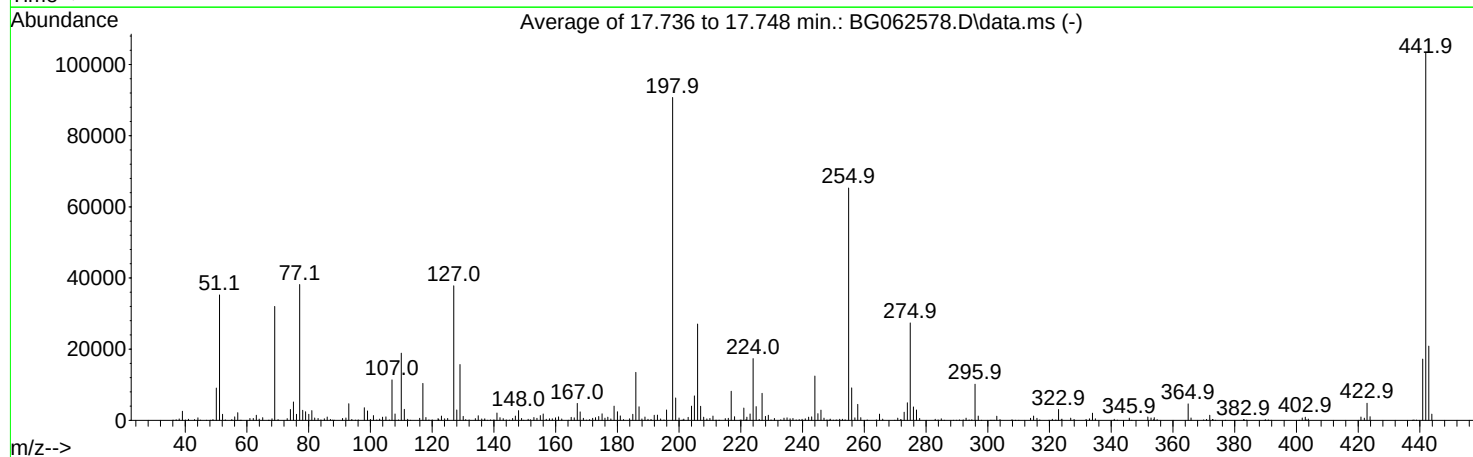


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082724\
Data File : BG062578.D
Acq On : 27 Aug 2024 14:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 28 00:59:59 2024

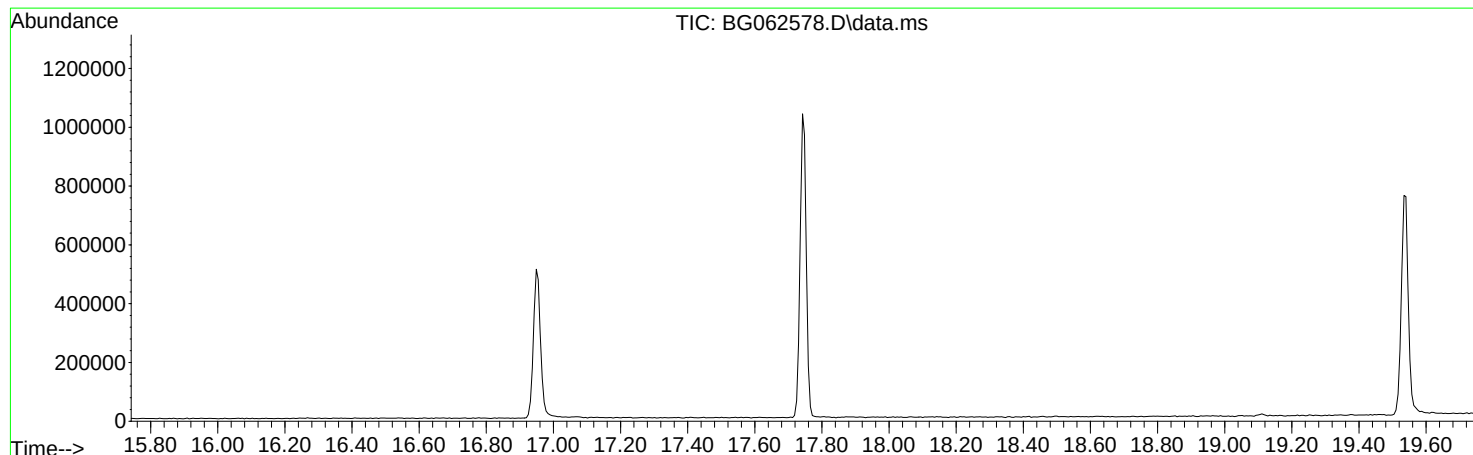

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	35248	PASS
68	69	0.00	2	1.4	458	PASS
69	198	0.00	100	35.3	31995	PASS
70	69	0.00	2	0.7	215	PASS
127	198	10	80	41.7	37829	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90733	PASS
199	198	5	9	6.9	6303	PASS
275	198	10	60	30.2	27371	PASS
365	198	1	100	5.1	4645	PASS
441	198	0.01	100	19.0	17225	PASS
442	442	50	100	100.0	103368	PASS
443	442	15	24	20.2	20874	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/27/2024	BNA_G	<u>BG062578.D</u>
Compound Name	Response	Retention Time
DDT	226815	20.768
DDD	2834	20.38
DDE	0	19.852
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2834	229649	1.23

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082724\
Data File : BG062578.D
Acq On : 27 Aug 2024 14:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 28 01:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 00:59:59 2024
Response via : Initial Calibration

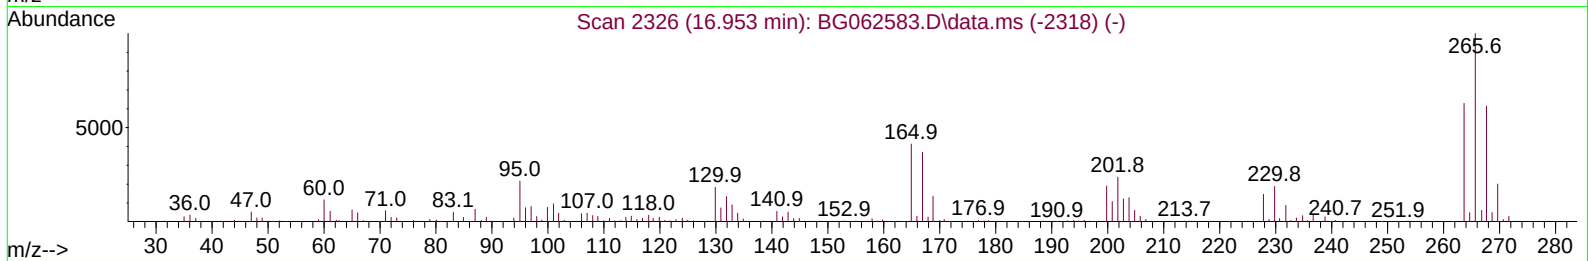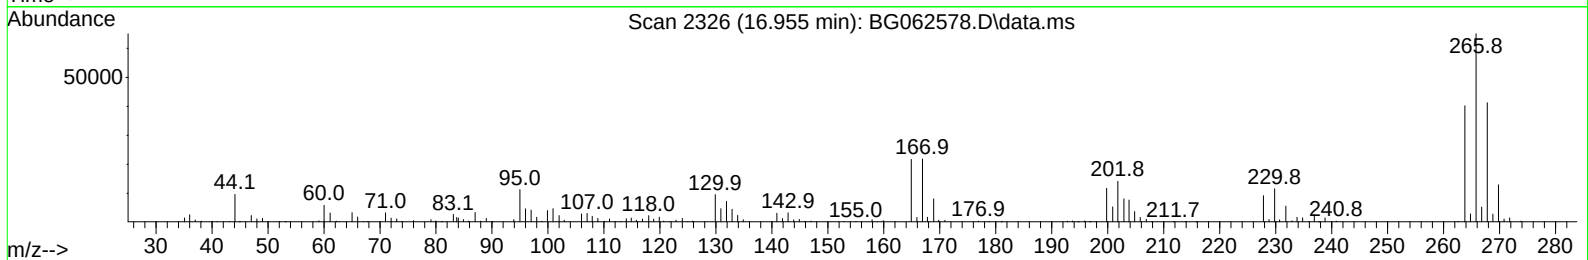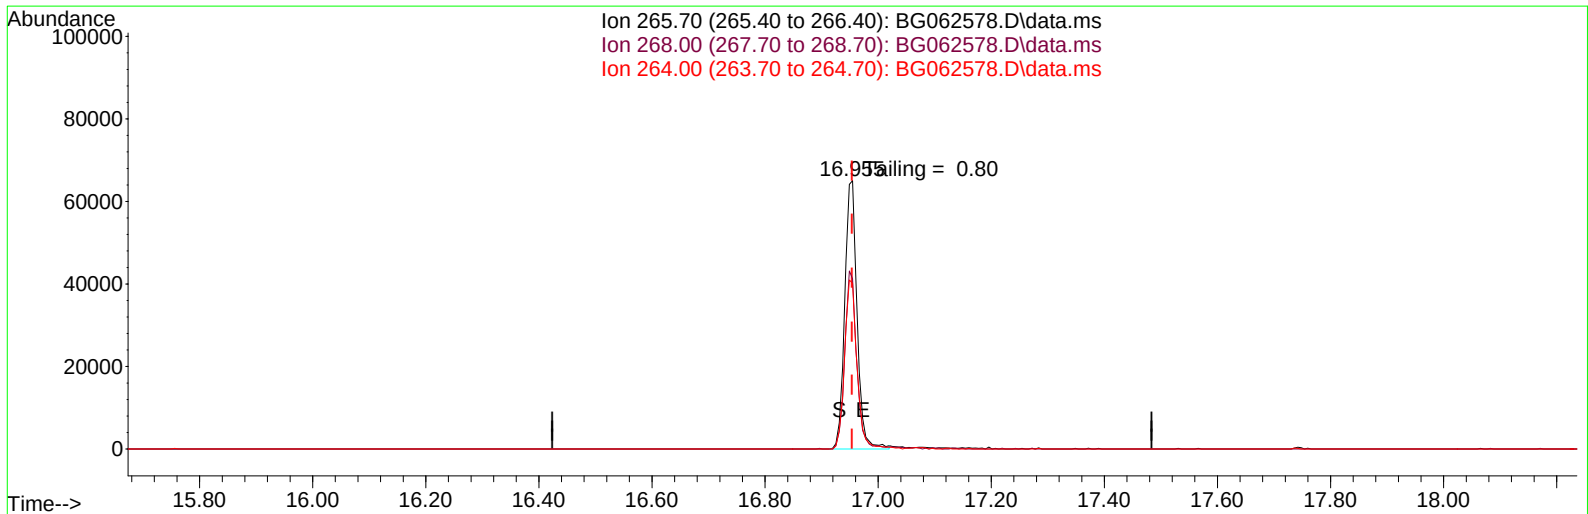

TIC: BG062578.D\data.ms

(70) Pentachlorophenol (C)

16.955min (+ 0.001) 69538.07 ng




response 99660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.40	63.42
264.00	67.80	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082724\
Data File : BG062578.D
Acq On : 27 Aug 2024 14:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 28 01:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 00:59:59 2024
Response via : Initial Calibration

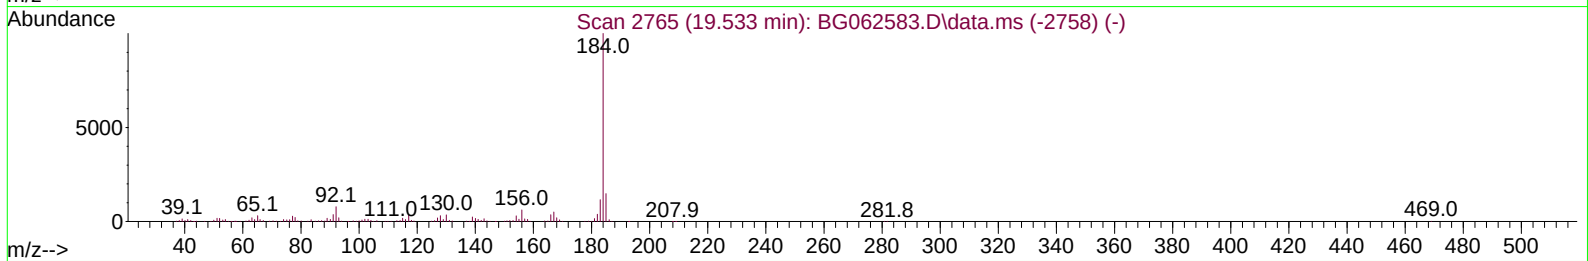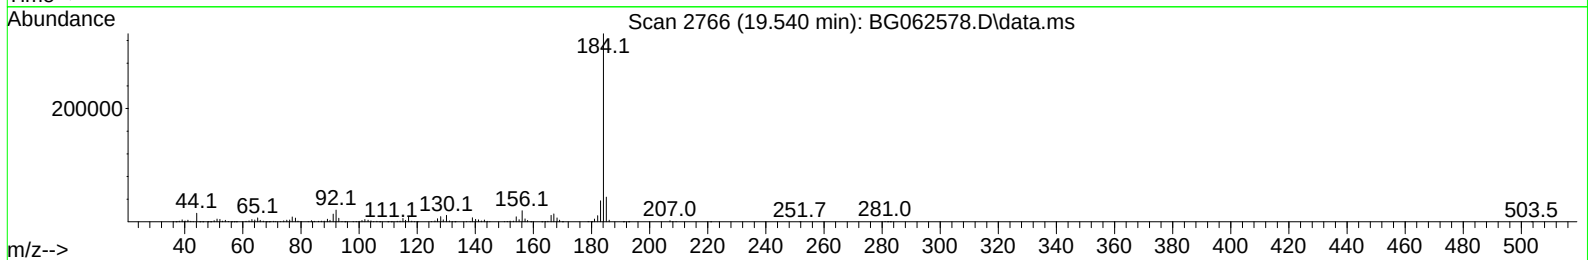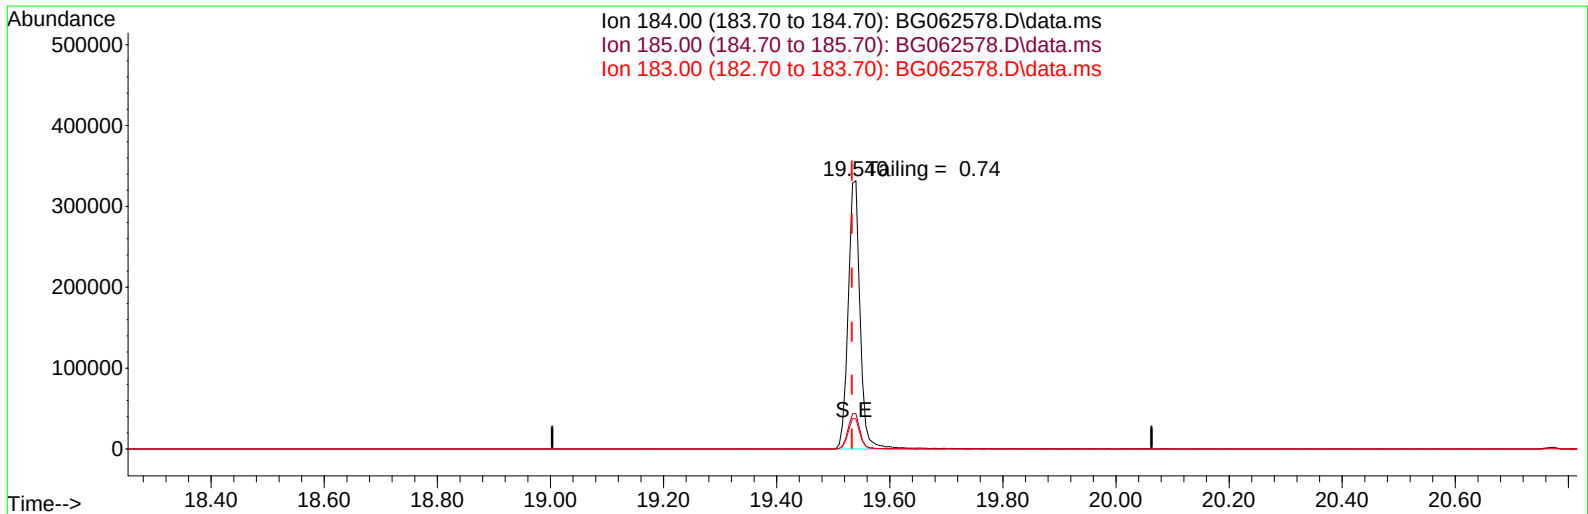

TIC: BG062578.D\data.ms

(77) Benzidine

19.540min (+ 0.007) 53666.69 ng

response 483627

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.18
183.00	11.60	11.21
0.00	0.00	0.00