


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082818\
 Data File : BG036460.D
 Acq On : 28 Aug 2018 15:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

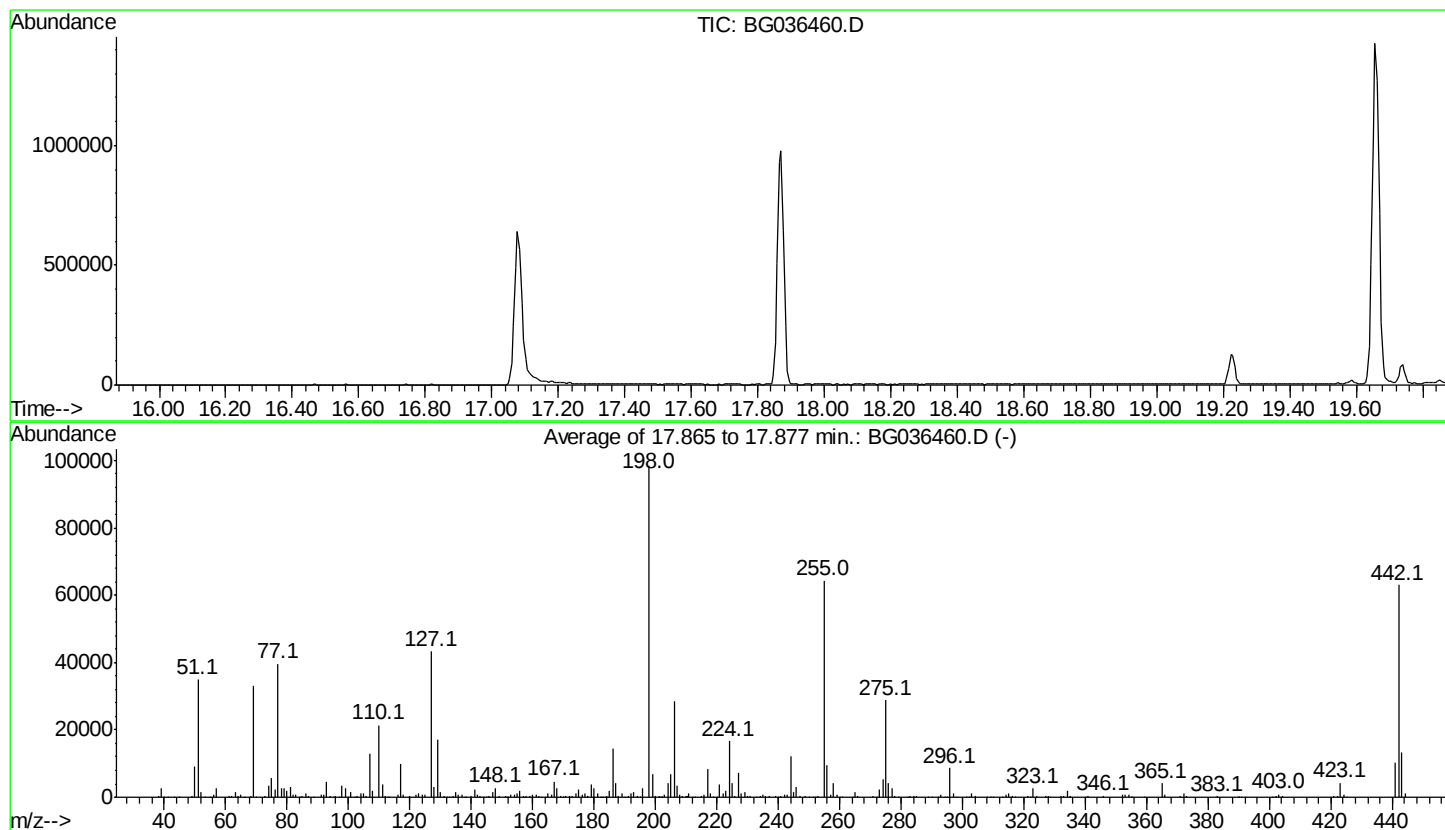

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	34837	PASS
68	69	0.00	2	1.0	322	PASS
69	198	0.00	100	33.6	33088	PASS
70	69	0.00	2	0.2	78	PASS
127	198	10	80	43.8	43162	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98474	PASS
199	198	5	9	6.8	6729	PASS
275	198	10	60	29.2	28725	PASS
365	198	1	100	4.2	4109	PASS
441	198	0.01	100	10.5	10334	PASS
442	198	50	100	64.0	63066	PASS
443	442	15	24	20.9	13151	PASS