


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082818\
 Data File : BG036478.D
 Acq On : 29 Aug 2018 5:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

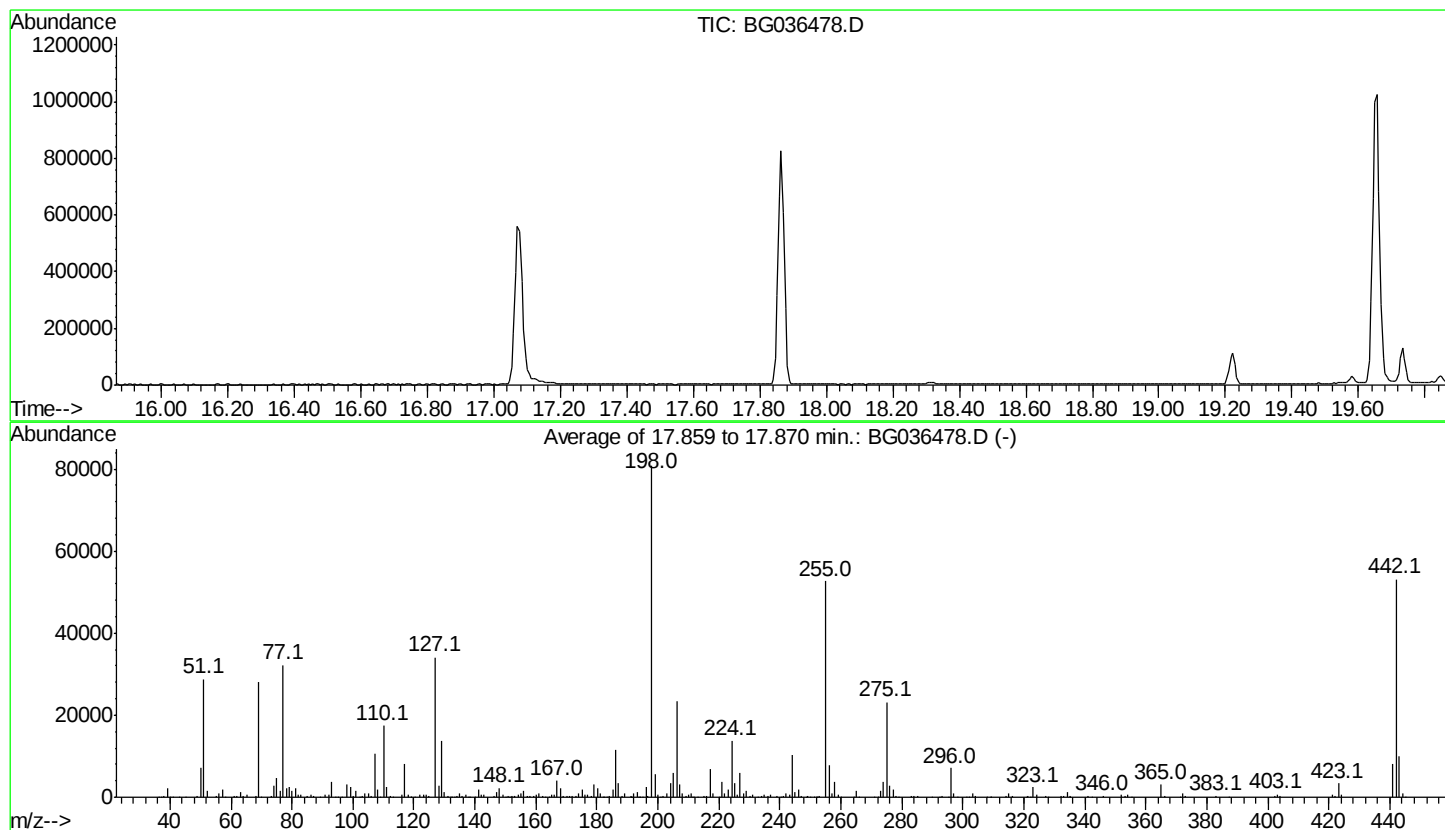

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	28786	PASS
68	69	0.00	2	1.5	424	PASS
69	198	0.00	100	34.8	28090	PASS
70	69	0.00	2	0.2	55	PASS
127	198	10	80	42.1	34013	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80829	PASS
199	198	5	9	7.1	5701	PASS
275	198	10	60	28.7	23200	PASS
365	198	1	100	3.7	3031	PASS
441	198	0.01	100	10.0	8090	PASS
442	198	50	100	65.7	53130	PASS
443	442	15	24	18.6	9876	PASS