
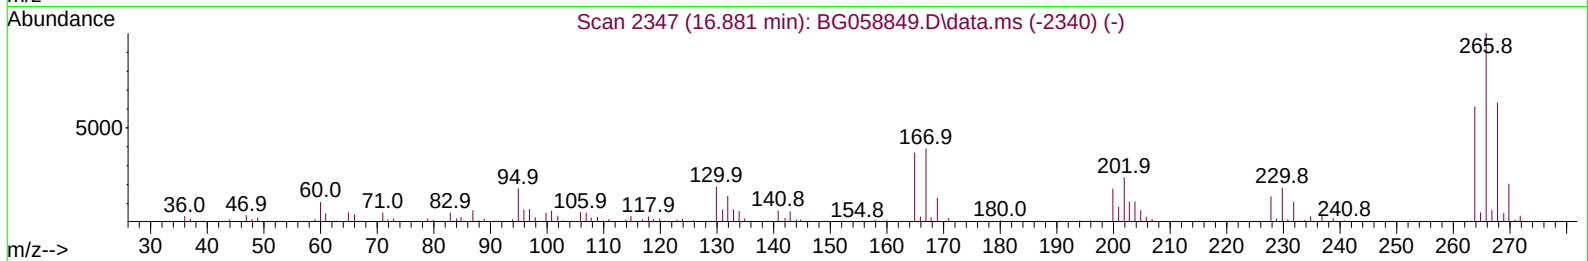
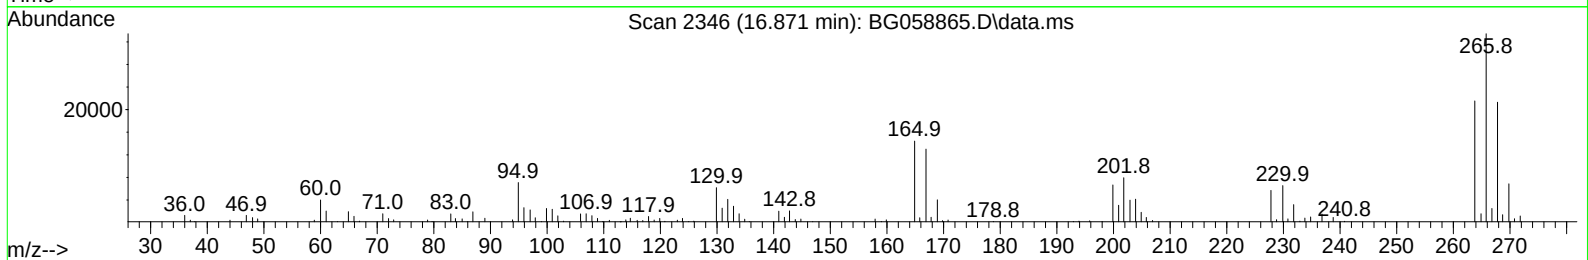


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058865.D
Acq On : 28 Aug 2023 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 02:45:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

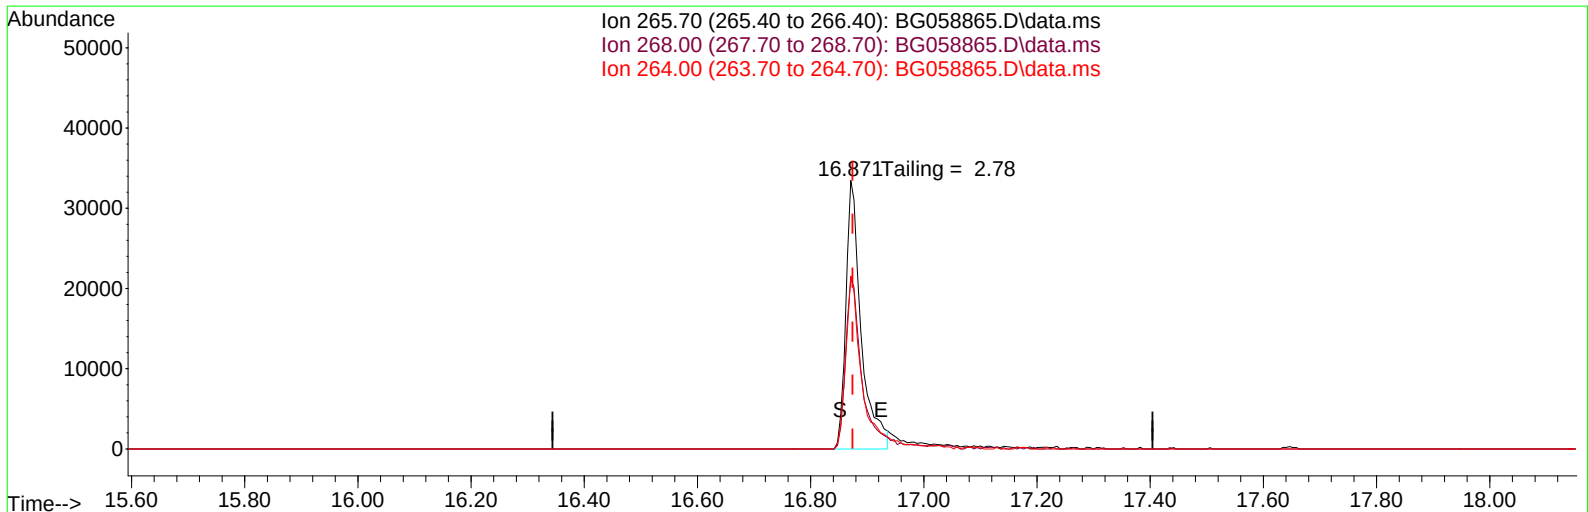

TIC: BG058865.D\data.ms

(70) Pentachlorophenol (C)




16.871min (-0.003) 31995.33 ng

response 68955

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	67.85
264.00	61.90	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058865.D
Acq On : 28 Aug 2023 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 02:45:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

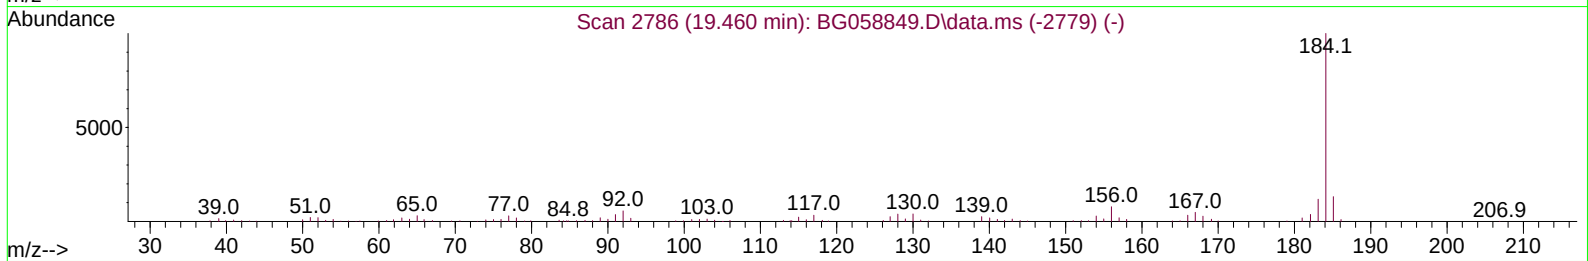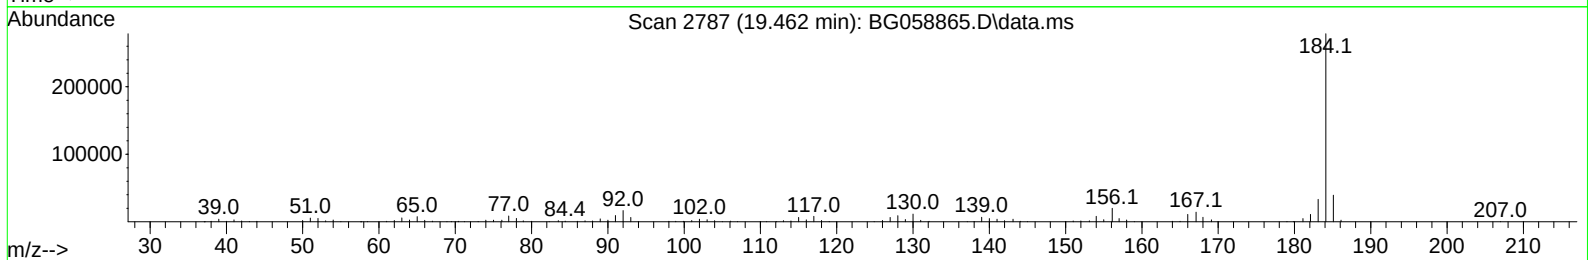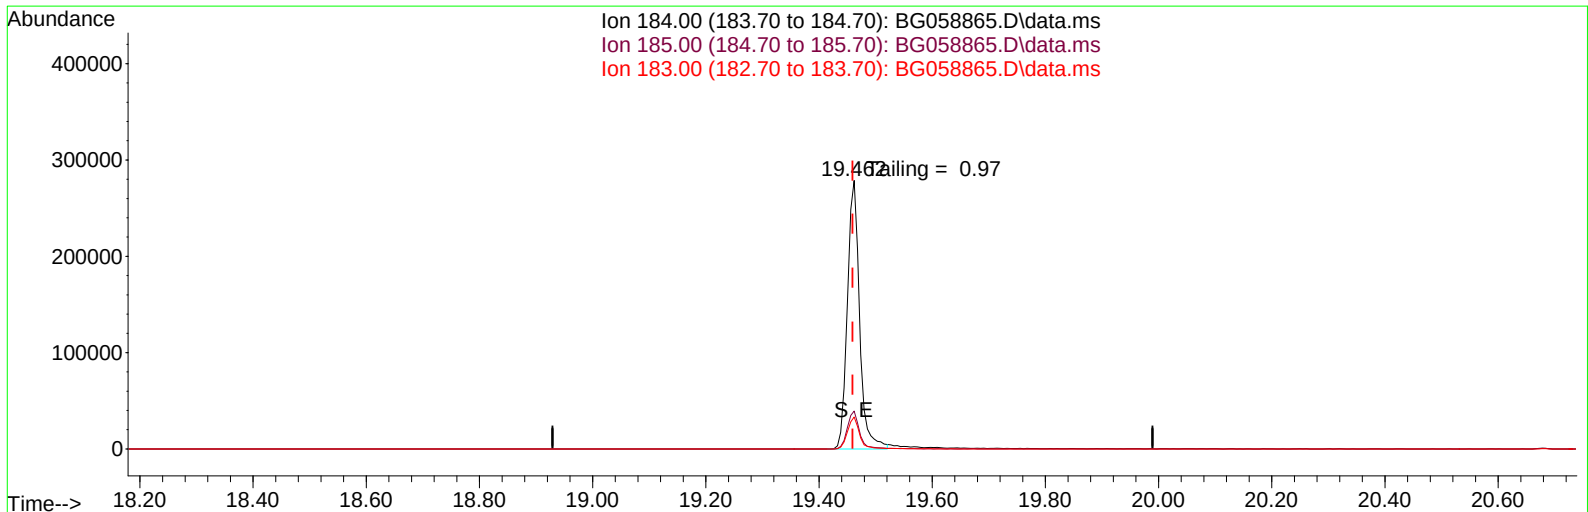

TIC: BG058865.D\data.ms

(77) Benzidine

19.462min (+ 0.003) 0.00 ng

response 426032

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.11
183.00	12.50	11.89
0.00	0.00	0.00