

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
 Data File : BG058867.D
 Acq On : 28 Aug 2023 10:30
 Operator : MA/JU
 Sample : PB155083BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB155083BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.400	387	393	406	rBV	353096	563207	39.92%	9.017%
2	6.998	658	665	679	rBV	325127	569406	40.36%	9.117%
3	7.826	799	806	815	rBV	88122	150154	10.64%	2.404%
4	8.990	996	1004	1013	rBV	184376	338425	23.99%	5.418%
5	10.629	1274	1283	1296	rBV	96988	200629	14.22%	3.212%
6	13.091	1695	1702	1715	rBV	477746	758231	53.74%	12.140%
7	14.471	1930	1937	1953	rVB	167330	277362	19.66%	4.441%
8	15.964	2184	2191	2207	rBV	381389	658058	46.64%	10.536%
9	17.215	2398	2404	2420	rBV	215554	383032	27.15%	6.133%
10	19.836	2844	2850	2858	rBV	1075359	1410864	100.00%	22.589%
11	21.457	3120	3126	3140	rBV	243267	437995	31.04%	7.013%
12	21.863	3184	3195	3196	rBV7	10393	25924	1.84%	0.415%
13	24.536	3638	3650	3666	rBV2	164550	472548	33.49%	7.566%




Sum of corrected areas: 6245835

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058867.D
Acq On : 28 Aug 2023 10:30
Operator : MA/JU
Sample : PB155083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB155083BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

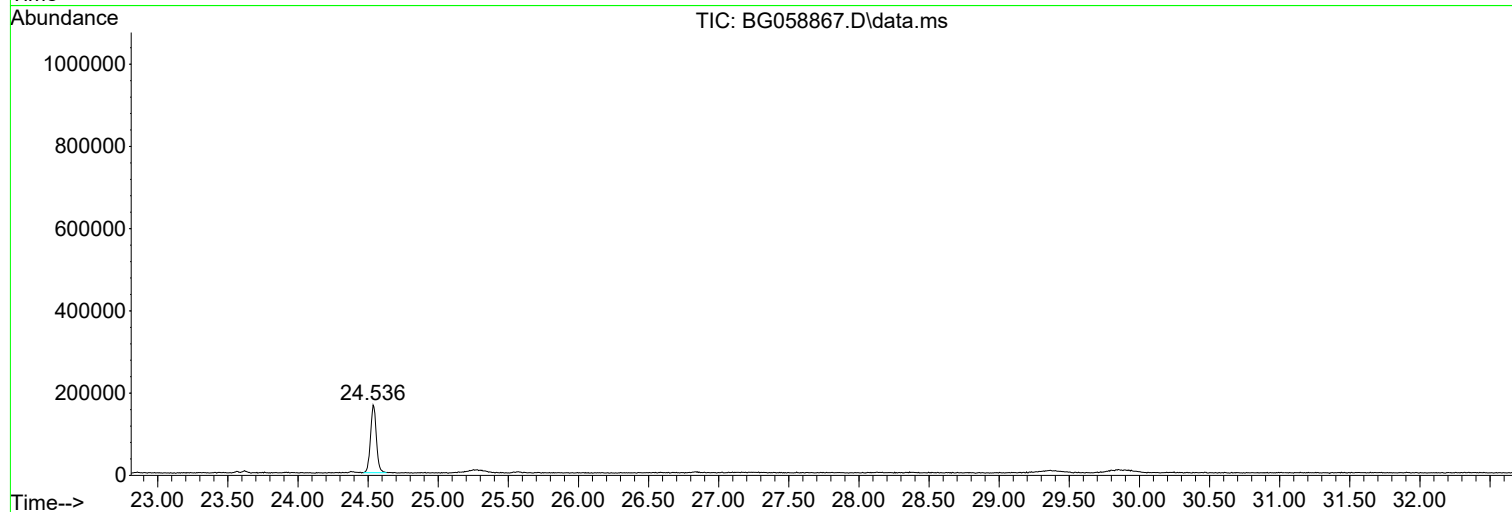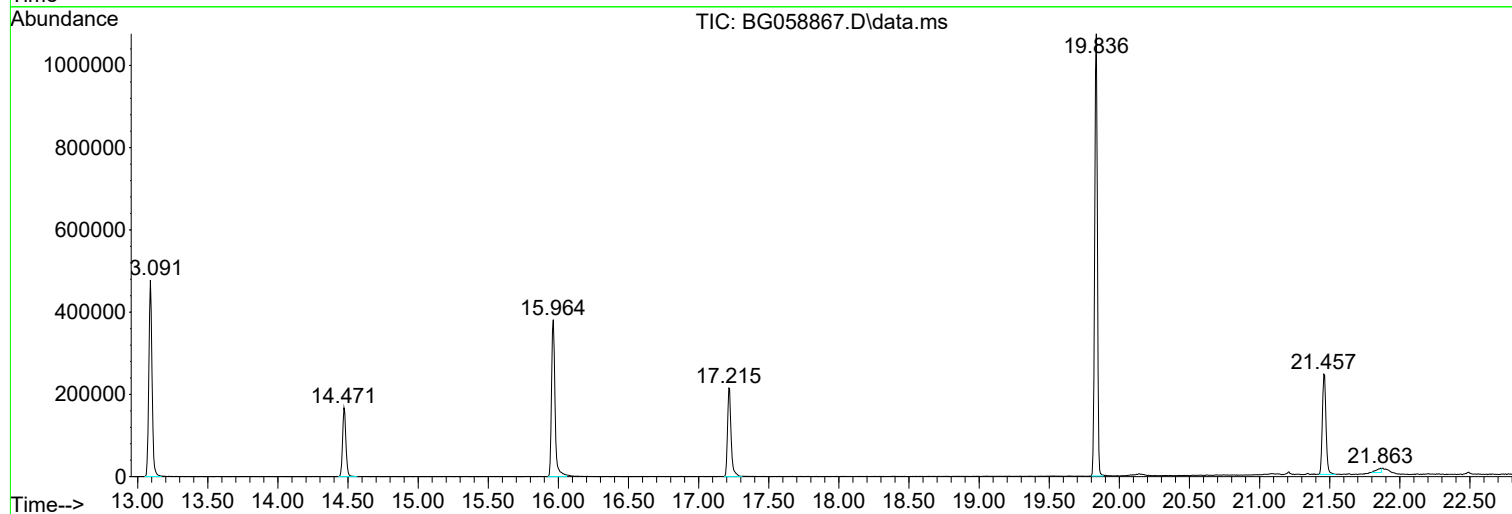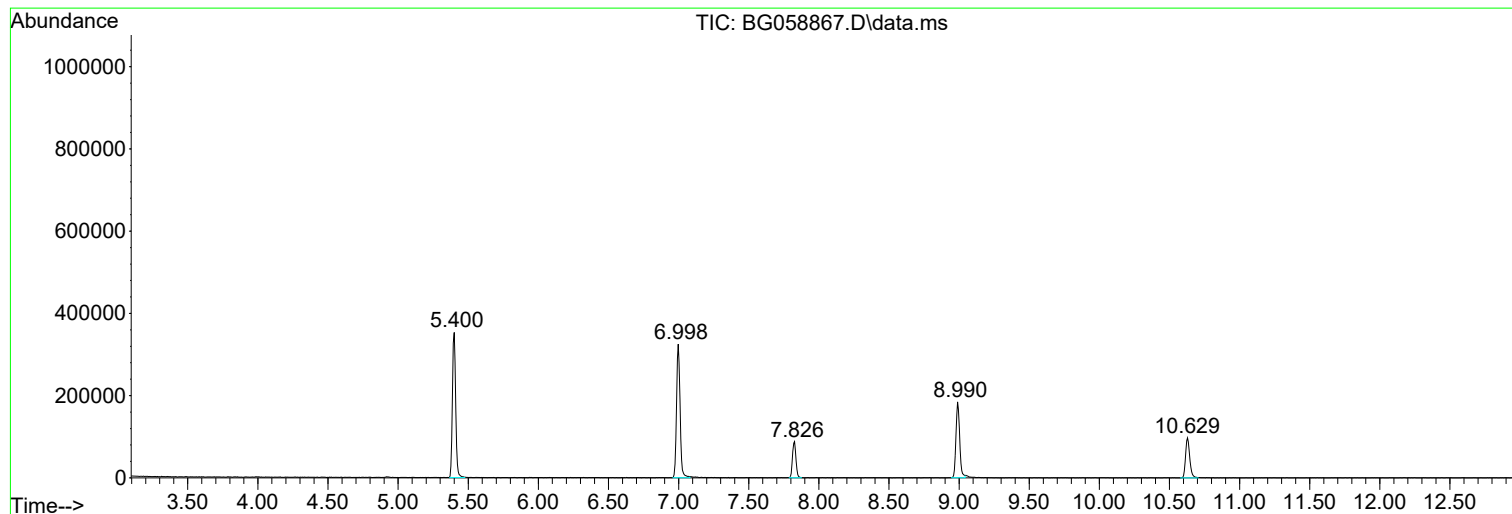

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058867.D
Acq On : 28 Aug 2023 10:30
Operator : MA/JU
Sample : PB155083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB155083BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058867.D
Acq On : 28 Aug 2023 10:30
Operator : MA/JU
Sample : PB155083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB155083BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------