


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058865.D
Acq On : 28 Aug 2023 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 29 14:27:28 2023

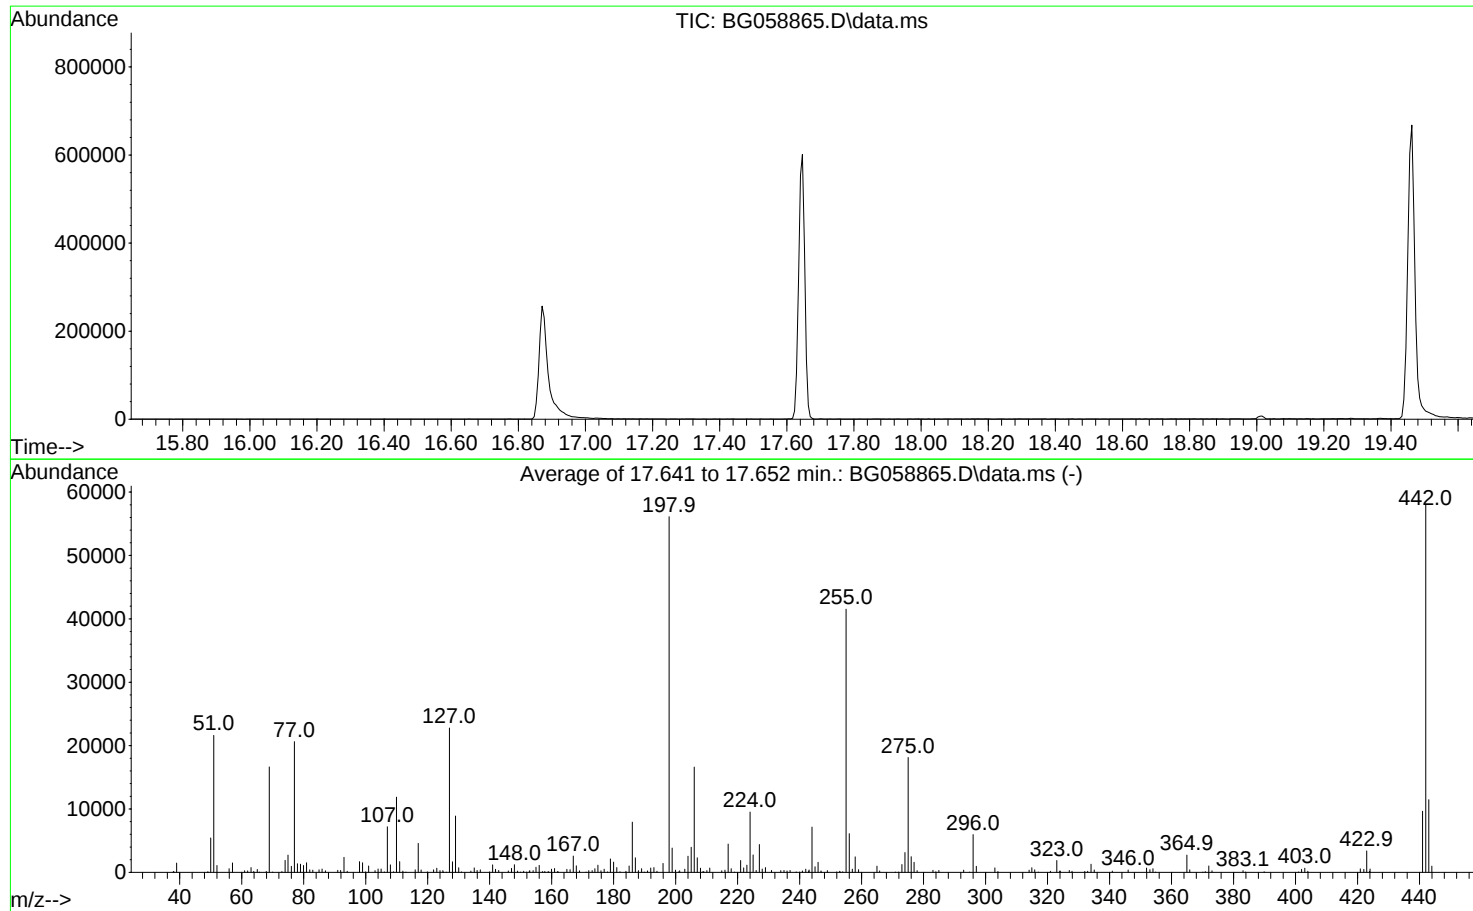




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	21619	PASS
68	69	0.00	2	0.9	152	PASS
69	198	0.00	100	29.6	16632	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	40.6	22777	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56117	PASS
199	198	5	9	6.8	3835	PASS
275	198	10	60	32.3	18122	PASS
365	198	1	100	4.9	2736	PASS
441	198	0.01	100	17.2	9635	PASS
442	442	50	100	100.0	58040	PASS
443	442	15	24	19.7	11450	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058865.D
Acq On : 28 Aug 2023 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 29 02:45:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

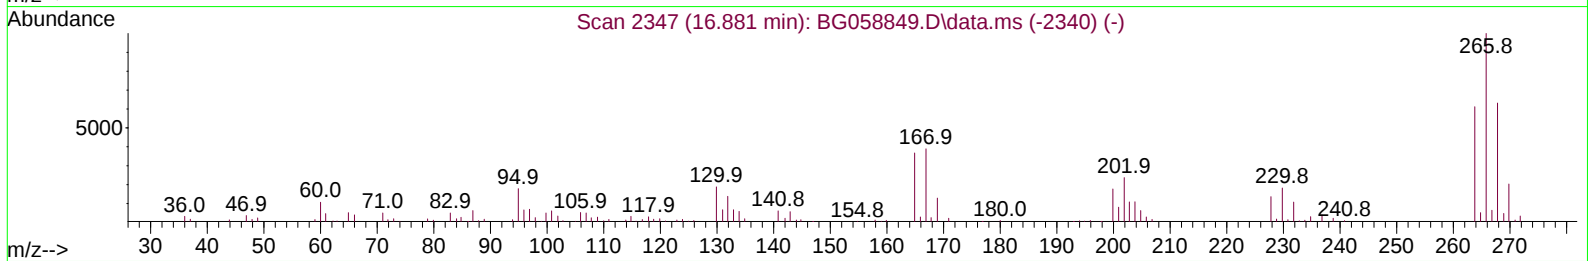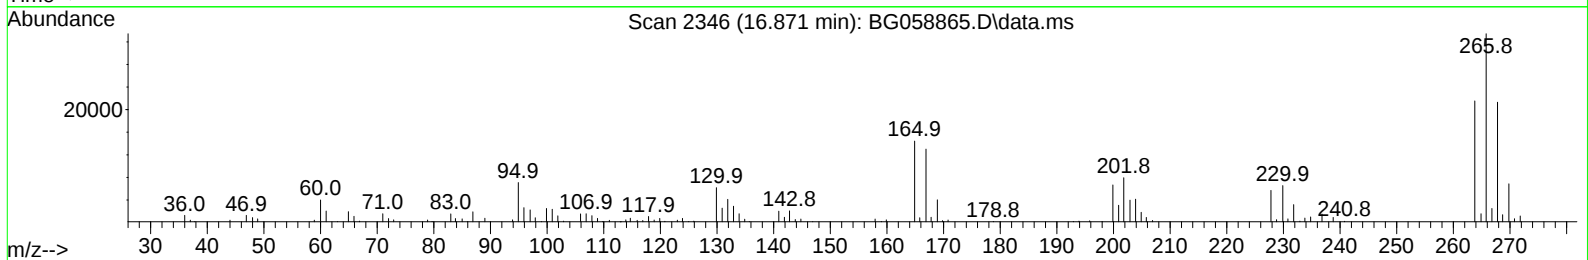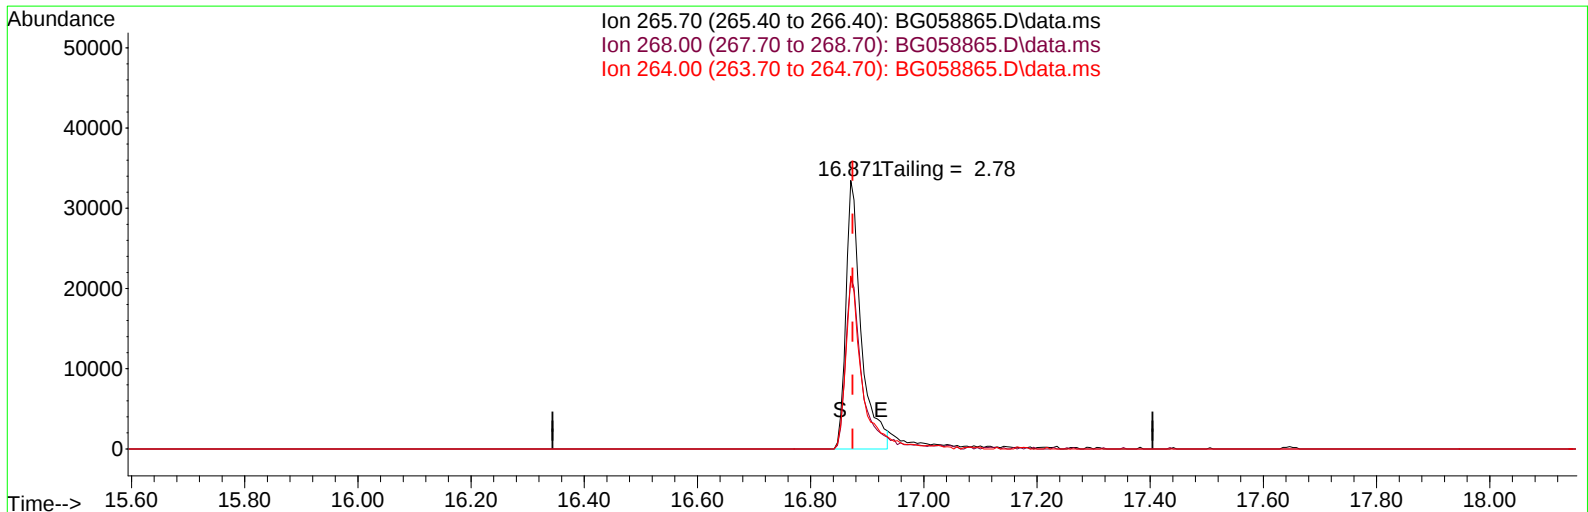

TIC: BG058865.D\data.ms

(70) Pentachlorophenol (C)

16.871min (-0.003) 31995.33 ng




response 68955

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	67.85
264.00	61.90	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082823\
Data File : BG058865.D
Acq On : 28 Aug 2023 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 29 02:45:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

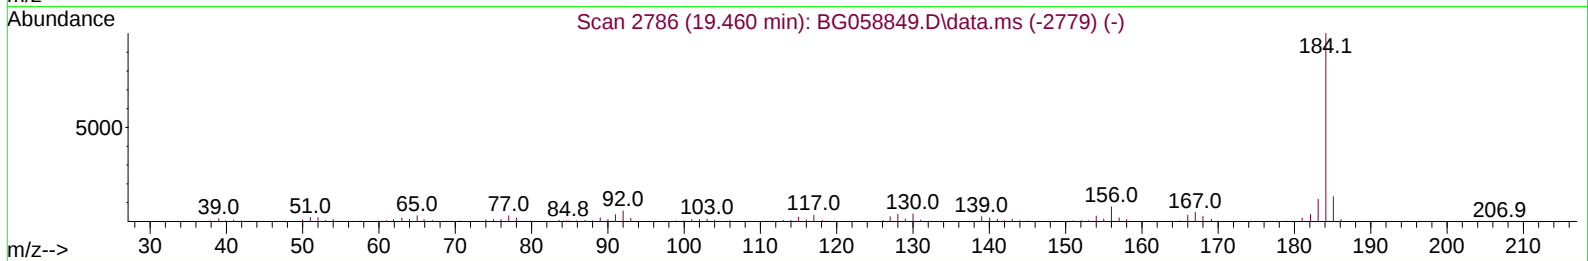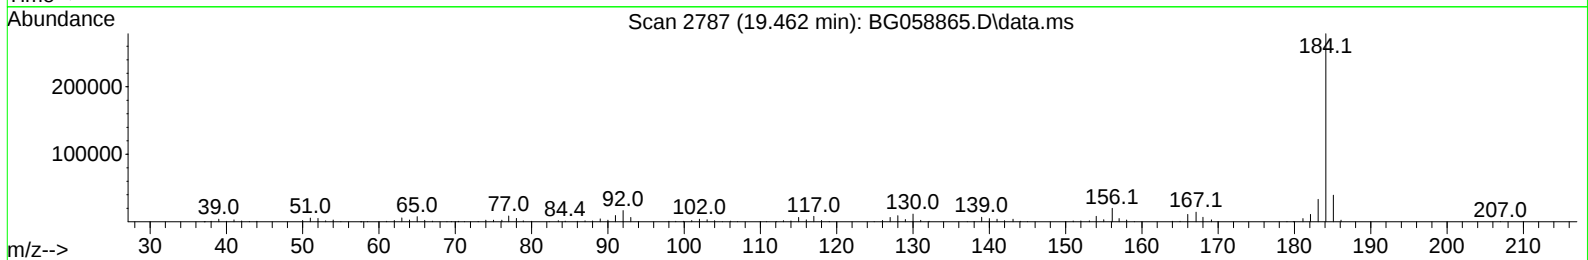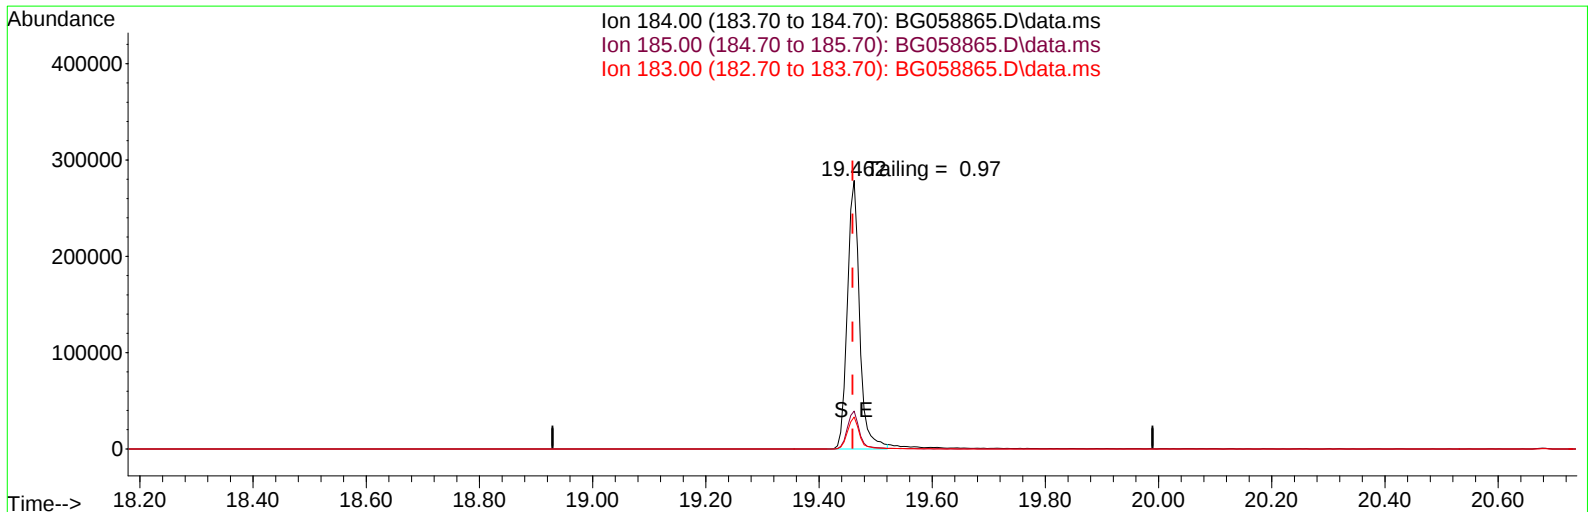

TIC: BG058865.D\data.ms

(77) Benzidine

19.462min (+ 0.003) 0.00 ng

response 426032

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.11
183.00	12.50	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/28/2023	BNA_G	<u>BG058865.D</u>
Compound Name	Response	Retention Time
DDT	208715	20.678
DDD	5829	20.249
DDE	406	19.744
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6235	214950	2.90

Instrument :
BNA_G
ClientSampleId :
DFTPP