
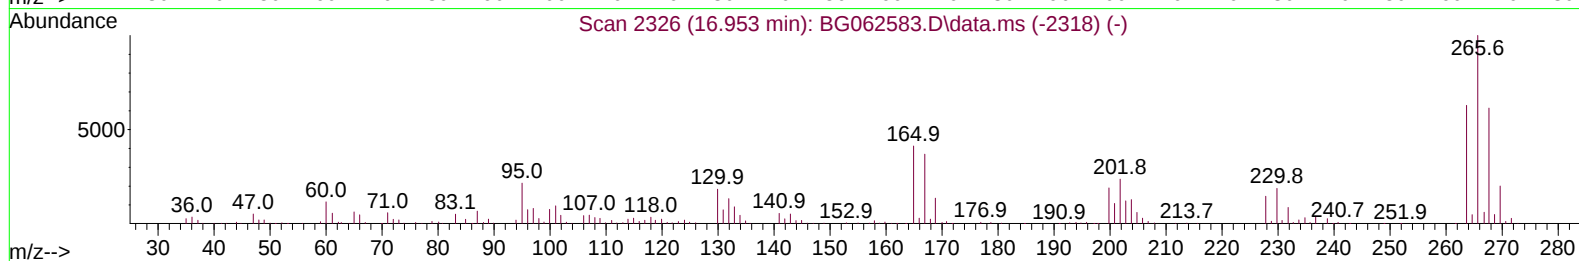
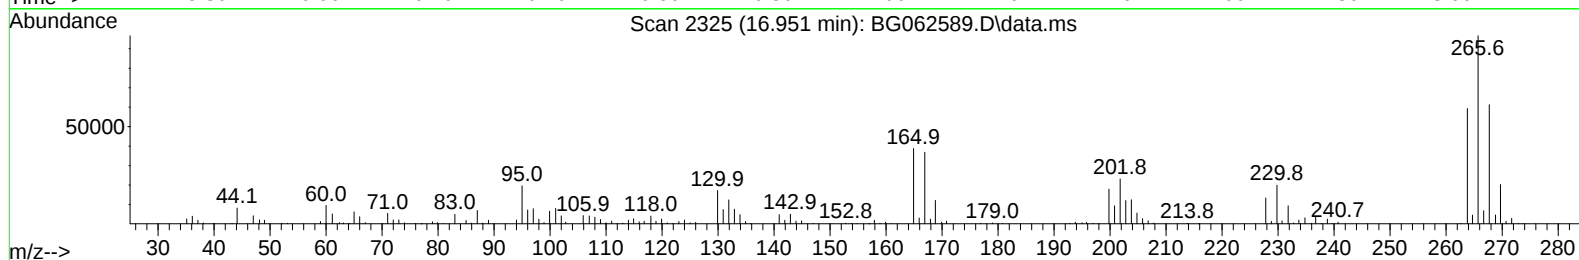


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG082824\  
Data File : BG062589.D  
Acq On : 28 Aug 2024 10:16  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 10:52:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG082724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 28 00:59:59 2024  
Response via : Initial Calibration

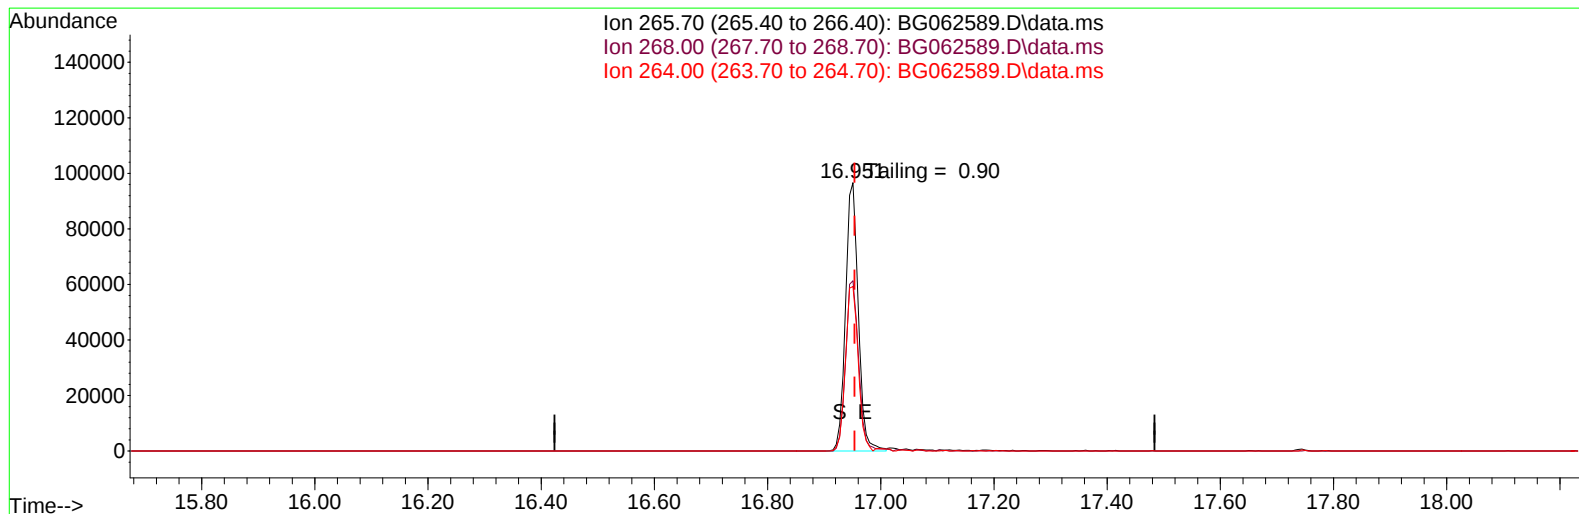

TIC: BG062589.D\data.ms

**(70) Pentachlorophenol (C)**




**16.951min (-0.003) 59827.54 ng**

**response 151546**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.40  | 63.42  |
| 264.00 | 67.80  | 66.05  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG082824\  
Data File : BG062589.D  
Acq On : 28 Aug 2024 10:16  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 10:52:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG082724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 28 00:59:59 2024  
Response via : Initial Calibration

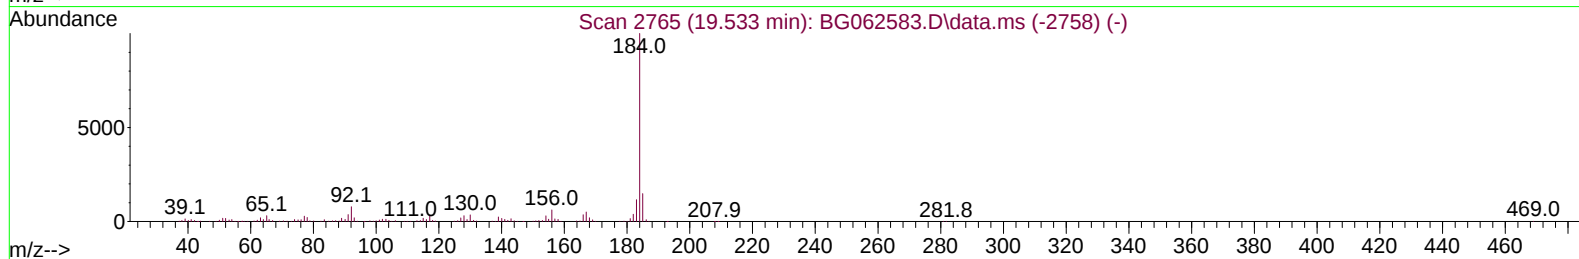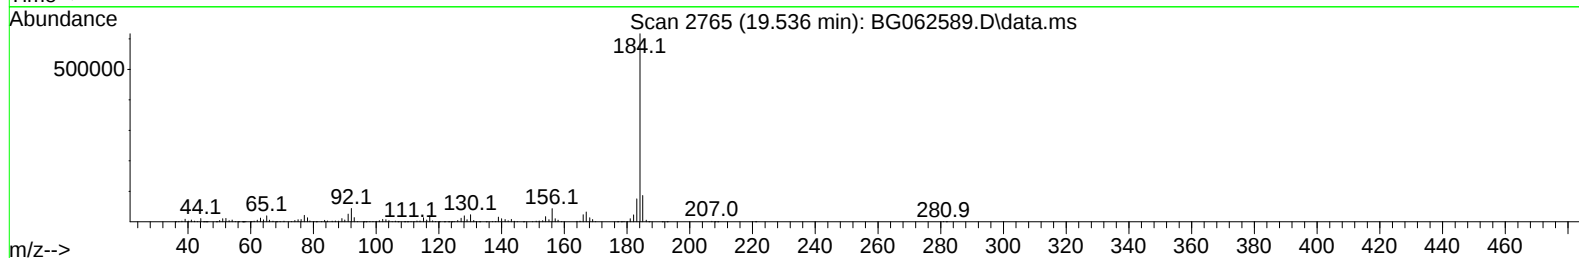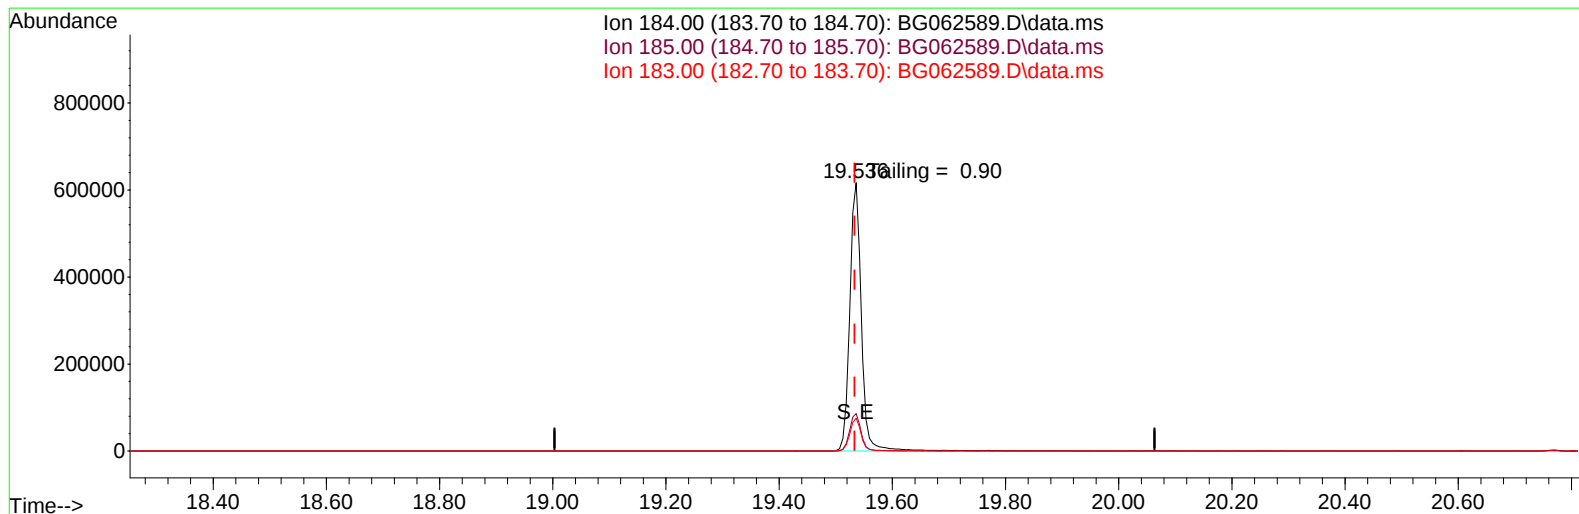

TIC: BG062589.D\data.ms

**(77) Benzidine****19.536min (+ 0.003) 16688.08 ng****response 872502**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 13.95  |
| 183.00 | 11.60  | 12.24  |
| 0.00   | 0.00   | 0.00   |