
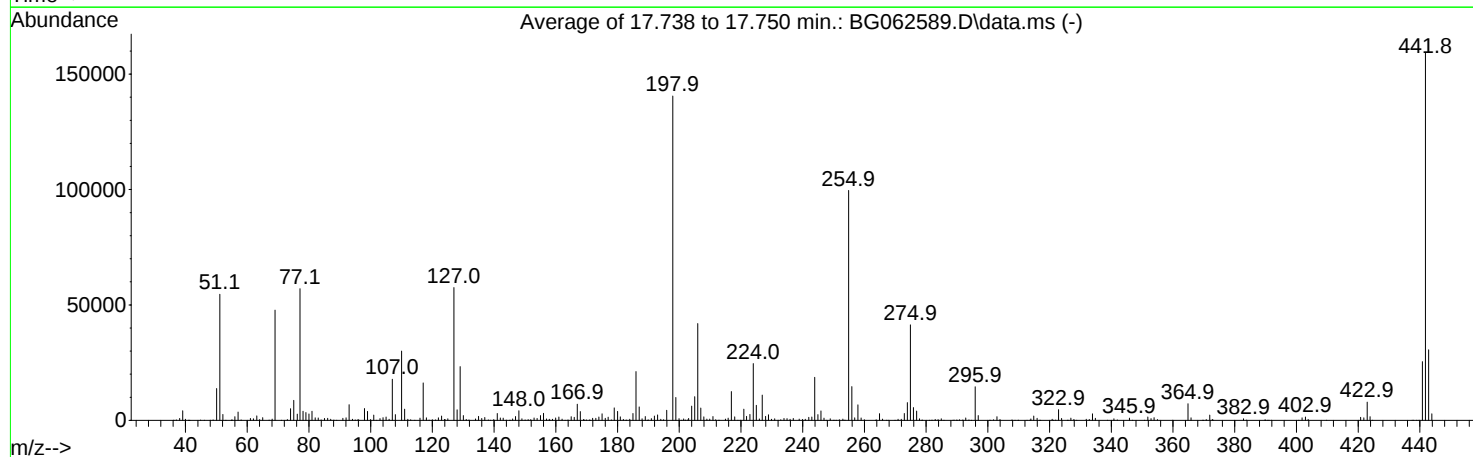


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082824\
Data File : BG062589.D
Acq On : 28 Aug 2024 10:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 28 00:59:59 2024

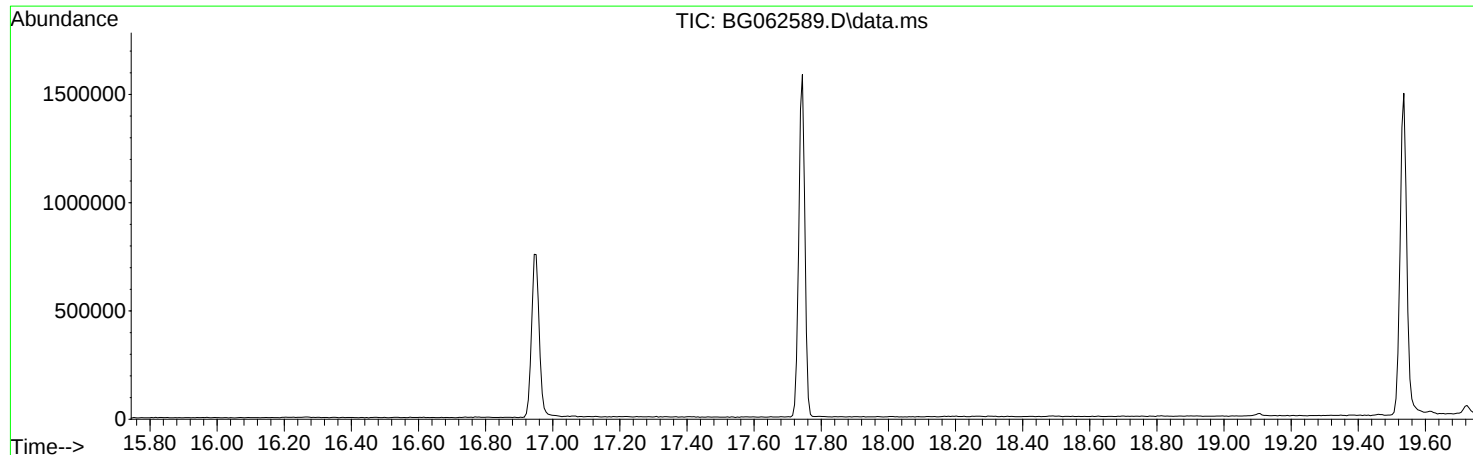

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	54598	PASS
68	69	0.00	2	1.2	584	PASS
69	198	0.00	100	34.0	47781	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	57509	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140515	PASS
199	198	5	9	7.0	9894	PASS
275	198	10	60	29.4	41365	PASS
365	198	1	100	5.1	7236	PASS
441	198	0.01	100	18.1	25435	PASS
442	442	50	100	100.0	159360	PASS
443	442	15	24	19.2	30592	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/28/2024	BNA_G	<u>BG062589.D</u>
Compound Name	Response	Retention Time
DDT	352997	20.77
DDD	6971	20.329
DDE	119	19.824
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7090	360087	1.97

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082824\
Data File : BG062589.D
Acq On : 28 Aug 2024 10:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 28 10:52:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 00:59:59 2024
Response via : Initial Calibration

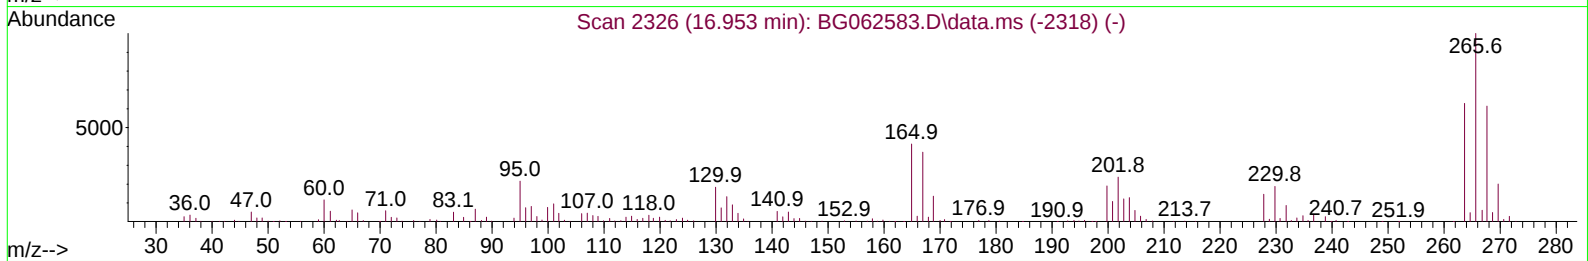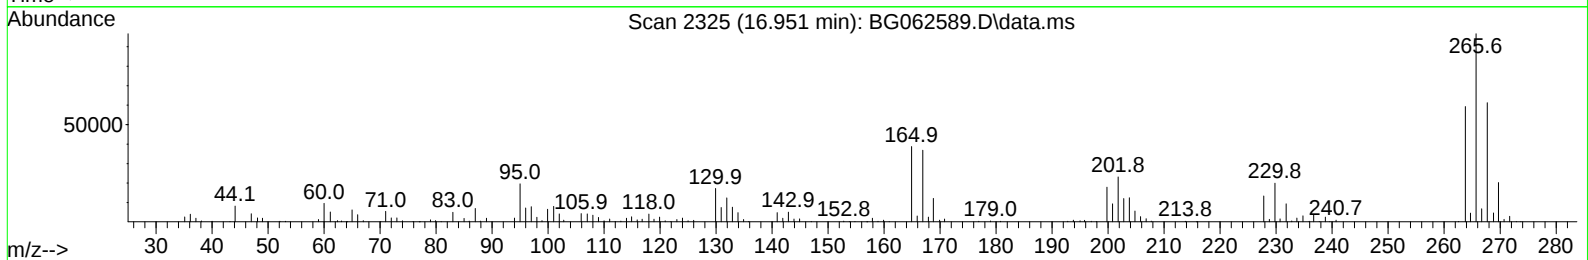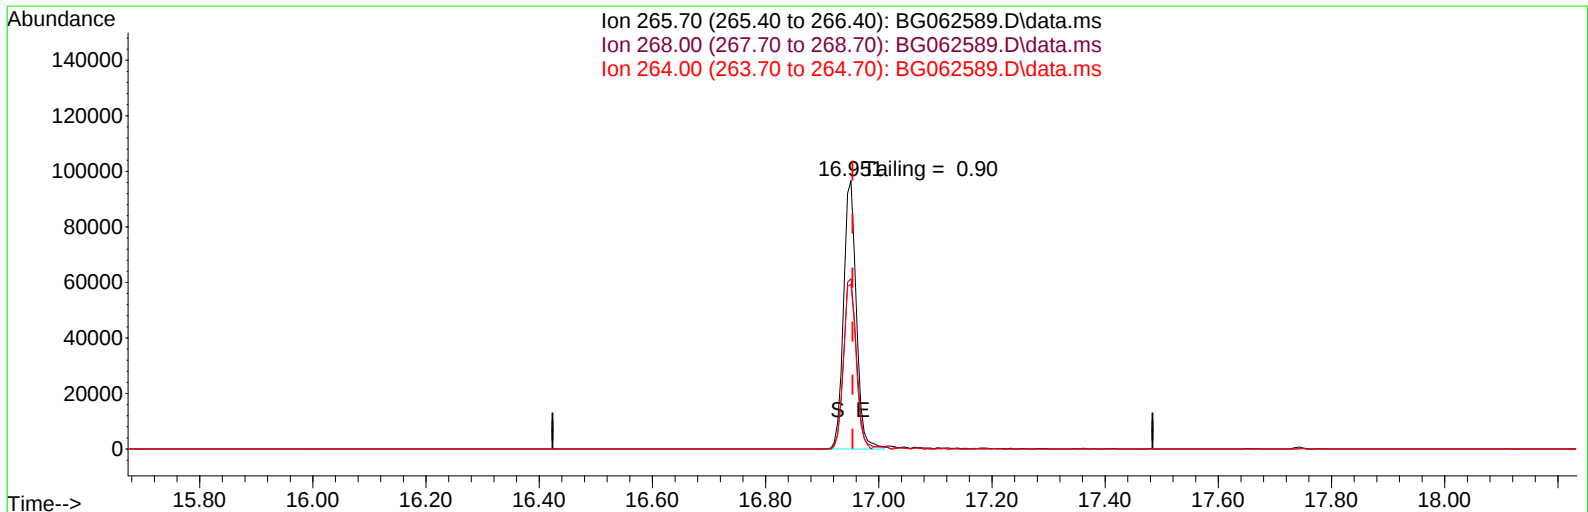

TIC: BG062589.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.003) 59827.54 ng




response 151546

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.40	63.42
264.00	67.80	66.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082824\
Data File : BG062589.D
Acq On : 28 Aug 2024 10:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 28 10:52:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 00:59:59 2024
Response via : Initial Calibration

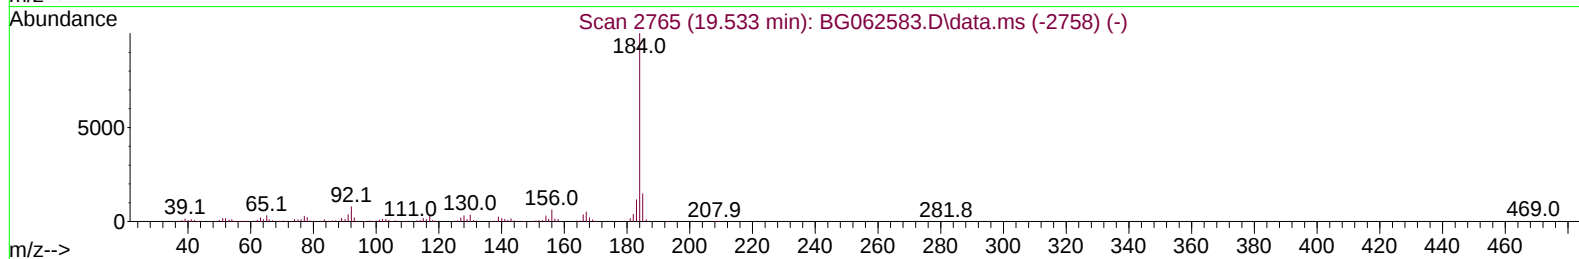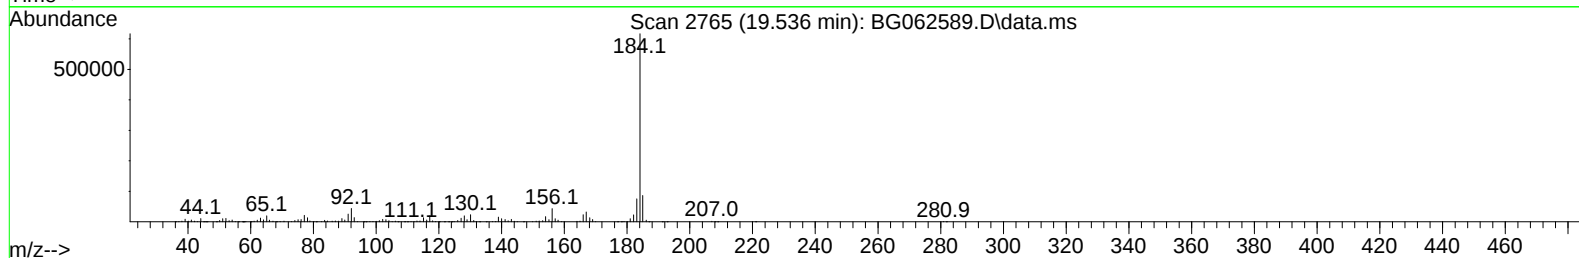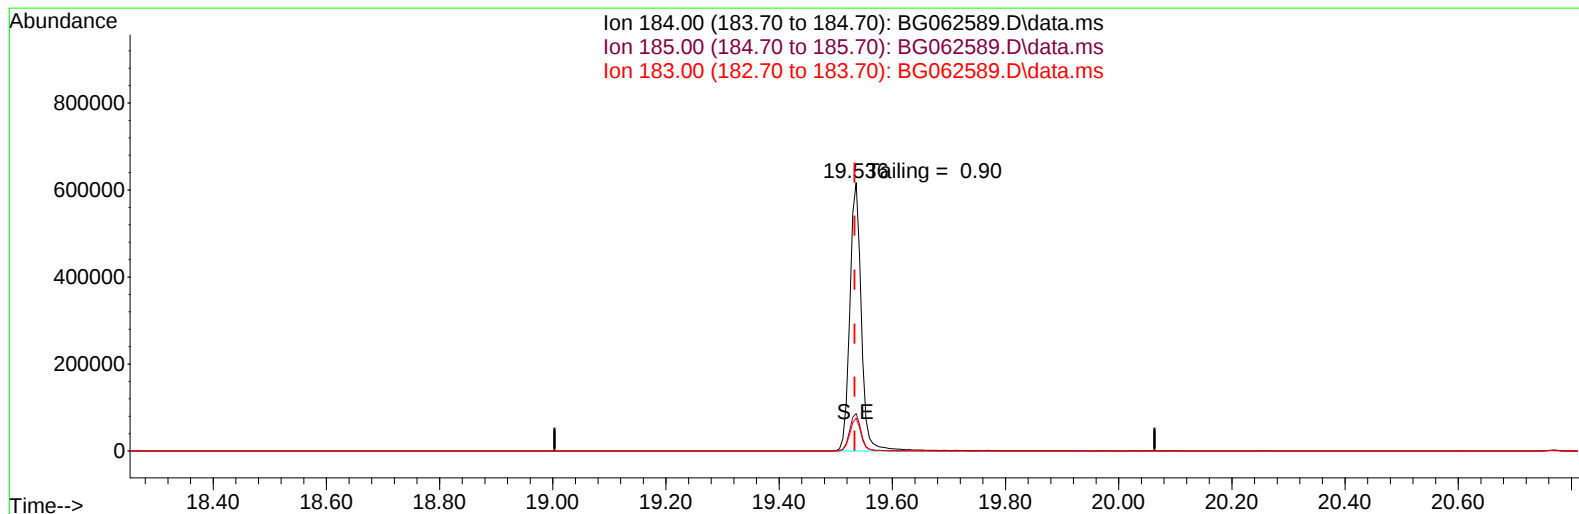

TIC: BG062589.D\data.ms

(77) Benzidine

19.536min (+ 0.003) 16688.08 ng

response 872502

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.95
183.00	11.60	12.24
0.00	0.00	0.00