
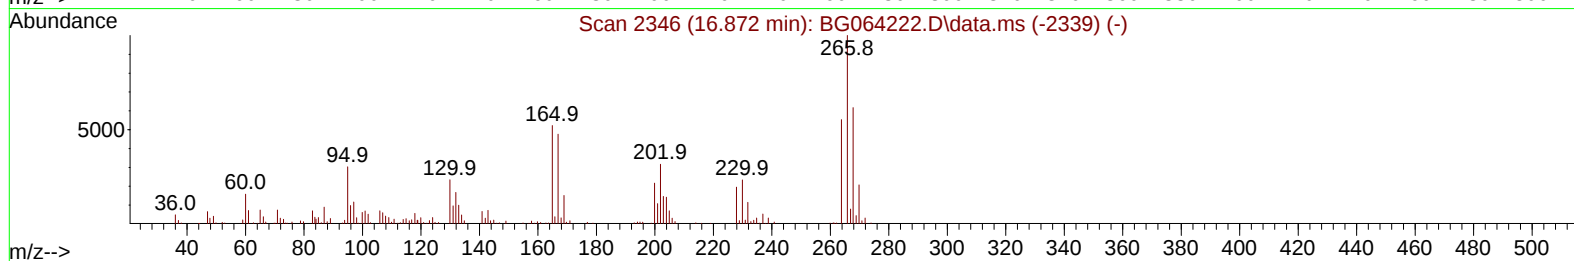
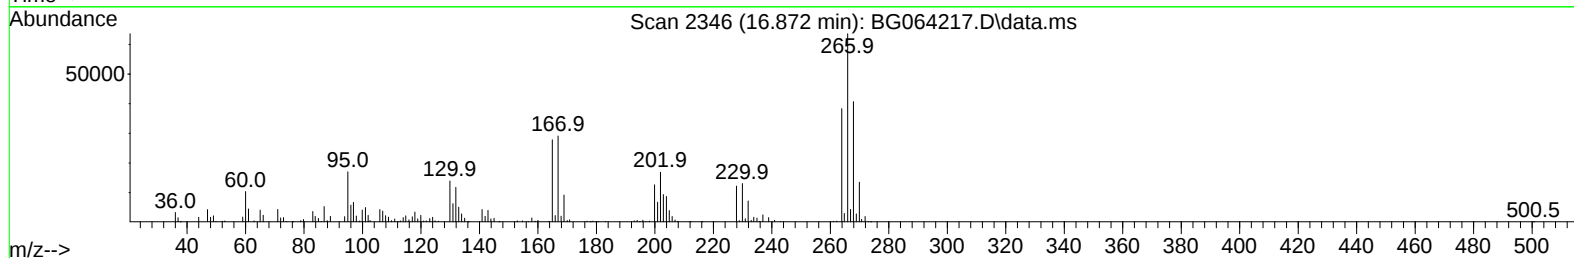


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082825\
Data File : BG064217.D
Acq On : 28 Aug 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 14:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 14:36:10 2025
Response via : Initial Calibration

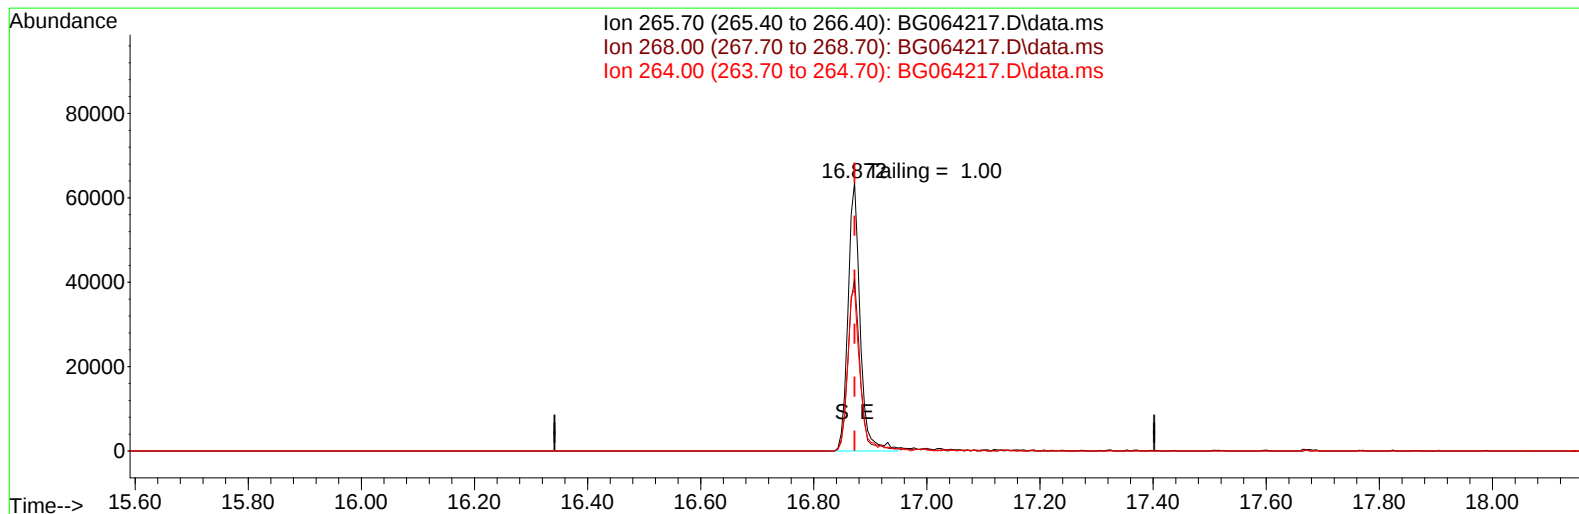

TIC: BG064217.D\data.ms

(70) Pentachlorophenol (C)




16.872min (-0.000) 25238.02 ng

response 93526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.00
264.00	55.40	60.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082825\
Data File : BG064217.D
Acq On : 28 Aug 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 14:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 14:36:10 2025
Response via : Initial Calibration

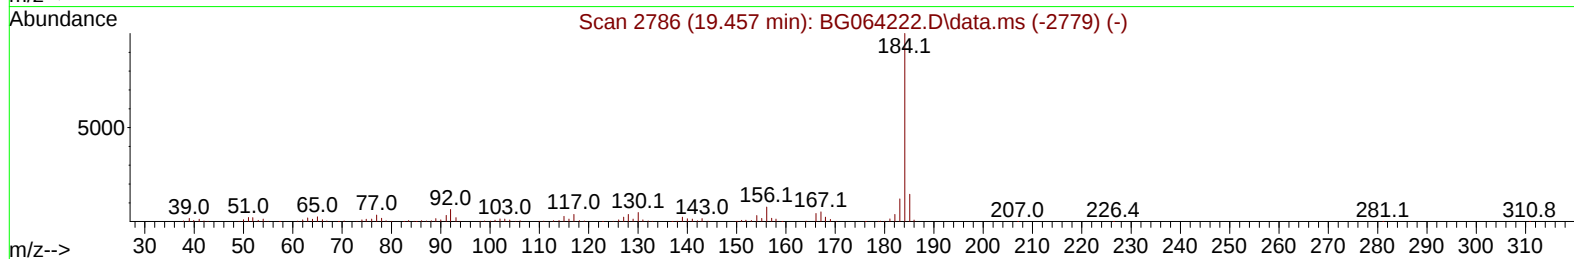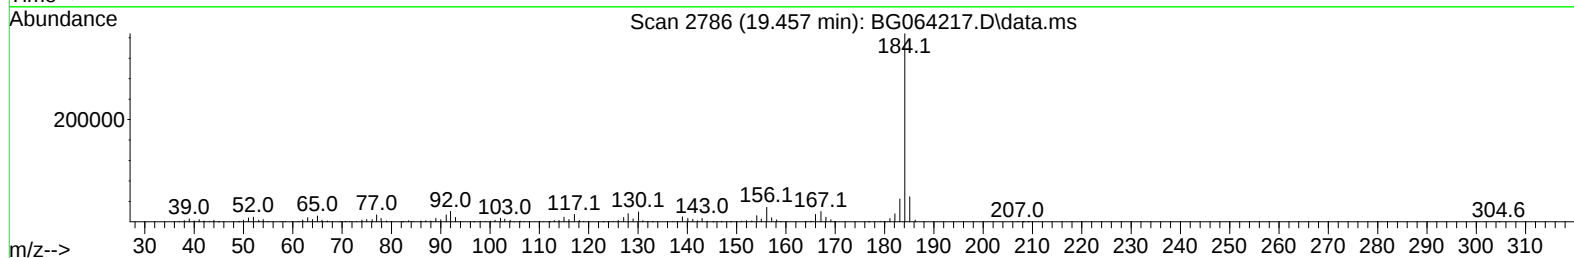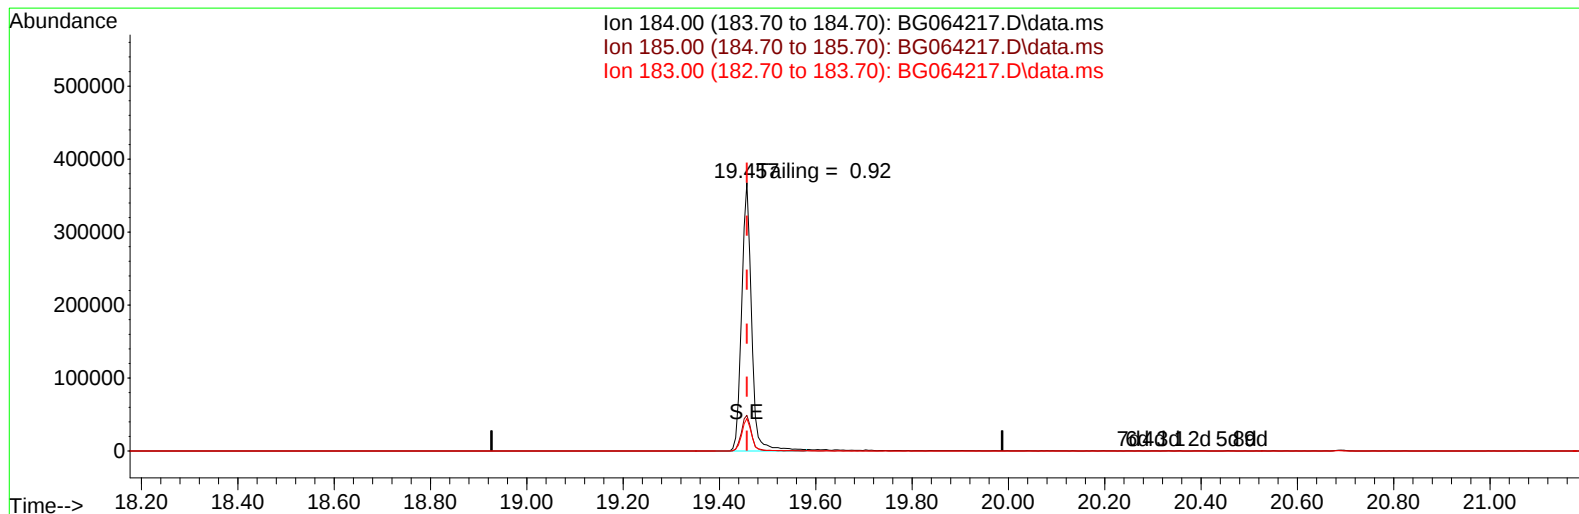

TIC: BG064217.D\data.ms

(77) Benzidine

19.457min (-0.000) 328145.89 ng m

response 550762

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.29
183.00	12.10	12.10
0.00	0.00	0.00