

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082919\
 Data File : BG042580.D
 Acq On : 30 Aug 2019 00:40
 Operator : HP/JU
 Sample : K4514-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S602-M-2.0-2.5-082319

Quant Time: Aug 30 05:37:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	34880	20.00	ng	-0.01
21) Naphthalene-d8	10.82	136	135268	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	99222	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	233495	20.00	ng	-0.01
76) Chrysene-d12	21.69	240	248061	20.00	ng	-0.01
87) Perylene-d12	24.92	264	295922	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	160948	93.45	ng	0.00
7) Phenol-d6	7.16	99	213231	91.66	ng	-0.01
23) Nitrobenzene-d5	9.16	82	117764	60.16	ng	-0.01
42) 2,4,6-Tribromophenol	16.15	330	106523	75.53	ng	-0.01
45) 2-Fluorobiphenyl	13.28	172	255726	43.59	ng	0.00
79) Terphenyl-d14	20.02	244	429567	37.44	ng	-0.01
Target Compounds						
10) Phenol	7.19	94	12401	5.243	ng	88
19) n-Nitroso-di-n-propylamine	9.16	70	15430	10.238	ng	# 68
50) Dimethylphthalate	14.11	163	44139	6.165	ng	98
51) 2,6-Dinitrotoluene	14.65	165	12766	7.693	ng	# 36
57) 2,4-Dinitrotoluene	14.65	165	12766	5.372	ng	# 38
67) 4-Bromophenyl-phenylether	16.15	248	7089	2.394	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082919\
Data File : BG042580.D
Acq On : 30 Aug 2019 00:40
Operator : HP/JU
Sample : K4514-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S602-M-2.0-2.5-082319

Quant Time: Aug 30 05:37:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

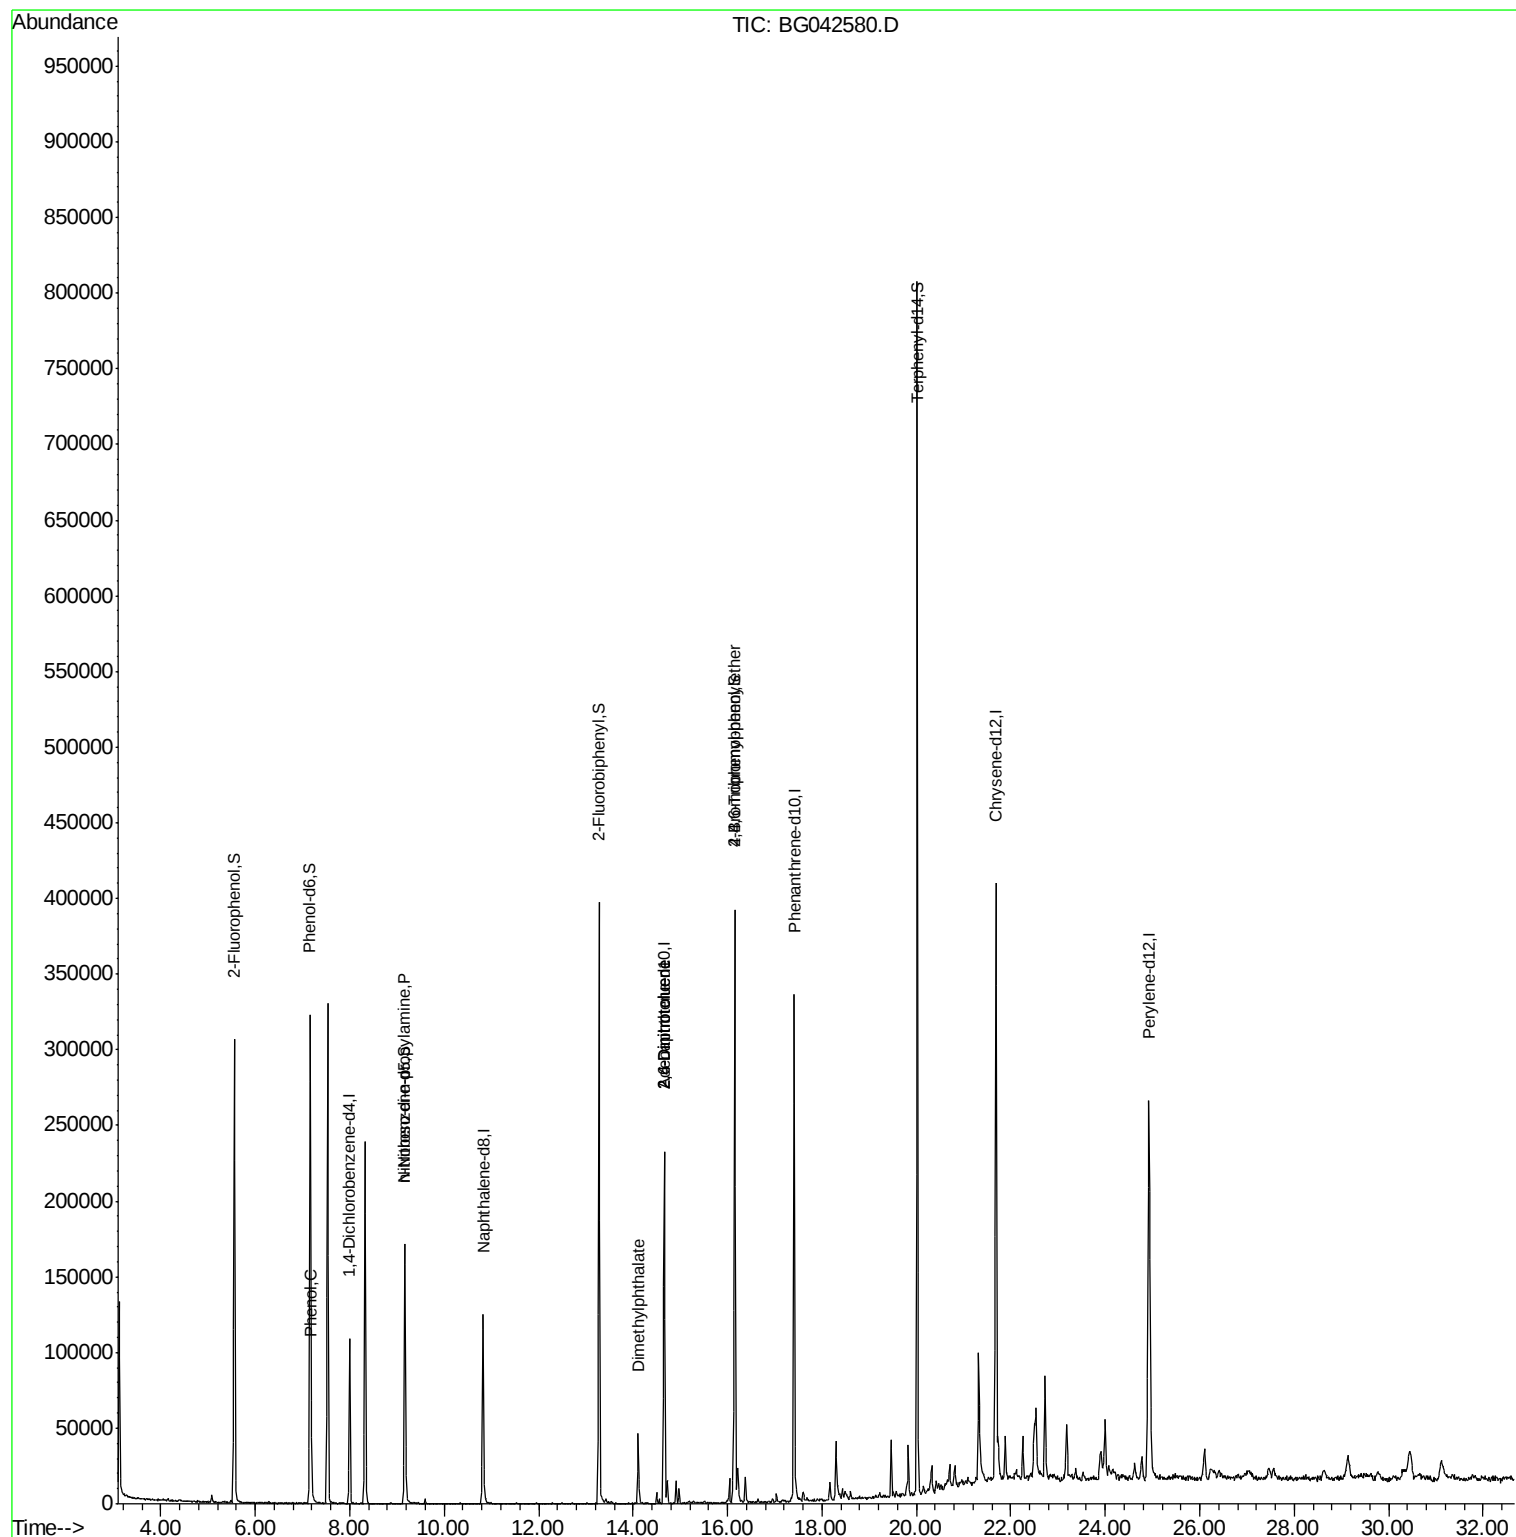







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 835
Delta R.T. -0.01 min
Lab File: BG042580.D
Acq: 30 Aug 2019 00:40

Instrument :
BNA_G
ClientSampleId :
S602-M-2.0-2.5-082319




Tgt Ion:152 Resp: 34880
Ion Ratio Lower Upper
152 100
150 150.2 125.4 188.0
115 49.2 38.5 57.7

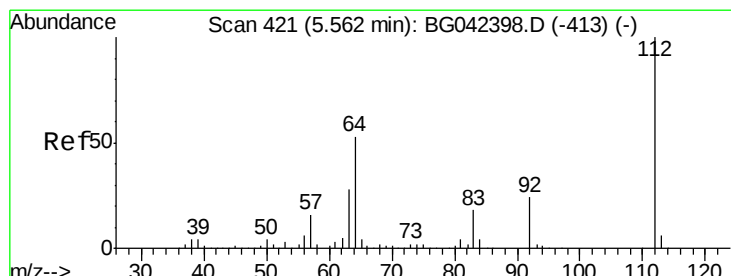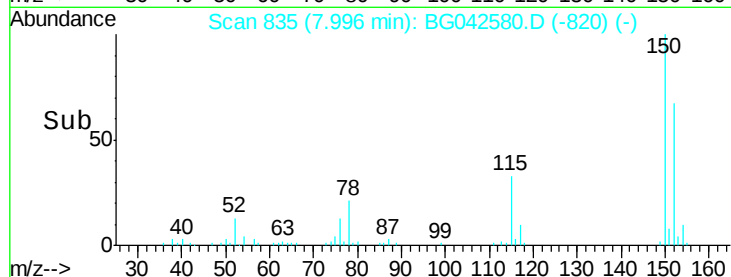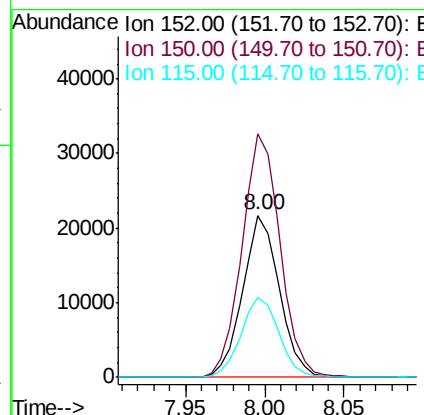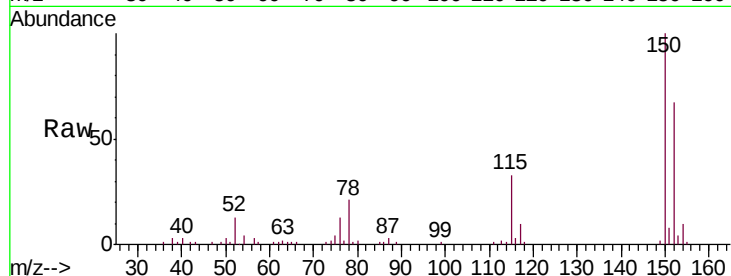


#5

2-Fluorophenol
Concen: 93.454 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.00 min
Lab File: BG042580.D
Acq: 30 Aug 2019 00:40

Tgt Ion:112 Resp: 160948
Ion Ratio Lower Upper
112 100
64 52.9 42.8 64.2
63 28.5 22.7 34.1

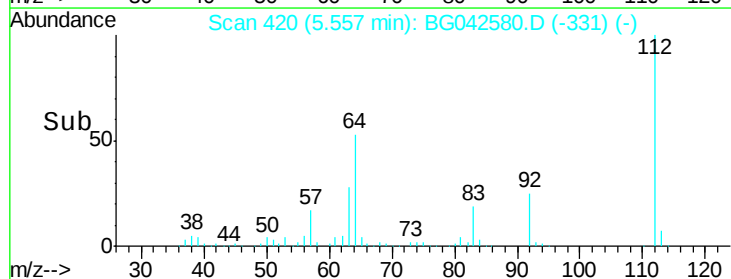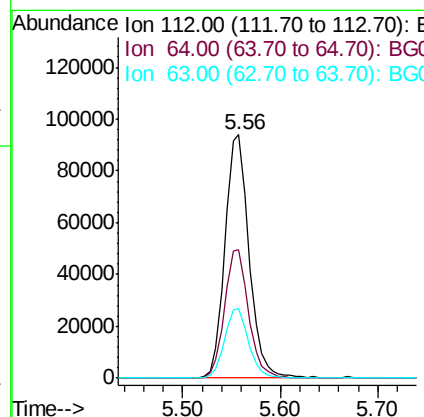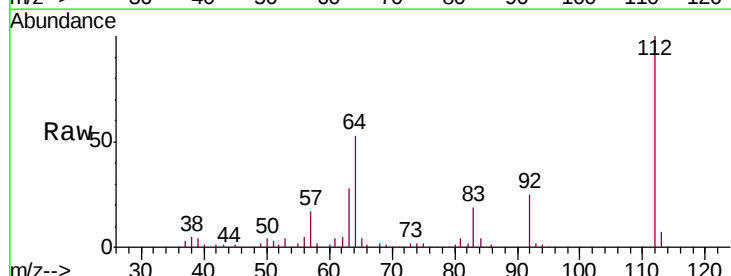

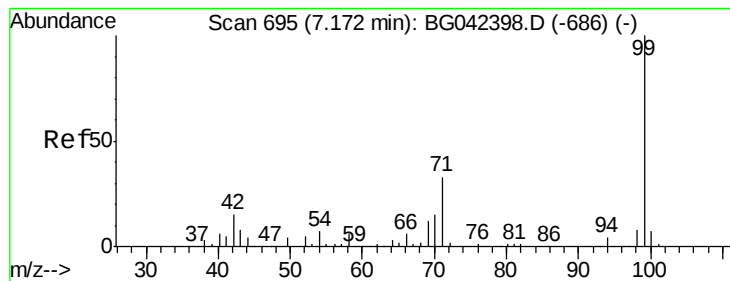

#7

Phenol-d6

Concen: 91.660 ng

RT: 7.16 min Scan# 693

Delta R.T. -0.01 min

Lab File: BG042580.D

Acq: 30 Aug 2019 00:40

Instrument :

BNA_G

ClientSampleId :

S602-M-2.0-2.5-082319


Tgt Ion: 99 Resp: 213231

Ion Ratio Lower Upper




99 100

42 15.1 12.0 18.0

71 34.8 26.3 39.5

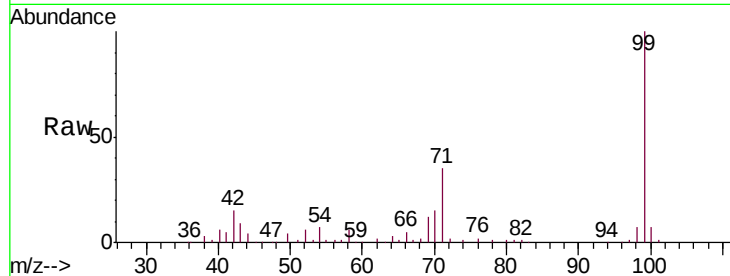

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

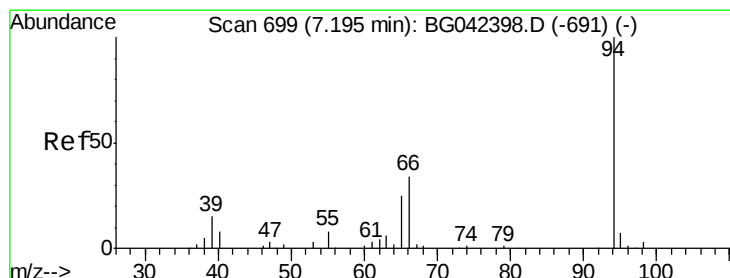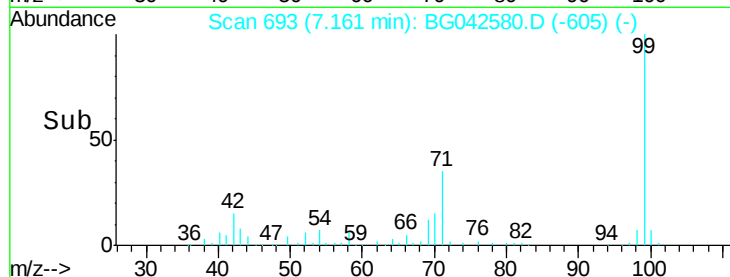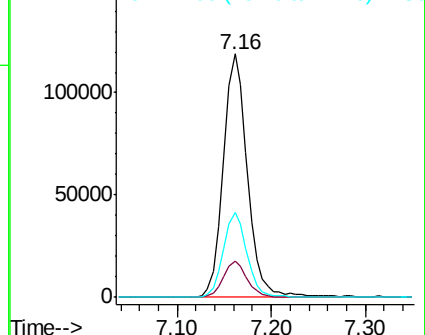

#10

Phenol

Concen: 5.243 ng

RT: 7.19 min Scan# 698

Delta R.T. -0.00 min

Lab File: BG042580.D

Acq: 30 Aug 2019 00:40


Tgt Ion: 94 Resp: 12401

Ion Ratio Lower Upper



94 100



65 30.0 5.6 45.6

66 44.8 16.0 56.0

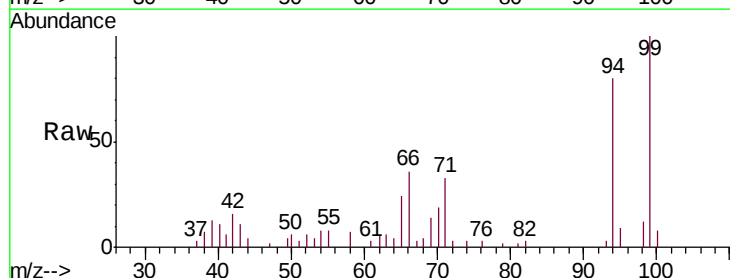

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



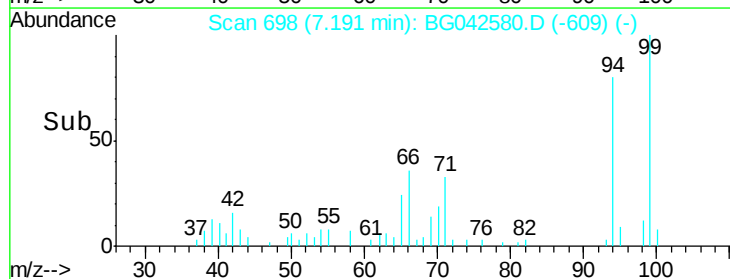
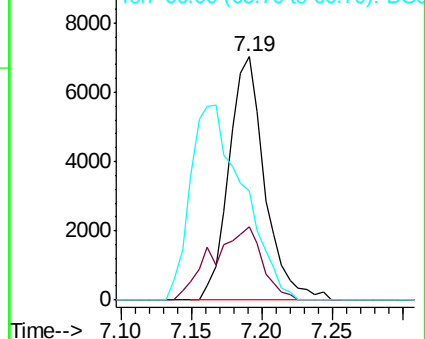


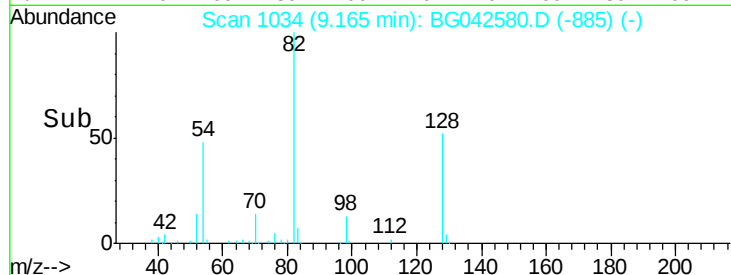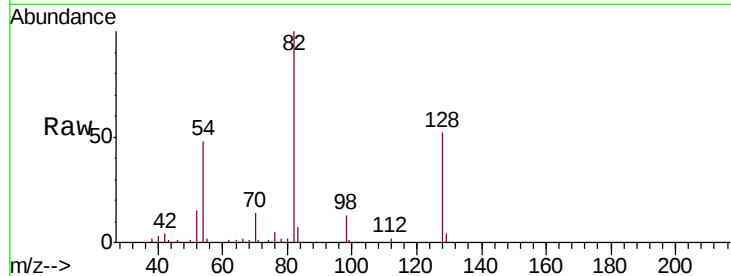

#19
n-Nitroso-di-n-propylamine
Concen: 10.238 ng
RT: 9.16 min Scan# 1034
Delta R.T. 0.35 min
Lab File: BG042580.D
Acq: 30 Aug 2019 00:40


Instrument :
BNA_G
ClientSampleId :
S602-M-2.0-2.5-082319

Tgt Ion: 70 Resp: 15430
Ion Ratio Lower Upper
70 100
42 31.5 38.8 58.2#
101 0.0 9.0 13.6#
130 2.1 20.0 30.0#

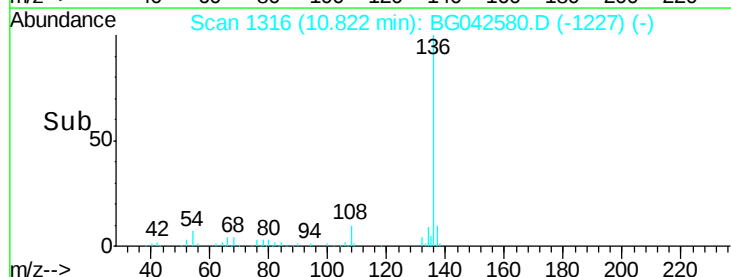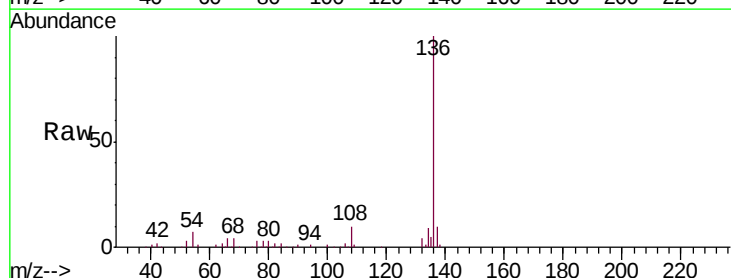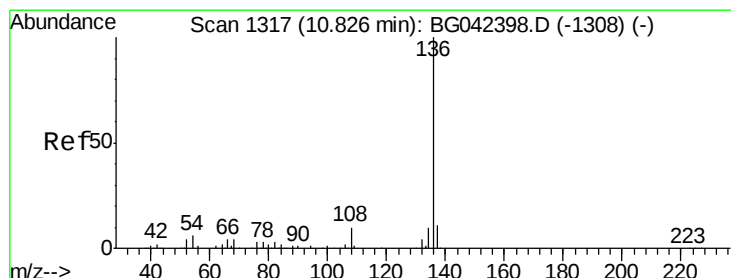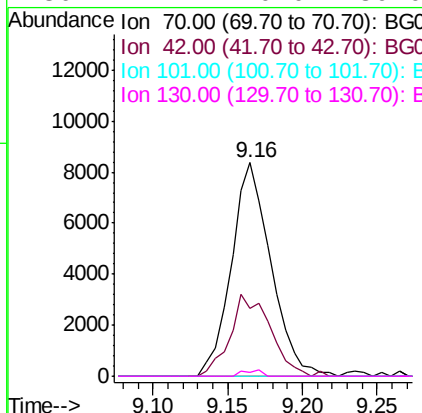

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.82 min Scan# 1316
Delta R.T. -0.00 min
Lab File: BG042580.D
Acq: 30 Aug 2019 00:40

Tgt Ion: 136 Resp: 135268
Ion Ratio Lower Upper
136 100
137 10.3 8.7 13.1
54 6.5 4.9 7.3
68 3.6 3.6 5.4#




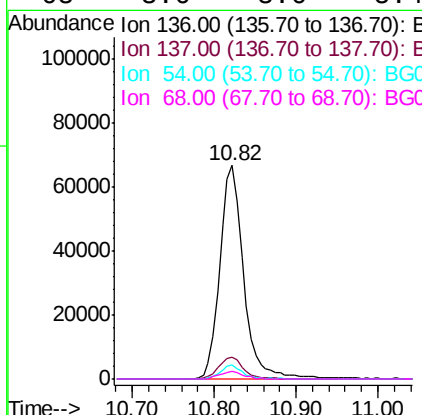




#23
 Nitrobenzene-d5
 Concen: 60.162 ng
 RT: 9.16 min Scan# 1034
 Delta R.T. -0.01 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40




Instrument :
 BNA_G
 ClientSampleId :
 S602-M-2.0-2.5-082319


Tgt Ion: 82 Resp: 117764
 Ion Ratio Lower Upper
 82 100
 128 52.1 40.7 61.1
 54 48.5 36.3 54.5

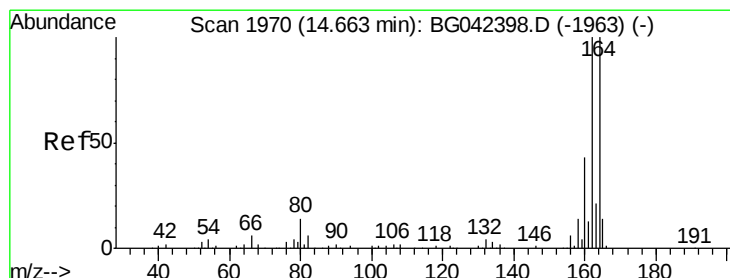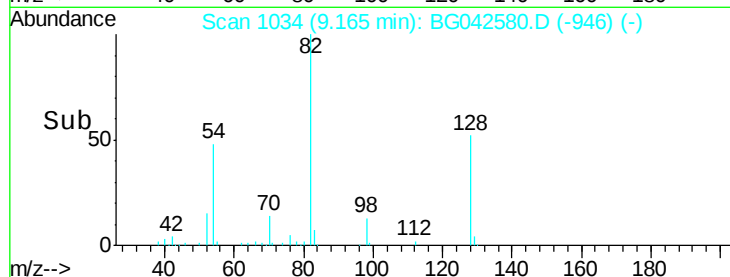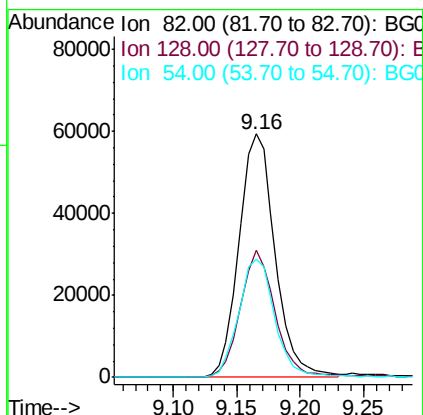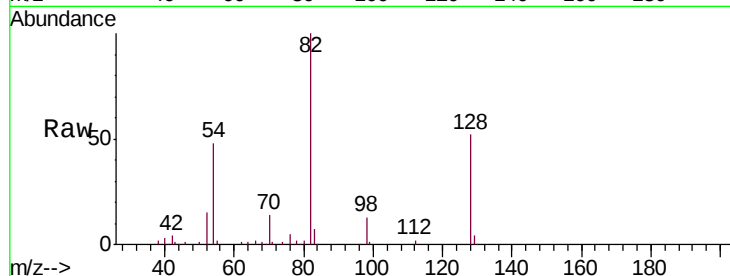

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1969
 Delta R.T. -0.00 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Tgt Ion: 164 Resp: 99222
 Ion Ratio Lower Upper
 164 100
 162 102.9 79.9 119.9
 160 45.9 34.3 51.5

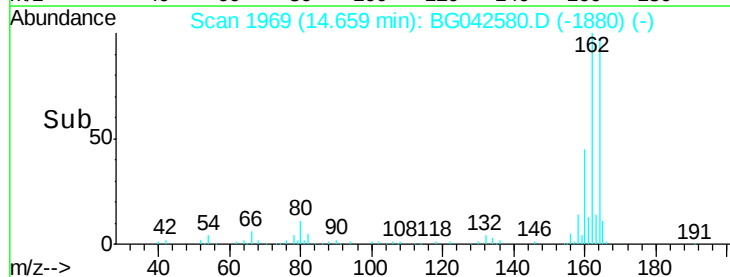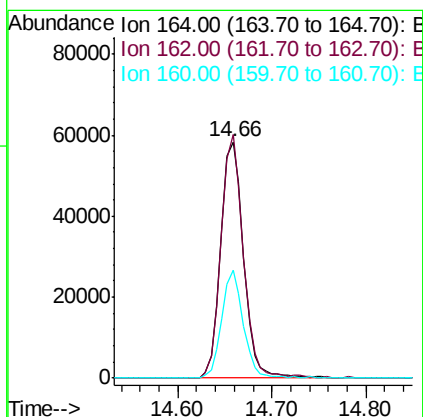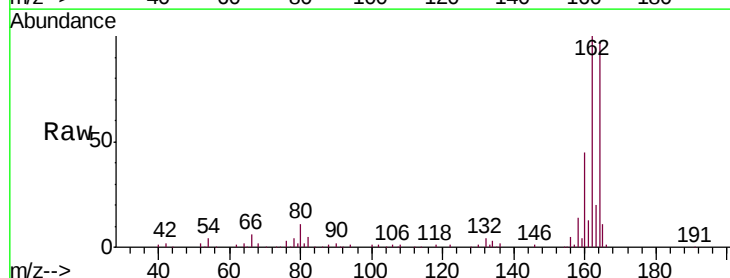


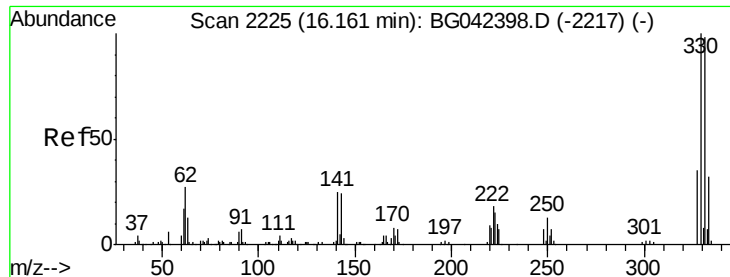




#42
 2,4,6-Tribromophenol
 Concen: 75.533 ng
 RT: 16.15 min Scan# 2223
 Delta R.T. -0.01 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Instrument :
 BNA_G
 ClientSampleId :
 S602-M-2.0-2.5-082319

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.6	77.4	116.0
141	26.7	21.4	32.0

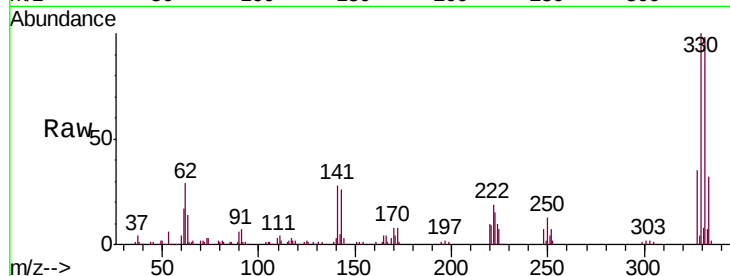


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

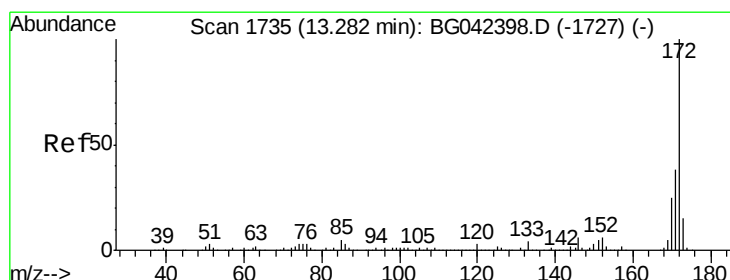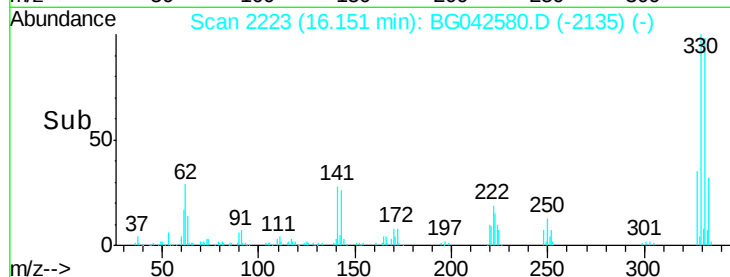
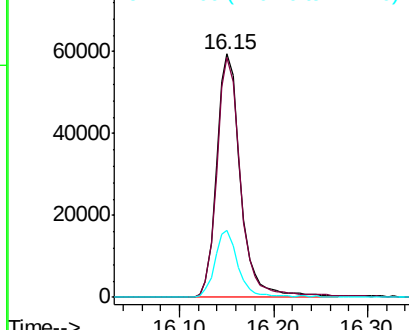


#45
 2-Fluorobiphenyl
 Concen: 43.590 ng
 RT: 13.28 min Scan# 1734
 Delta R.T. -0.00 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	30.5	45.7
170	23.3	20.2	30.2

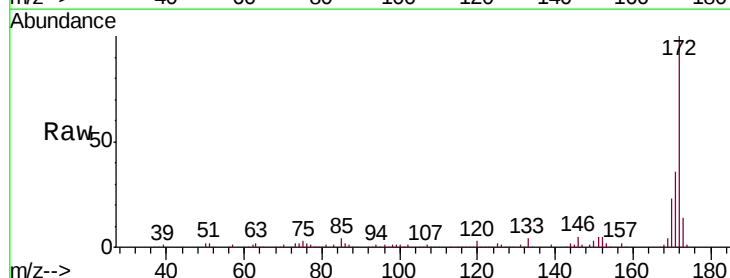

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

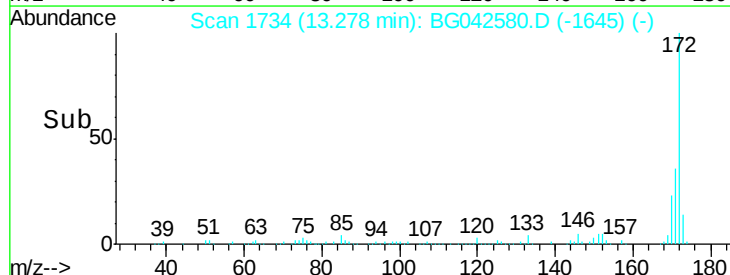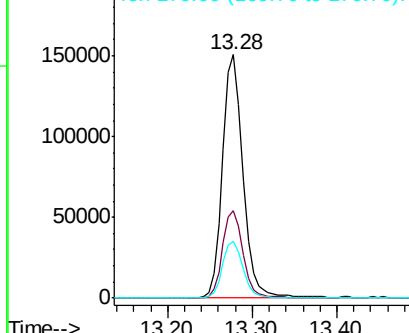



#50

Dimethylphthalate

Concen: 6.165 ng

RT: 14.11 min Scan# 1875

Delta R.T. -0.01 min

Lab File: BG042580.D

Acq: 30 Aug 2019 00:40





Instrument :

BNA_G

ClientSampleId :

S602-M-2.0-2.5-082319

Tgt Ion:	163	Resp:	44139
Ion	Ratio	Lower	Upper
163	100		
194	4.9	4.2	6.2
164	10.3	8.8	13.2

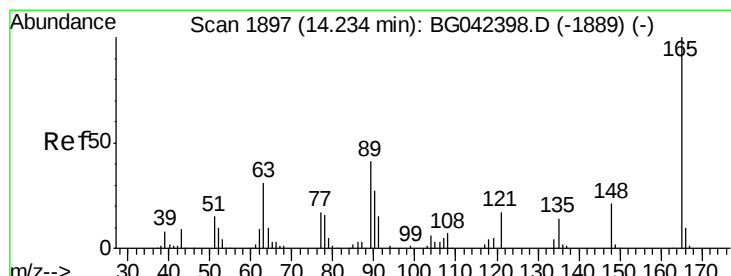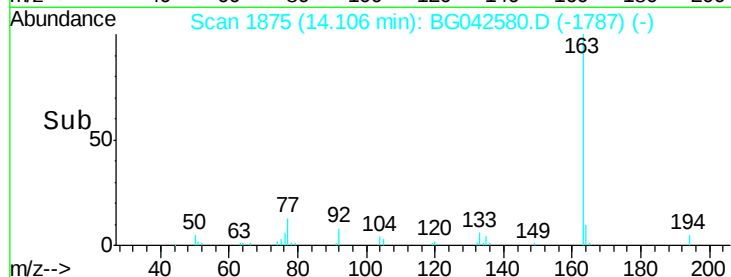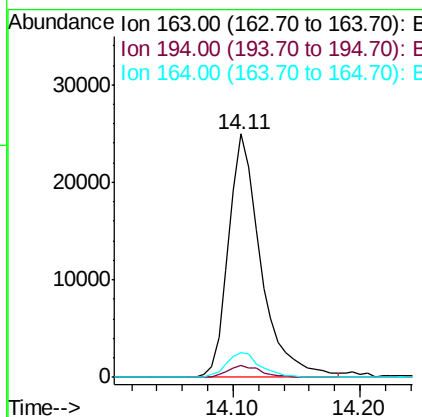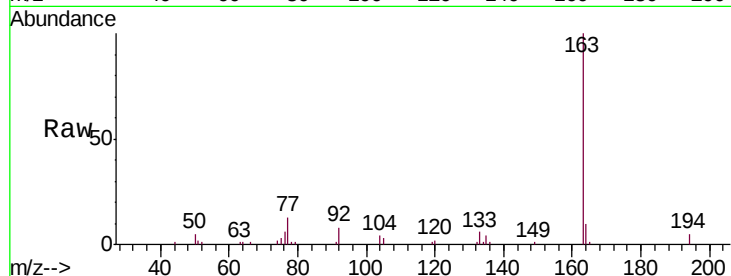

#51

2,6-Dinitrotoluene

Concen: 7.693 ng




RT: 14.65 min Scan# 1968


Delta R.T. 0.42 min

Lab File: BG042580.D

Acq: 30 Aug 2019 00:40

Tgt Ion:	165	Resp:	12766
Ion	Ratio	Lower	Upper
165	100		
63	0.0	30.6	45.8#
89	0.0	32.6	49.0#


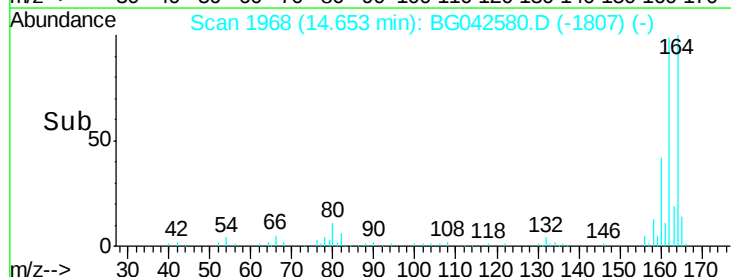
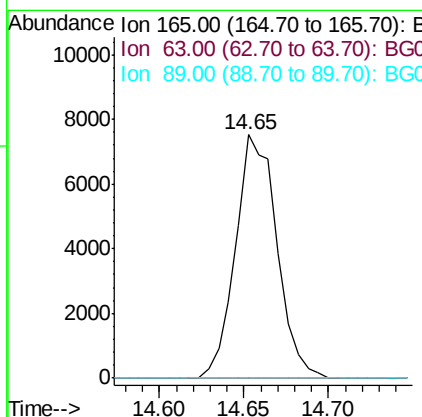
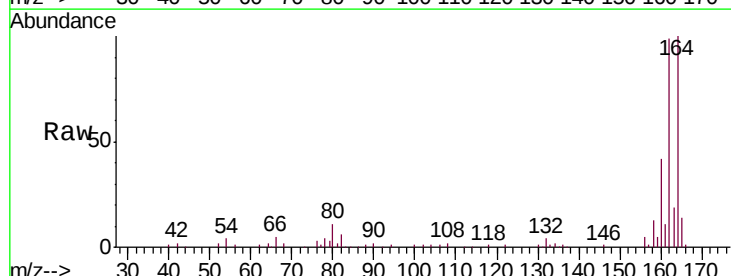


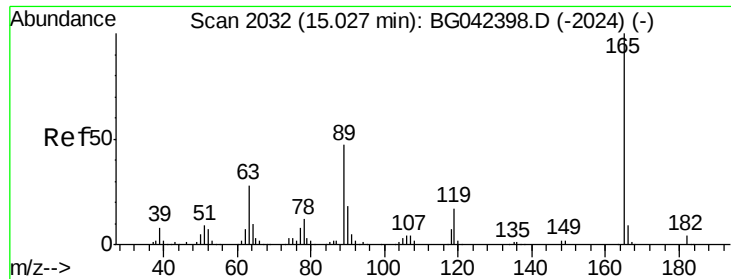

#57
 2,4-Dinitrotoluene
 Concen: 5.372 ng
 RT: 14.65 min Scan# 1968
 Delta R.T. -0.37 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40




Instrument :
 BNA_G
 ClientSampleId :
 S602-M-2.0-2.5-082319


Tgt Ion:	165	Resp:	12766
Ion	Ratio	Lower	Upper
165	100		
63	0.0	22.5	33.7#
89	0.0	37.8	56.6#
182	0.0	3.0	4.4#

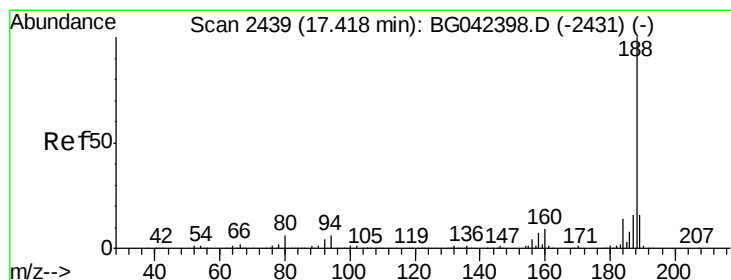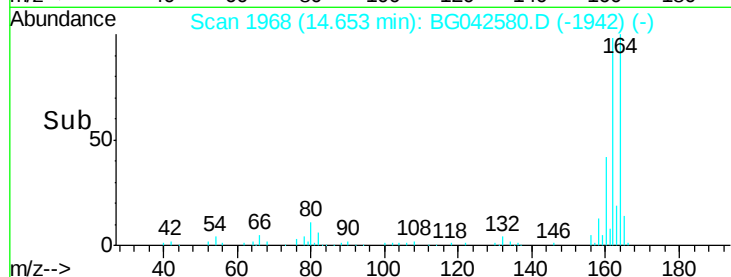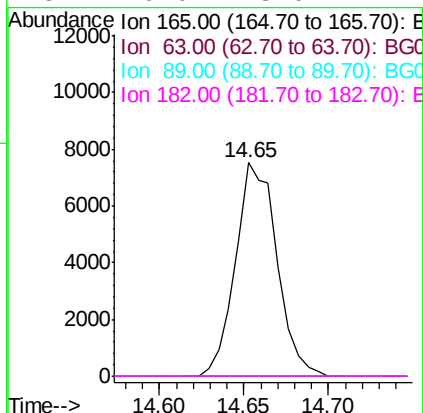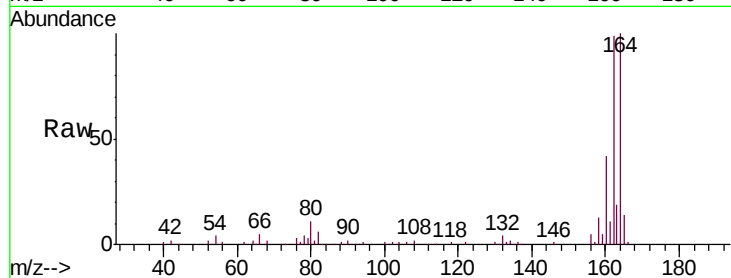

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.41 min Scan# 2437
 Delta R.T. -0.01 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Tgt Ion:	188	Resp:	233495
Ion	Ratio	Lower	Upper
188	100		
94	5.1	4.5	6.7
80	5.4	4.9	7.3

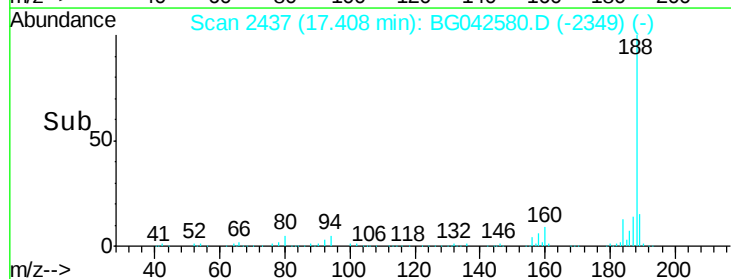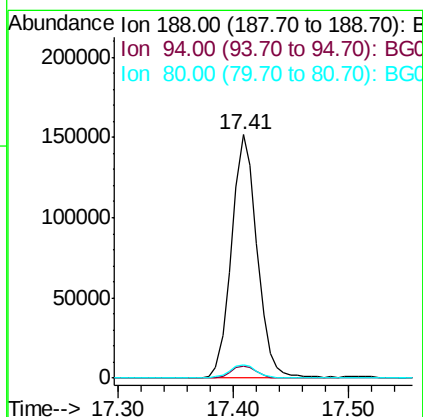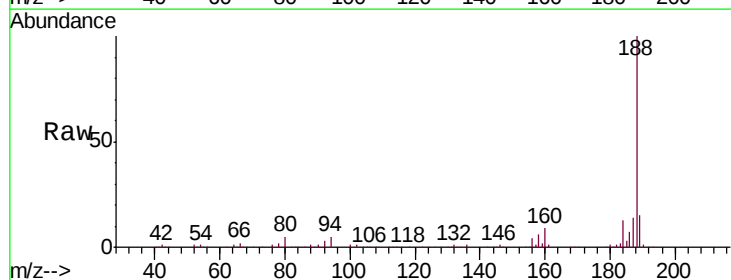


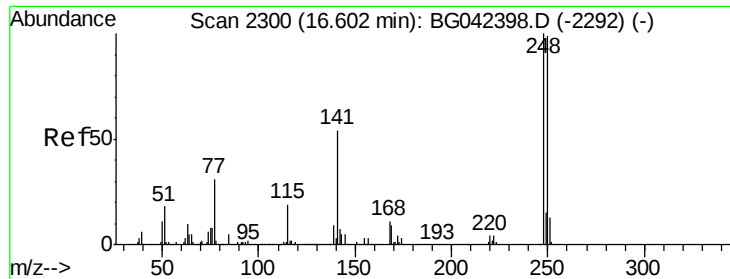




#67
 4-Bromophenyl-phenylether
 Concen: 2.394 ng
 RT: 16.15 min Scan# 2223
 Delta R.T. -0.45 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Instrument :
 BNA_G
 ClientSampleId :
 S602-M-2.0-2.5-082319

Tgt Ion: 248 Resp: 7089
 Ion Ratio Lower Upper
 248 100
 250 185.8 78.9 118.3#
 141 378.9 43.3 64.9#

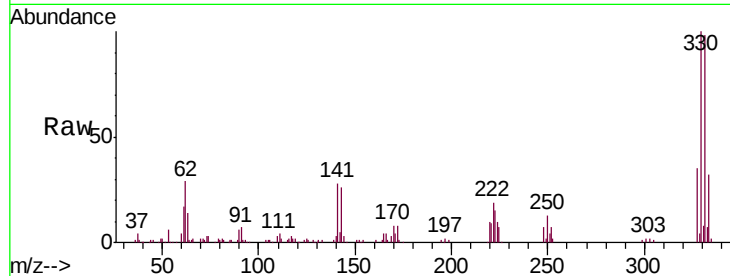


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

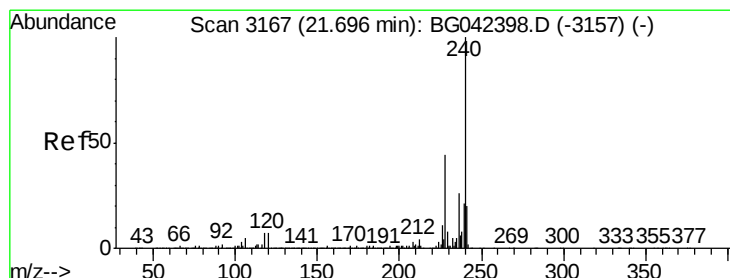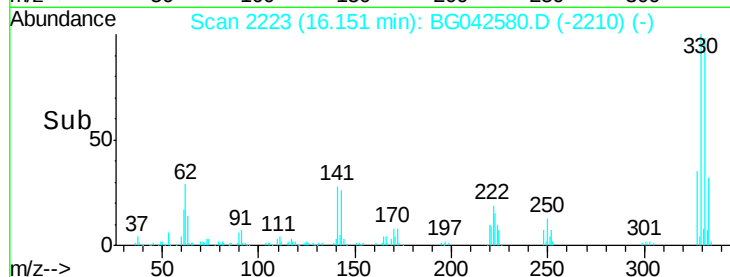
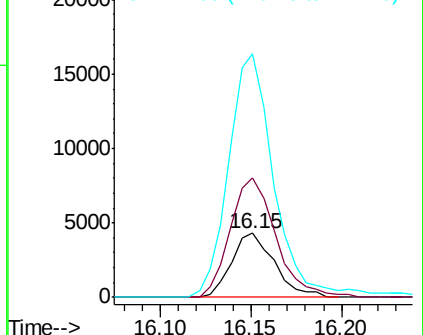



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.69 min Scan# 3165
 Delta R.T. -0.01 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Tgt Ion: 240 Resp: 248061
 Ion Ratio Lower Upper
 240 100
 120 5.9 5.7 8.5
 236 26.4 21.0 31.4

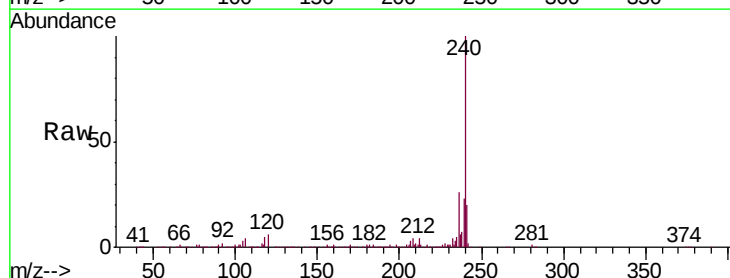

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



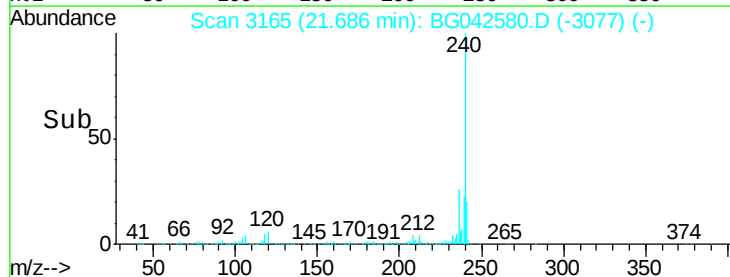
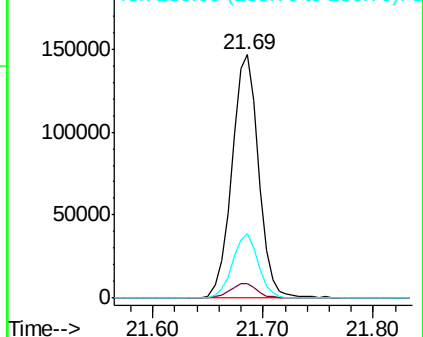


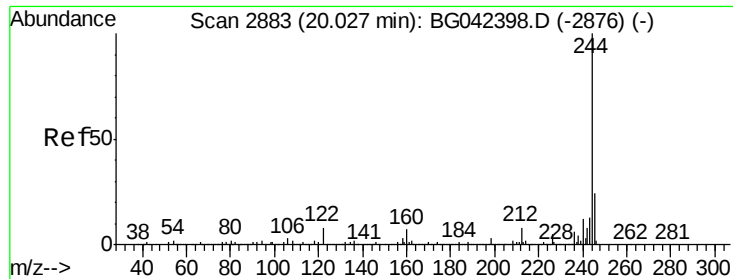

#79
 Terphenyl-d14
 Concen: 37.438 ng
 RT: 20.02 min Scan# 2881
 Delta R.T. -0.01 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Instrument :
 BNA_G
 ClientSampleId :
 S602-M-2.0-2.5-082319

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.5	6.0	9.0
122	7.0	6.7	10.1

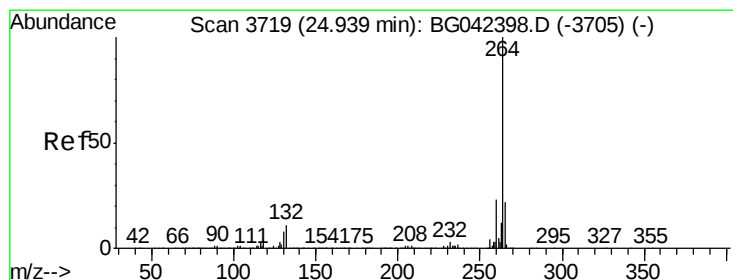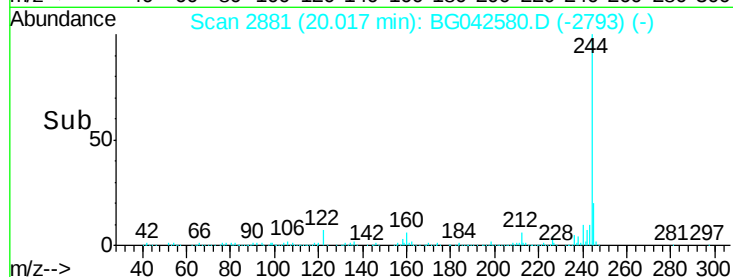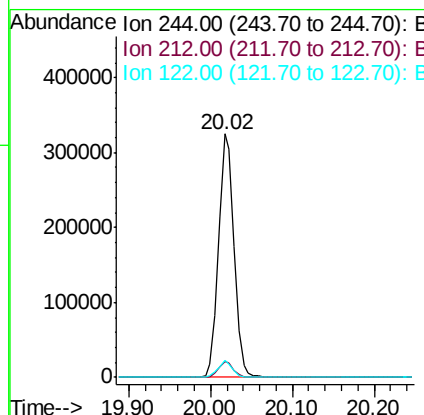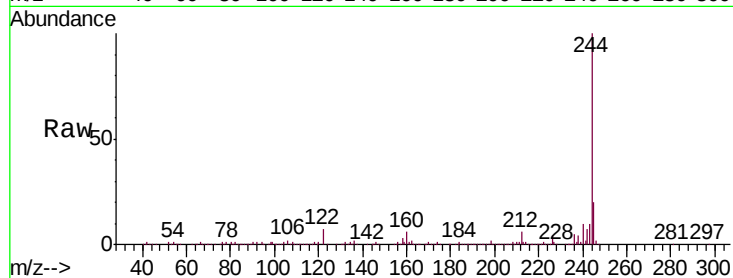

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.92 min Scan# 3716
 Delta R.T. -0.02 min
 Lab File: BG042580.D
 Acq: 30 Aug 2019 00:40

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.8	18.5	27.7
265	22.2	17.6	26.4

