
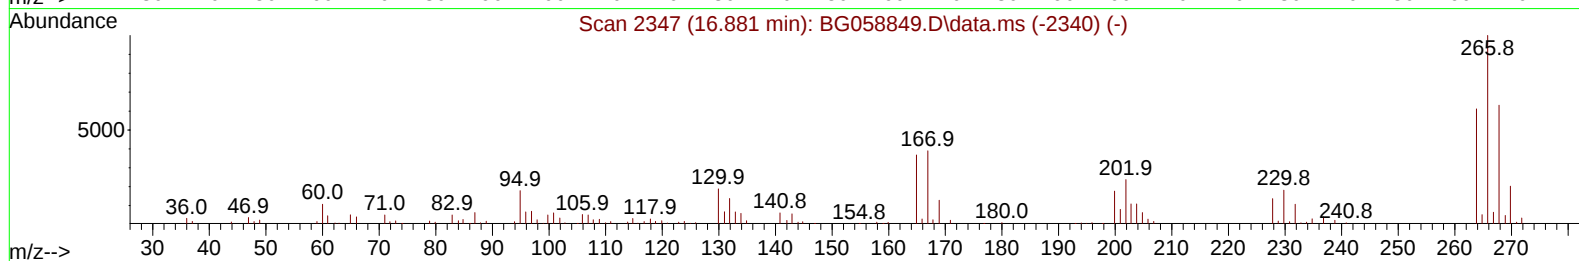
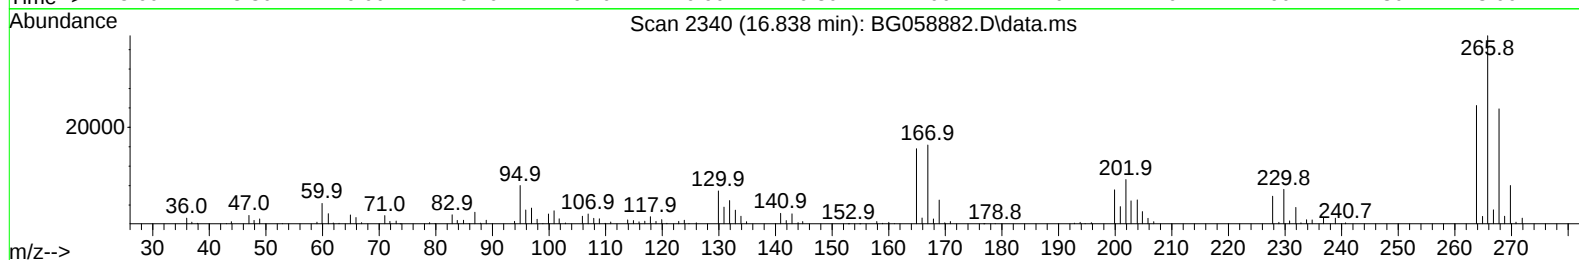


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082923\
Data File : BG058882.D
Acq On : 29 Aug 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 12:33:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

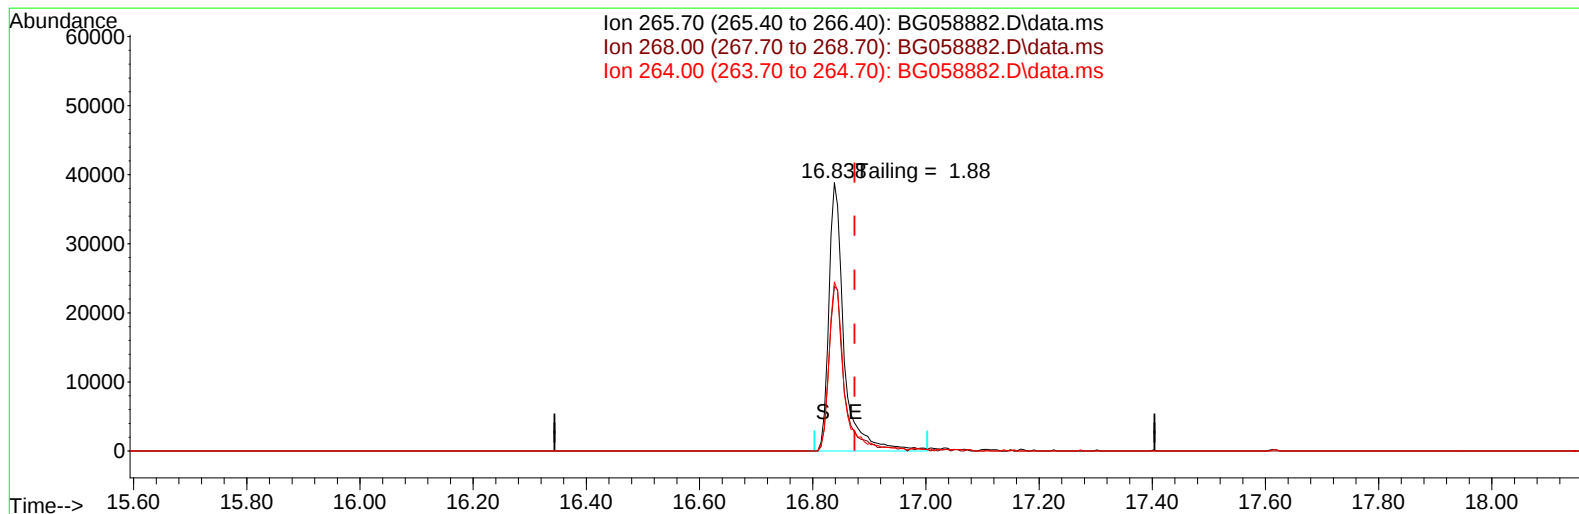

TIC: BG058882.D\data.ms

(70) Pentachlorophenol (C)




16.838min (-0.036) 34457.69 ng

response 72768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	61.27
264.00	61.90	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082923\
Data File : BG058882.D
Acq On : 29 Aug 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 12:33:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

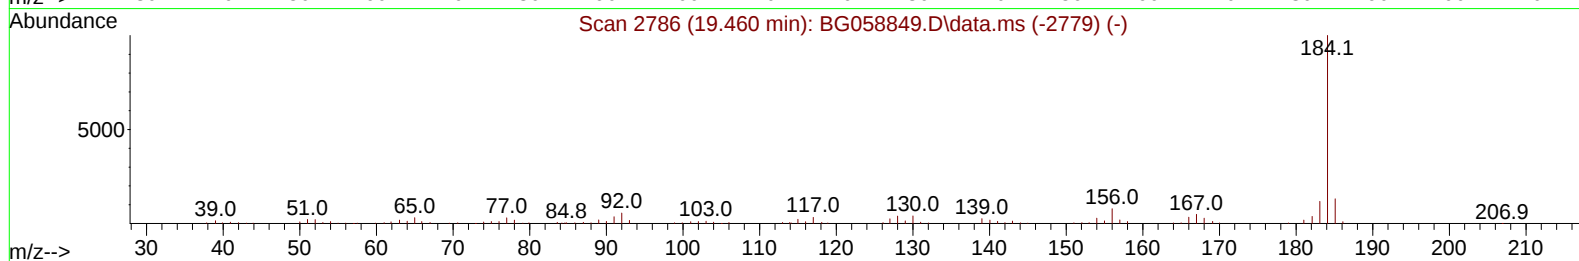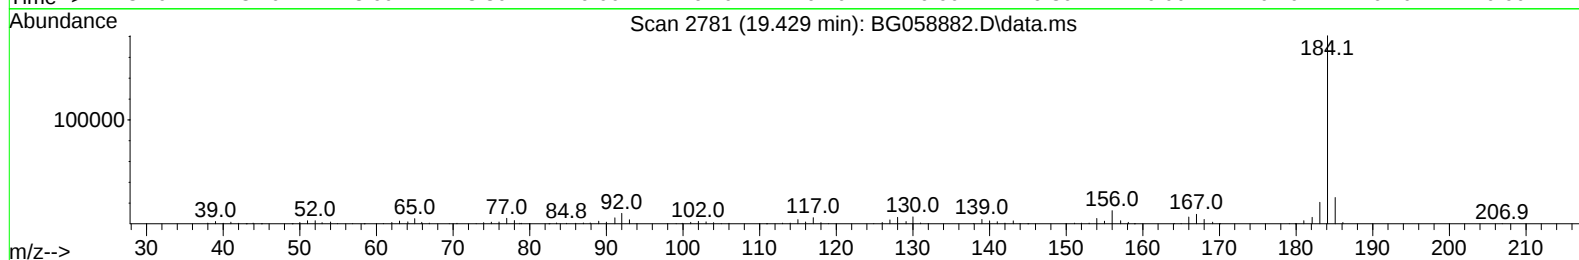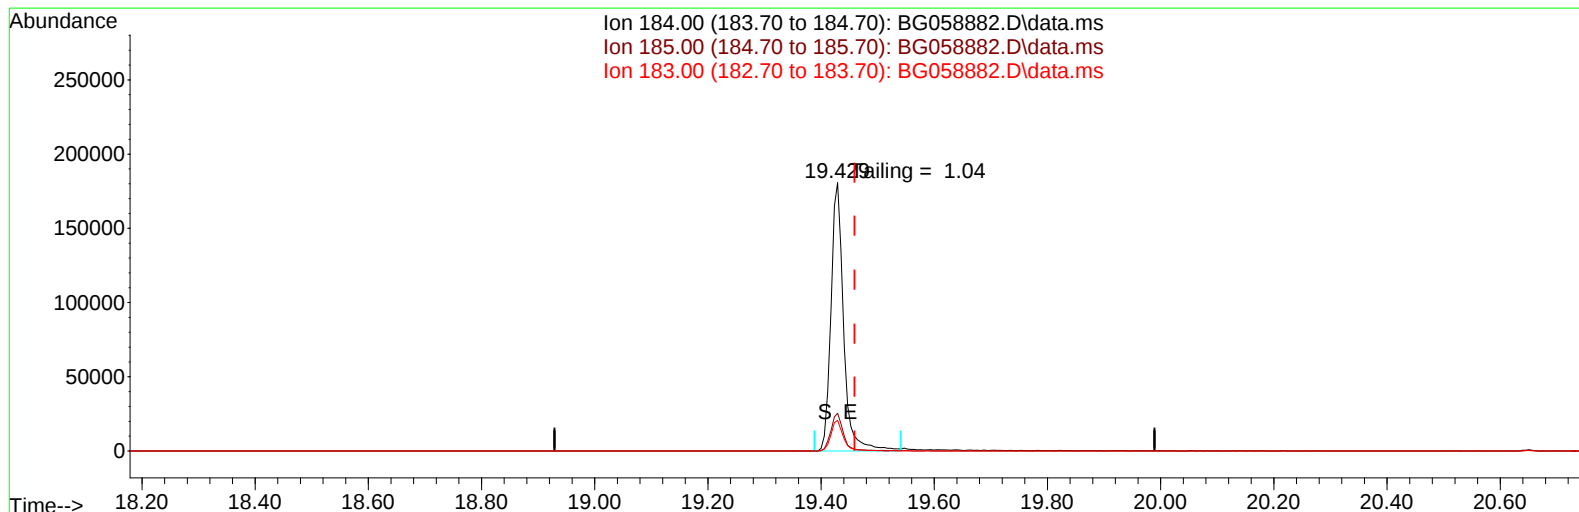

TIC: BG058882.D\data.ms

(77) Benzidine**19.429min (-0.030) 266653.21 ng****response 281957**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.06
183.00	12.50	11.46
0.00	0.00	0.00