
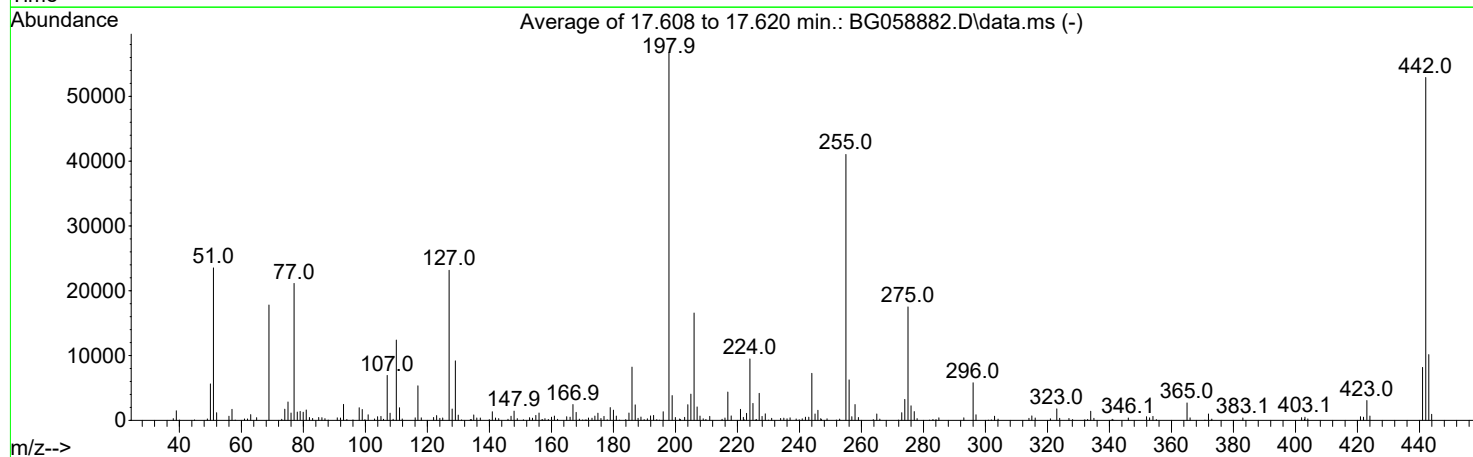


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082923\
 Data File : BG058882.D
 Acq On : 29 Aug 2023 10:56
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 29 14:27:28 2023

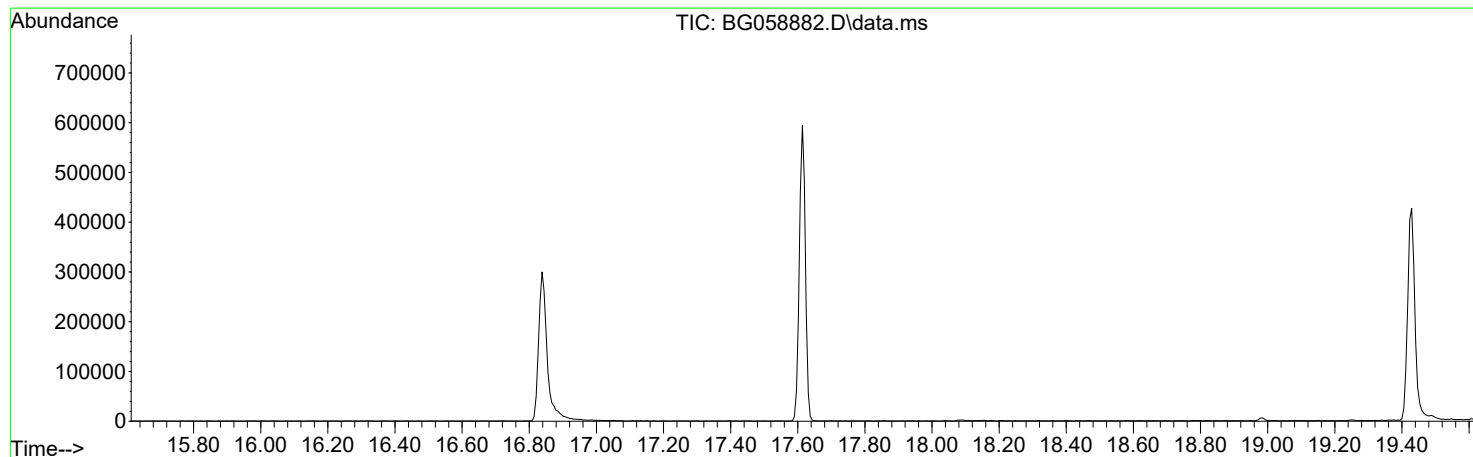




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	23523	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	17797	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	23165	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56763	PASS
199	198	5	9	6.7	3817	PASS
275	198	10	60	30.8	17506	PASS
365	198	1	100	4.7	2687	PASS
441	198	0.01	100	14.4	8176	PASS
442	442	50	100	100.0	52901	PASS
443	442	15	24	19.2	10153	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082923\
Data File : BG058882.D
Acq On : 29 Aug 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 29 12:33:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

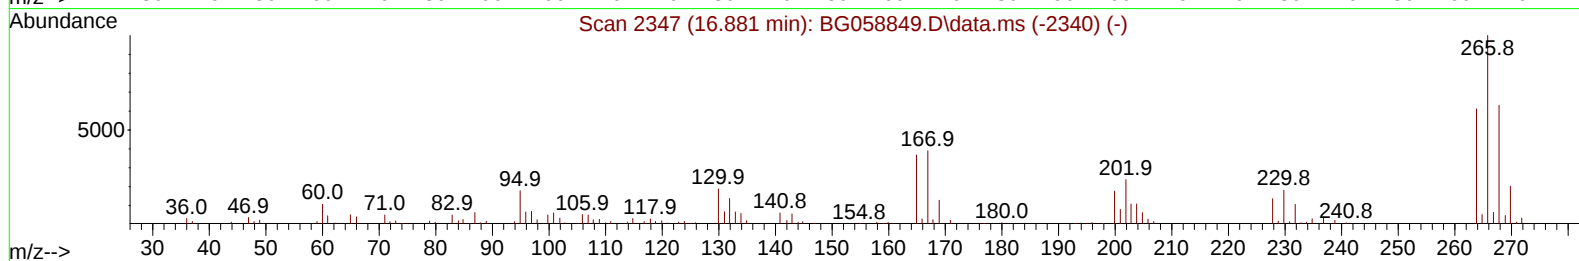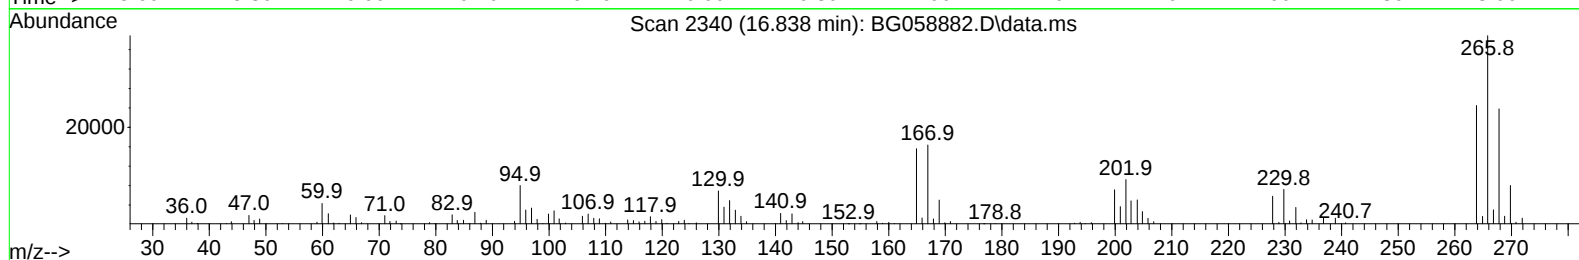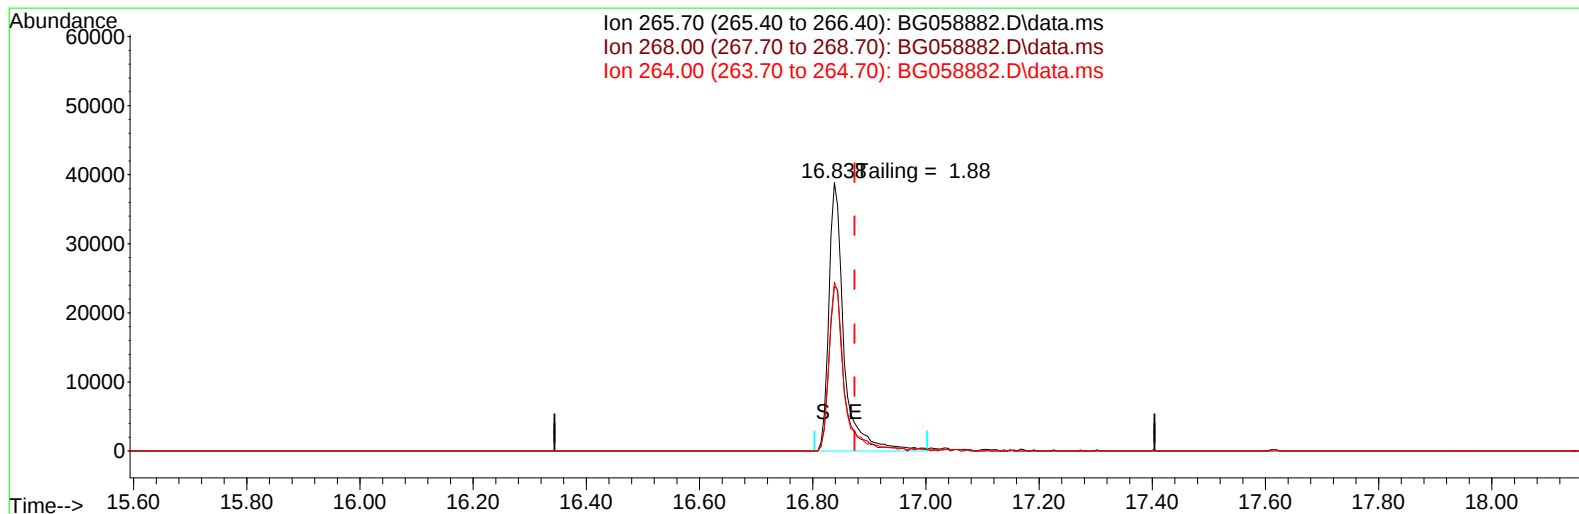

TIC: BG058882.D\data.ms

(70) Pentachlorophenol (C)

16.838min (-0.036) 34457.69 ng




response 72768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	61.27
264.00	61.90	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082923\
Data File : BG058882.D
Acq On : 29 Aug 2023 10:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 29 12:33:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 01:35:28 2023
Response via : Initial Calibration

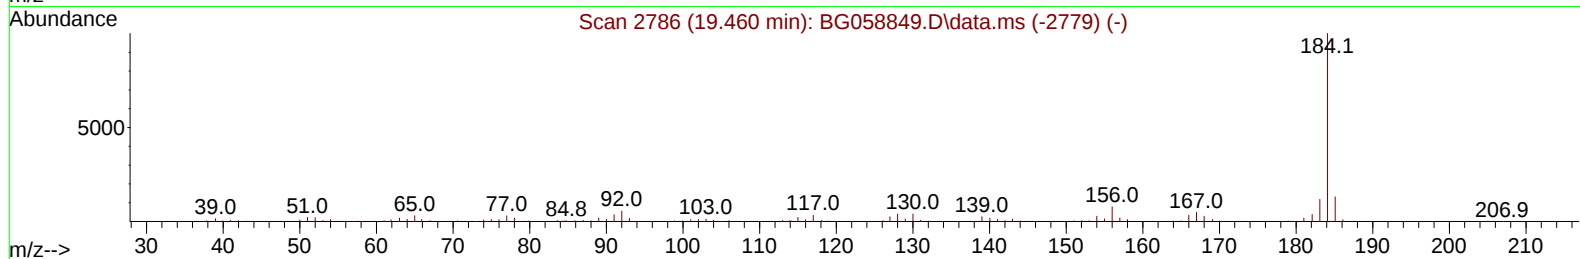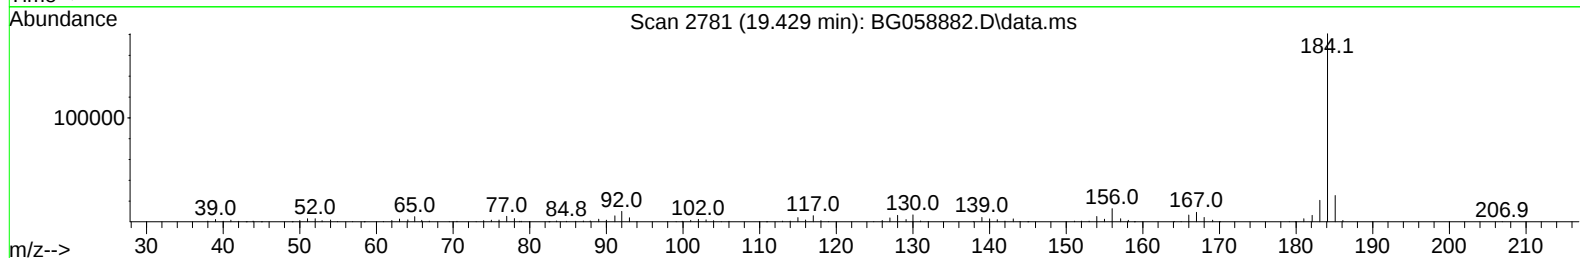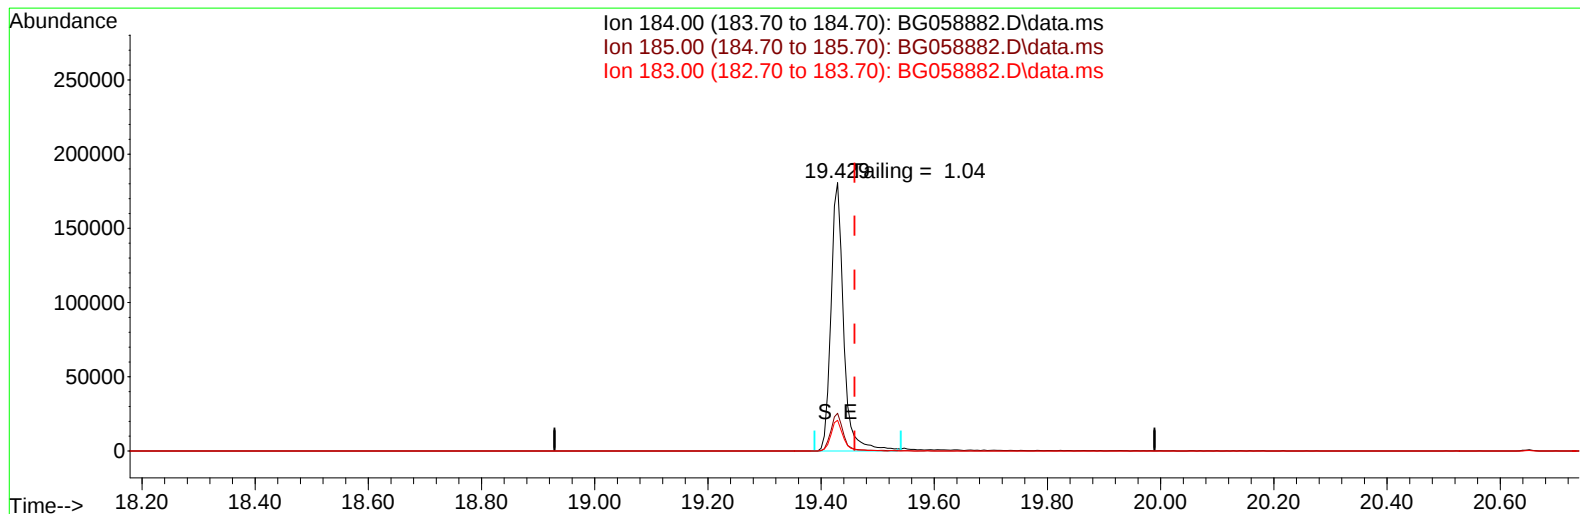

TIC: BG058882.D\data.ms

(77) Benzidine

19.429min (-0.030) 266653.21 ng

response 281957

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.06
183.00	12.50	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2023	BNA_G	BG058882.D
Compound Name	Response	Retention Time
DDT	190858	20.651
DDD	3021	20.264
DDE	0	19.744
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3021	193879	1.56

Instrument :
BNA_G
ClientSampleId :
DFTPP