
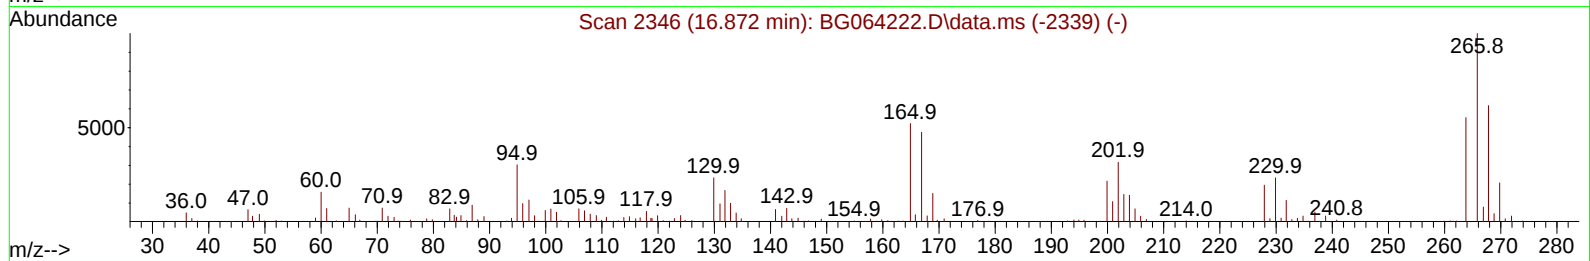
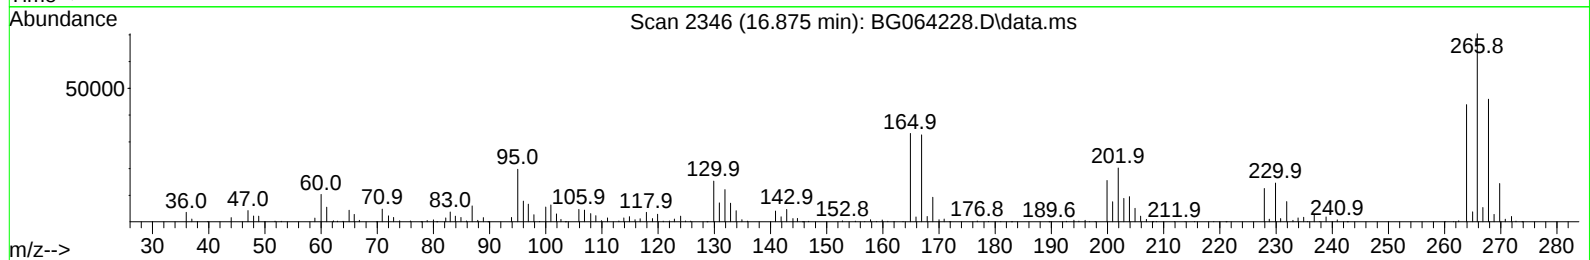


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082925\
Data File : BG064228.D
Acq On : 29 Aug 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 15:18:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

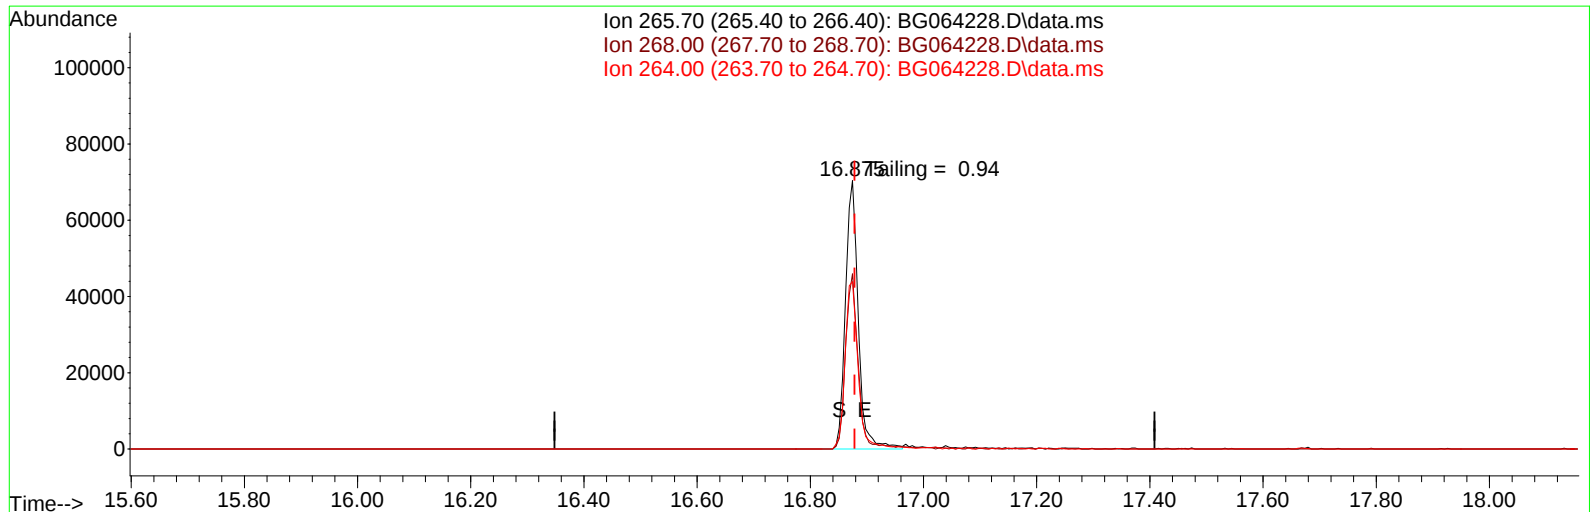

TIC: BG064228.D\data.ms

(70) Pentachlorophenol (C)




16.875min (-0.003) 97482.03 ng

response 110848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.28
264.00	55.40	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082925\
Data File : BG064228.D
Acq On : 29 Aug 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 15:18:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

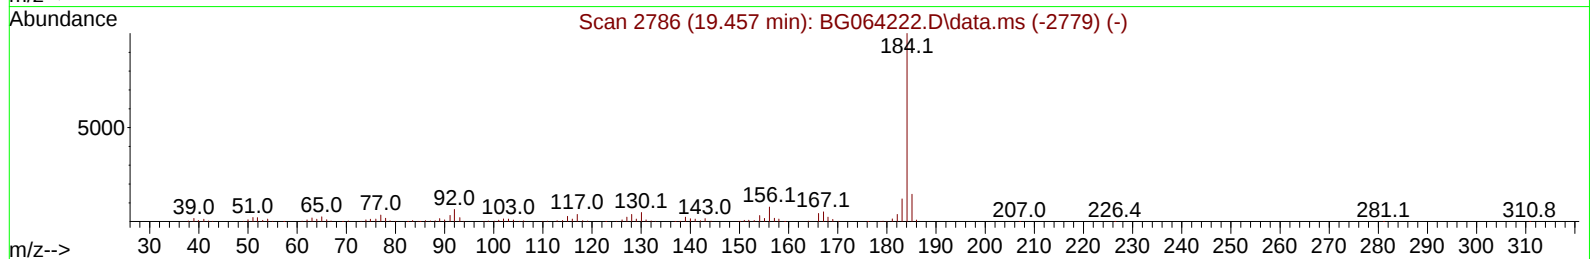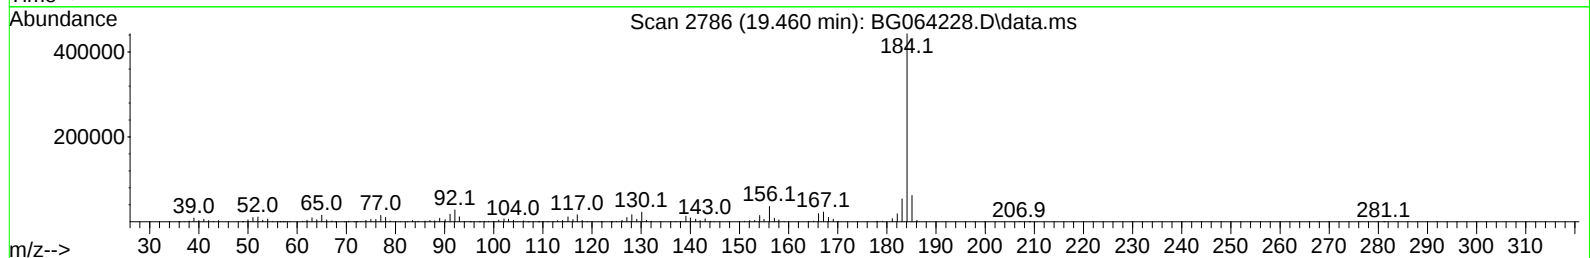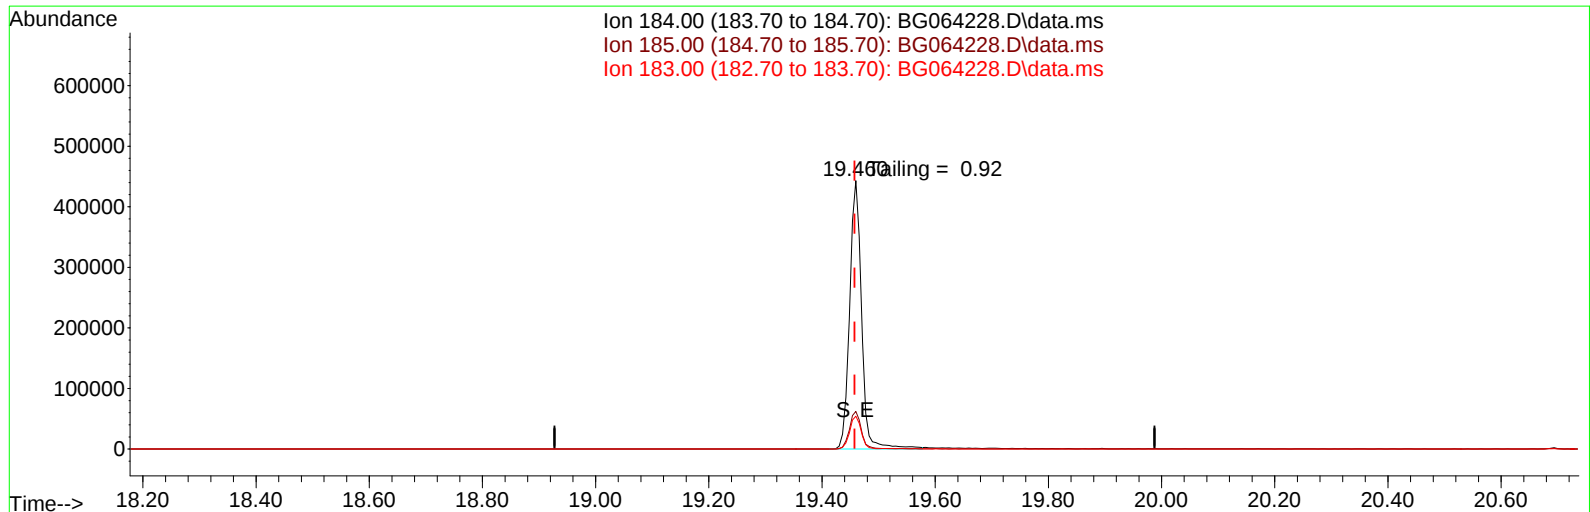

TIC: BG064228.D\data.ms

(77) Benzidine**19.460min (+ 0.002) 517458.75 ng****response 653131**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.03
183.00	12.10	12.21
0.00	0.00	0.00